

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034574.D
 Acq On : 13 Mar 2024 14:53
 Operator : SY/MD
 Sample : P1739-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034574.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	124775	134675	12.19%	1.505%
2	1.529	146	152	166	rVB	125334	146196	13.24%	1.633%
3	2.060	307	317	332	rBV	232252	339273	30.72%	3.791%
4	2.439	432	435	448	rBV6	1221	1889	0.17%	0.021%
5	2.561	465	473	479	rBV4	976	1419	0.13%	0.016%
6	2.635	492	496	501	rVB3	341	398	0.04%	0.004%
7	2.703	514	517	519	rBV2	331	163	0.01%	0.002%
8	2.793	543	545	547	rBV	124	70	0.01%	0.001%
9	3.114	641	645	647	rBV2	356	280	0.03%	0.003%
10	3.253	685	688	691	rBV2	98	71	0.01%	0.001%
11	3.269	691	693	699	rVB	164	124	0.01%	0.001%
12	3.420	737	740	744	rVB2	229	151	0.01%	0.002%
13	3.439	745	746	750	rBV2	181	144	0.01%	0.002%
14	3.487	758	761	764	rBV2	127	104	0.01%	0.001%
15	3.519	769	771	774	rBV2	188	114	0.01%	0.001%
16	3.584	788	791	794	rBV2	91	80	0.01%	0.001%
17	3.683	815	822	824	rBV2	187	213	0.02%	0.002%
18	3.786	846	854	895	rBV	116741	342159	30.98%	3.823%
19	4.249	982	998	1027	rBV	185330	470712	42.62%	5.259%
20	4.577	1098	1100	1102	rBV2	376	234	0.02%	0.003%
21	4.658	1123	1125	1132	rVB3	386	282	0.03%	0.003%
22	4.761	1155	1157	1160	rVB2	285	165	0.01%	0.002%
23	4.777	1160	1162	1165	rVB	178	111	0.01%	0.001%
24	4.809	1169	1172	1174	rBV2	210	127	0.01%	0.001%
25	4.876	1190	1193	1195	rVB2	383	189	0.02%	0.002%
26	4.953	1201	1217	1249	rBV2	414973	1104382	100.00%	12.339%
27	5.227	1300	1302	1304	rBV	327	150	0.01%	0.002%
28	5.330	1332	1334	1338	rBV	230	213	0.02%	0.002%
29	5.423	1361	1363	1366	rVB2	275	143	0.01%	0.002%
30	5.458	1369	1374	1376	rBV	415	258	0.02%	0.003%
31	5.471	1376	1378	1383	rVB3	390	272	0.02%	0.003%
32	5.532	1383	1397	1434	rBV	350471	732869	66.36%	8.188%
33	5.773	1470	1472	1474	rBV2	346	124	0.01%	0.001%
34	5.838	1479	1492	1518	rVV2	54648	127084	11.51%	1.420%
35	5.989	1526	1539	1571	rBV	248867	518572	46.96%	5.794%
36	6.259	1621	1623	1627	rBV	159	131	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031324\
 Data File : VW034574.D
 Acq On : 13 Mar 2024 14:53
 Operator : SY/MD
 Sample : P1739-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.291	1630	1633	1636	rVB	433	228	0.02%	0.003%
38	6.368	1653	1657	1660	rBV2	130	117	0.01%	0.001%
39	6.439	1676	1679	1681	rBV2	146	75	0.01%	0.001%
40	6.461	1684	1686	1688	rBV2	150	89	0.01%	0.001%
41	6.587	1719	1725	1728	rBV4	827	1021	0.09%	0.011%
42	6.699	1757	1760	1764	rVB3	314	211	0.02%	0.002%
43	6.777	1782	1784	1787	rBV2	325	135	0.01%	0.002%
44	6.793	1787	1789	1791	rBV2	195	83	0.01%	0.001%
45	6.828	1797	1800	1805	rVB2	154	87	0.01%	0.001%
46	6.867	1809	1812	1816	rBV2	150	116	0.01%	0.001%
47	6.912	1817	1826	1857	rBV	122278	236573	21.42%	2.643%
48	7.243	1917	1929	1955	rBV	444136	785467	71.12%	8.776%
49	7.555	2016	2026	2050	rBV	84596	158257	14.33%	1.768%
50	7.728	2079	2080	2084	rBV3	248	139	0.01%	0.002%
51	7.764	2089	2091	2093	rBV2	423	206	0.02%	0.002%
52	7.854	2116	2119	2121	rBV2	565	363	0.03%	0.004%
53	7.937	2142	2145	2148	rVB2	197	117	0.01%	0.001%
54	7.973	2152	2156	2158	rBV	275	212	0.02%	0.002%
55	8.024	2162	2172	2217	rBV	402897	757963	68.63%	8.469%
56	8.667	2369	2372	2375	rBV2	285	218	0.02%	0.002%
57	8.783	2395	2408	2442	rBV	519764	868956	78.68%	9.709%
58	9.101	2504	2507	2509	rVB	170	102	0.01%	0.001%
59	9.117	2509	2512	2514	rVB2	237	135	0.01%	0.002%
60	9.140	2514	2519	2521	rBV	375	197	0.02%	0.002%
61	9.175	2529	2530	2535	rVB	215	113	0.01%	0.001%
62	9.201	2535	2538	2540	rBV2	147	105	0.01%	0.001%
63	9.297	2566	2568	2571	rBV2	167	121	0.01%	0.001%
64	9.371	2590	2591	2594	rVB	220	73	0.01%	0.001%
65	9.391	2594	2597	2599	rBV2	197	117	0.01%	0.001%
66	9.439	2610	2612	2615	rBV	216	137	0.01%	0.002%
67	9.493	2621	2629	2632	rBV2	441	482	0.04%	0.005%
68	9.513	2632	2635	2638	rVV	249	164	0.01%	0.002%
69	9.551	2644	2647	2649	rVV2	192	130	0.01%	0.001%
70	9.580	2653	2656	2660	rVB2	207	152	0.01%	0.002%
71	9.654	2676	2679	2681	rBV	328	139	0.01%	0.002%
72	9.699	2691	2693	2696	rVB	261	94	0.01%	0.001%
73	9.751	2704	2709	2711	rBV2	155	130	0.01%	0.001%
74	9.783	2716	2719	2724	rBV2	165	146	0.01%	0.002%
75	10.149	2819	2833	2861	rBV	372801	596451	54.01%	6.664%
76	10.545	2952	2956	2959	rBV2	327	298	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034574.D
 Acq On : 13 Mar 2024 14:53
 Operator : SY/MD
 Sample : P1739-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.651	2986	2989	2991	rBV2	131	90	0.01%	0.001%
78	10.715	3006	3009	3011	rBV	177	131	0.01%	0.001%
79	10.744	3016	3018	3022	rVB	233	126	0.01%	0.001%
80	10.767	3022	3025	3026	rBV	254	155	0.01%	0.002%
81	11.034	3106	3108	3112	rVB	349	209	0.02%	0.002%
82	11.133	3136	3139	3143	rBV3	355	270	0.02%	0.003%
83	11.185	3143	3155	3182	rBV	532697	829584	75.12%	9.269%
84	11.439	3232	3234	3237	rBV	139	81	0.01%	0.001%
85	11.497	3250	3252	3257	rVB2	253	152	0.01%	0.002%
86	11.558	3260	3271	3303	rBV	489288	781607	70.77%	8.733%
87	11.992	3404	3406	3407	rBV	239	92	0.01%	0.001%
88	12.429	3539	3542	3543	rBV	290	154	0.01%	0.002%
89	12.725	3630	3634	3638	rBV	300	252	0.02%	0.003%
90	12.828	3663	3666	3669	rBV	279	170	0.02%	0.002%
91	13.075	3740	3743	3745	rBV2	290	209	0.02%	0.002%
92	13.136	3760	3762	3764	rBV2	261	125	0.01%	0.001%
93	13.162	3767	3770	3773	rBV2	266	211	0.02%	0.002%
94	13.207	3781	3784	3790	rBV3	710	799	0.07%	0.009%
95	13.413	3844	3848	3850	rBV2	548	447	0.04%	0.005%
96	13.670	3923	3928	3929	rBV3	380	252	0.02%	0.003%
97	13.686	3929	3933	3937	rVV4	839	792	0.07%	0.009%
98	13.792	3963	3966	3968	rBV2	275	199	0.02%	0.002%
99	14.040	4040	4043	4046	rBV2	349	304	0.03%	0.003%
100	14.275	4113	4116	4118	rBV4	587	393	0.04%	0.004%




Sum of corrected areas: 8950264

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034574.D
Acq On : 13 Mar 2024 14:53
Operator : SY/MD
Sample : P1739-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

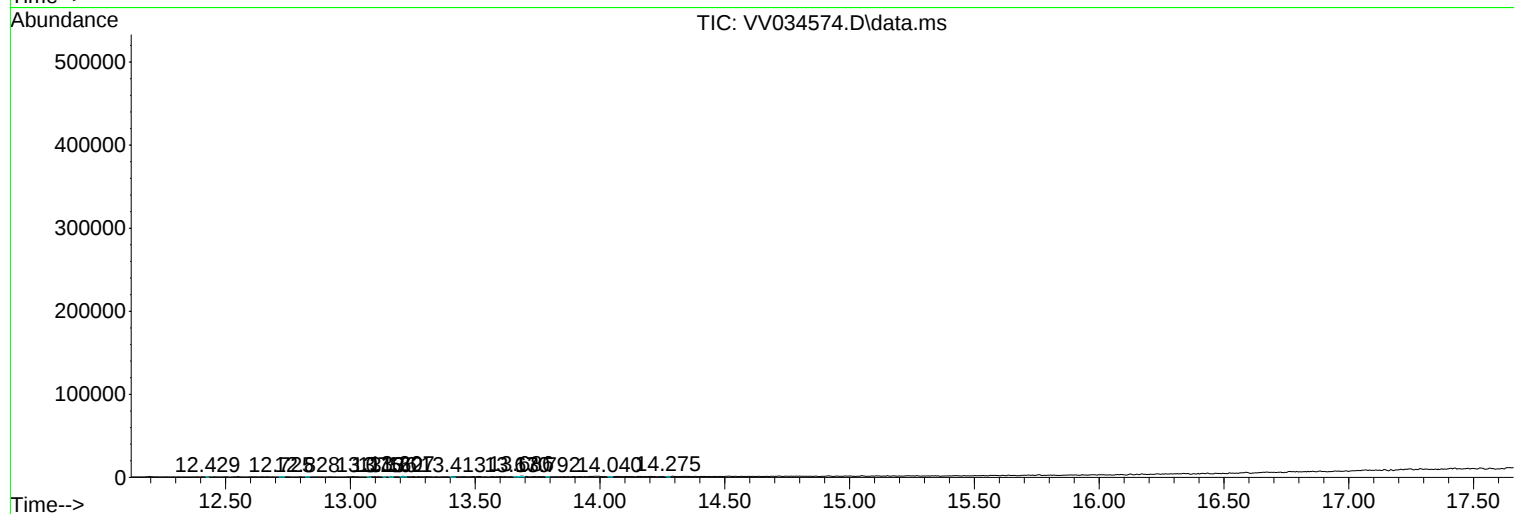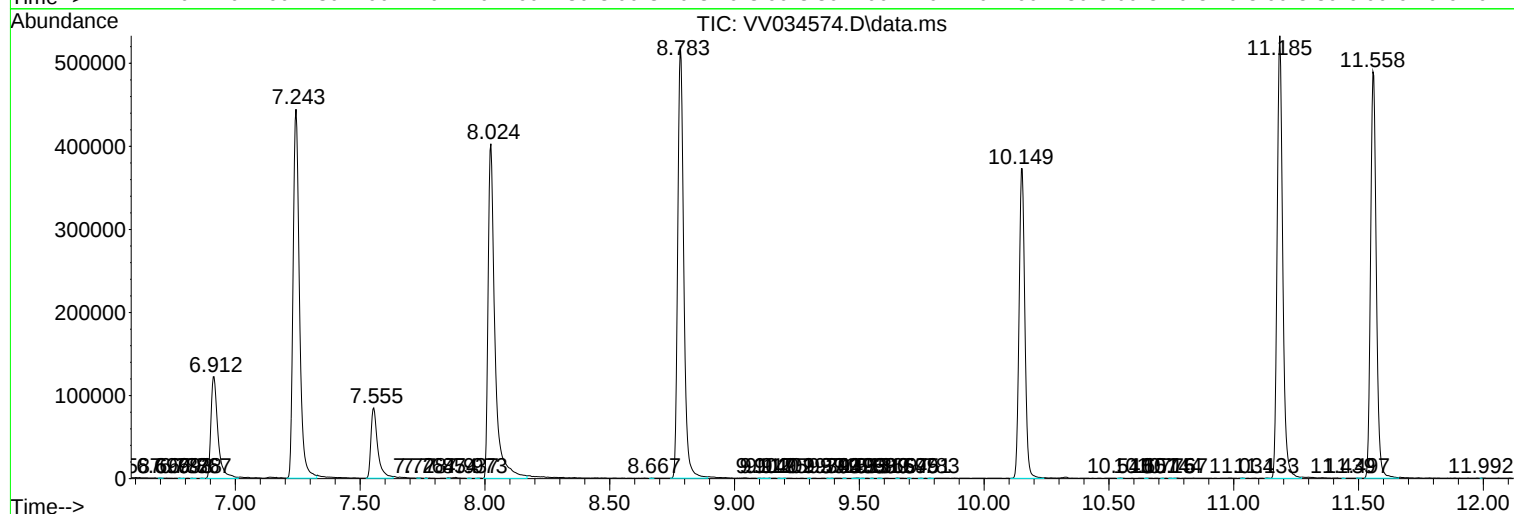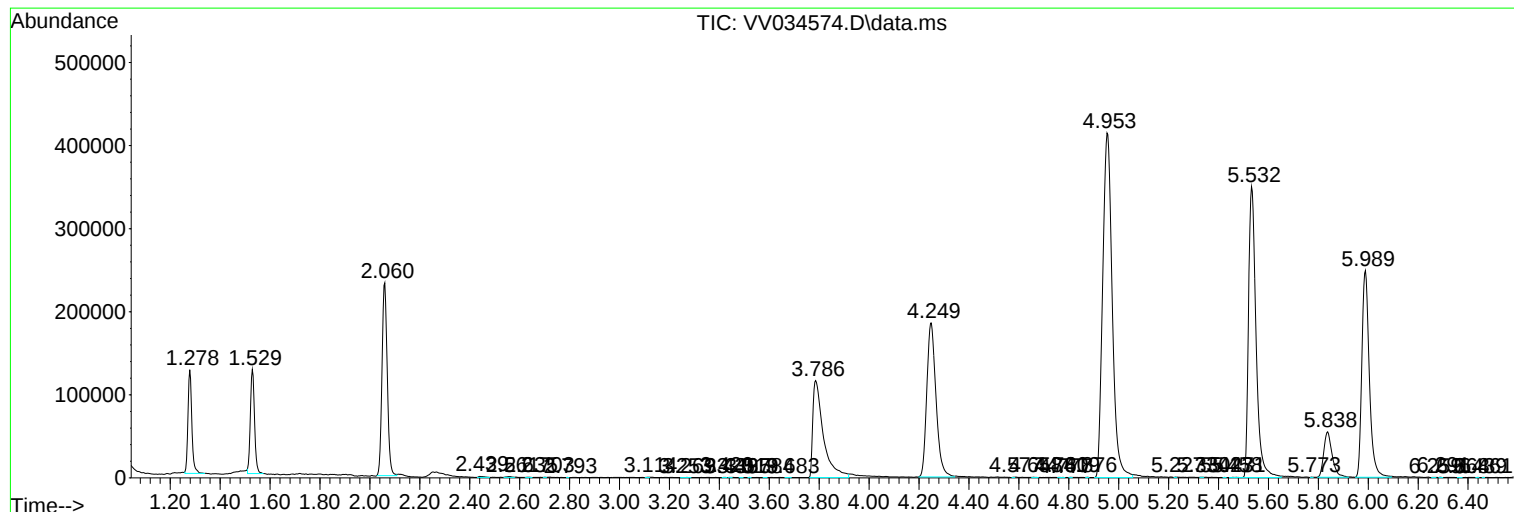

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034574.D
Acq On : 13 Mar 2024 14:53
Operator : SY/MD
Sample : P1739-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034574.D
Acq On : 13 Mar 2024 14:53
Operator : SY/MD
Sample : P1739-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------