

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034575.D
 Acq On : 13 Mar 2024 15:16
 Operator : SY/MD
 Sample : P1739-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034575.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	124885	133487	11.94%	1.493%
2	1.532	146	153	169	rVB	126342	146197	13.08%	1.635%
3	2.060	306	317	335	rBV	228205	339347	30.35%	3.794%
4	2.291	372	389	391	rBV3	4916	10654	0.95%	0.119%
5	2.446	432	437	438	rBV3	1301	934	0.08%	0.010%
6	2.536	461	465	466	rBV2	383	275	0.02%	0.003%
7	3.111	641	644	647	rBV2	217	181	0.02%	0.002%
8	3.127	647	649	653	rVV	293	178	0.02%	0.002%
9	3.616	797	801	804	rVV	242	196	0.02%	0.002%
10	3.793	847	856	903	rBV	116531	362769	32.45%	4.056%
11	4.182	972	977	981	rBV3	461	559	0.05%	0.006%
12	4.249	981	998	1035	rVV	186788	480943	43.02%	5.377%
13	4.494	1072	1074	1079	rVB2	342	267	0.02%	0.003%
14	4.953	1201	1217	1257	rBV2	415662	1118055	100.00%	12.501%
15	5.179	1286	1287	1290	rVB2	613	217	0.02%	0.002%
16	5.204	1293	1295	1299	rVB2	474	221	0.02%	0.002%
17	5.259	1309	1312	1314	rBV2	367	222	0.02%	0.002%
18	5.378	1346	1349	1354	rVV3	372	280	0.03%	0.003%
19	5.407	1354	1358	1361	rBV2	246	231	0.02%	0.003%
20	5.445	1366	1370	1375	rVB3	382	336	0.03%	0.004%
21	5.532	1386	1397	1425	rBV	351565	731652	65.44%	8.181%
22	5.834	1480	1491	1512	rVB6	12490	30981	2.77%	0.346%
23	5.908	1512	1514	1516	rBV2	575	285	0.03%	0.003%
24	5.989	1526	1539	1563	rBV	252580	524696	46.93%	5.867%
25	6.140	1581	1586	1589	rBV4	839	635	0.06%	0.007%
26	6.236	1614	1616	1622	rVV3	238	211	0.02%	0.002%
27	6.269	1624	1626	1630	rVB3	324	236	0.02%	0.003%
28	6.294	1630	1634	1638	rBV2	408	244	0.02%	0.003%
29	6.333	1642	1646	1649	rVB2	382	234	0.02%	0.003%
30	6.587	1720	1725	1727	rBV3	919	950	0.08%	0.011%
31	6.912	1812	1826	1854	rBV	122856	240404	21.50%	2.688%
32	7.124	1888	1892	1893	rBV2	467	292	0.03%	0.003%
33	7.143	1893	1898	1900	rBV2	692	678	0.06%	0.008%
34	7.243	1918	1929	1954	rBV	440725	782200	69.96%	8.746%
35	7.555	2016	2026	2056	rVV	83680	158044	14.14%	1.767%
36	7.831	2108	2112	2114	rBV	269	198	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031324\
 Data File : VW034575.D
 Acq On : 13 Mar 2024 15:16
 Operator : SY/MD
 Sample : P1739-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	7.873	2116	2125	2140	rVB3	1570	2654	0.24%	0.030%
38	8.024	2162	2172	2219	rBV	394633	765380	68.46%	8.558%
39	8.275	2248	2250	2257	rVB4	513	428	0.04%	0.005%
40	8.558	2336	2338	2345	rVB4	491	339	0.03%	0.004%
41	8.590	2345	2348	2353	rBV2	372	410	0.04%	0.005%
42	8.641	2362	2364	2369	rBV3	261	201	0.02%	0.002%
43	8.783	2397	2408	2438	rBV	522687	868809	77.71%	9.714%
44	8.950	2458	2460	2462	rBV2	329	184	0.02%	0.002%
45	9.034	2481	2486	2488	rVB2	336	219	0.02%	0.002%
46	9.053	2488	2492	2495	rBV2	320	233	0.02%	0.003%
47	9.088	2501	2503	2508	rVB2	311	215	0.02%	0.002%
48	9.143	2515	2520	2524	rVB2	304	321	0.03%	0.004%
49	9.162	2524	2526	2529	rBV	470	290	0.03%	0.003%
50	9.243	2548	2551	2556	rVB2	320	207	0.02%	0.002%
51	9.603	2659	2663	2669	rVB2	331	285	0.03%	0.003%
52	9.696	2689	2692	2701	rVB2	204	255	0.02%	0.003%
53	9.770	2711	2715	2717	rVV2	190	178	0.02%	0.002%
54	9.876	2743	2748	2754	rVB3	473	482	0.04%	0.005%
55	9.905	2754	2757	2761	rBV	382	343	0.03%	0.004%
56	9.963	2770	2775	2780	rBV	147	185	0.02%	0.002%
57	9.998	2781	2786	2791	rVB2	212	239	0.02%	0.003%
58	10.149	2822	2833	2858	rBV	379325	597588	53.45%	6.682%
59	10.297	2876	2879	2880	rBV	426	244	0.02%	0.003%
60	10.323	2881	2887	2900	rVB7	1587	2782	0.25%	0.031%
61	10.439	2919	2923	2928	rVB2	243	228	0.02%	0.003%
62	10.513	2943	2946	2950	rVB2	261	211	0.02%	0.002%
63	10.583	2962	2968	2971	rBV	168	189	0.02%	0.002%
64	10.686	2994	3000	3003	rBV2	236	218	0.02%	0.002%
65	10.879	3056	3060	3063	rBV2	270	257	0.02%	0.003%
66	11.185	3144	3155	3177	rBV	524753	831981	74.41%	9.302%
67	11.333	3198	3201	3205	rVB2	568	392	0.04%	0.004%
68	11.374	3213	3214	3218	rVB2	493	236	0.02%	0.003%
69	11.397	3218	3221	3222	rBV	359	176	0.02%	0.002%
70	11.558	3260	3271	3294	rBV	496737	790301	70.69%	8.836%
71	11.690	3310	3312	3317	rVB2	610	558	0.05%	0.006%
72	11.841	3355	3359	3364	rVV	314	303	0.03%	0.003%
73	11.892	3372	3375	3378	rBV	220	177	0.02%	0.002%
74	12.194	3466	3469	3472	rBV3	339	275	0.02%	0.003%
75	12.329	3506	3511	3512	rBV	314	227	0.02%	0.003%
76	12.407	3533	3535	3539	rVB	496	210	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034575.D
 Acq On : 13 Mar 2024 15:16
 Operator : SY/MD
 Sample : P1739-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	12.432	3539	3543	3545	rBV2	352	270	0.02%	0.003%
78	12.892	3683	3686	3691	rVB	428	331	0.03%	0.004%
79	13.143	3760	3764	3766	rBV3	302	229	0.02%	0.003%
80	13.207	3782	3784	3787	rBV2	373	243	0.02%	0.003%
81	13.271	3802	3804	3806	rBV	341	217	0.02%	0.002%
82	13.284	3806	3808	3811	rVB	434	227	0.02%	0.003%
83	13.535	3882	3886	3887	rBV	294	196	0.02%	0.002%
84	13.686	3930	3933	3934	rBV2	476	326	0.03%	0.004%
85	13.767	3952	3958	3961	rBV3	437	465	0.04%	0.005%
86	13.805	3966	3970	3973	rBV2	346	321	0.03%	0.004%
87	13.902	3997	4000	4003	rBV	212	188	0.02%	0.002%
88	13.979	4020	4024	4028	rBV	665	692	0.06%	0.008%
89	14.030	4037	4040	4042	rBV	310	200	0.02%	0.002%
90	14.287	4117	4120	4123	rBV2	598	378	0.03%	0.004%
91	14.368	4143	4145	4149	rBV2	324	193	0.02%	0.002%
92	14.423	4160	4162	4167	rBV2	277	221	0.02%	0.002%
93	14.480	4177	4180	4183	rBV2	430	293	0.03%	0.003%
94	14.561	4202	4205	4208	rBV2	591	467	0.04%	0.005%
95	14.599	4215	4217	4221	rBV2	287	183	0.02%	0.002%
96	14.931	4318	4320	4323	rBV3	533	348	0.03%	0.004%
97	15.262	4421	4423	4426	rVB2	734	388	0.03%	0.004%
98	15.291	4426	4432	4434	rBV3	693	799	0.07%	0.009%
99	15.410	4467	4469	4471	rBV2	580	270	0.02%	0.003%
100	15.471	4486	4488	4491	rBV2	589	332	0.03%	0.004%




Sum of corrected areas: 8943676

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034575.D
Acq On : 13 Mar 2024 15:16
Operator : SY/MD
Sample : P1739-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

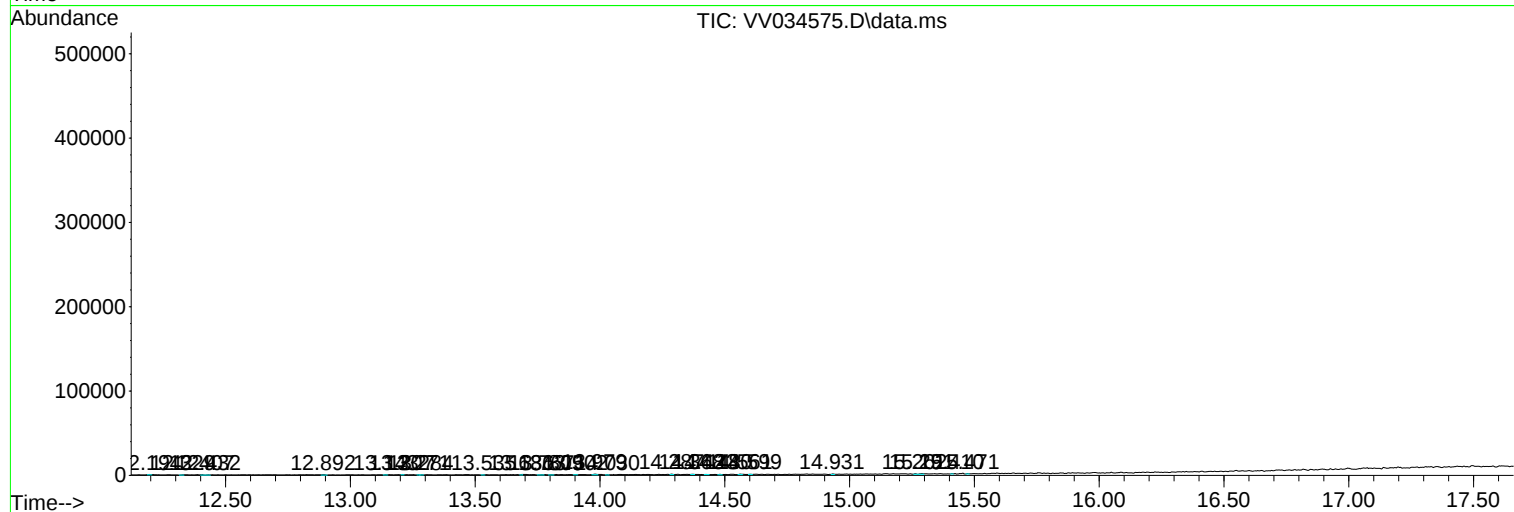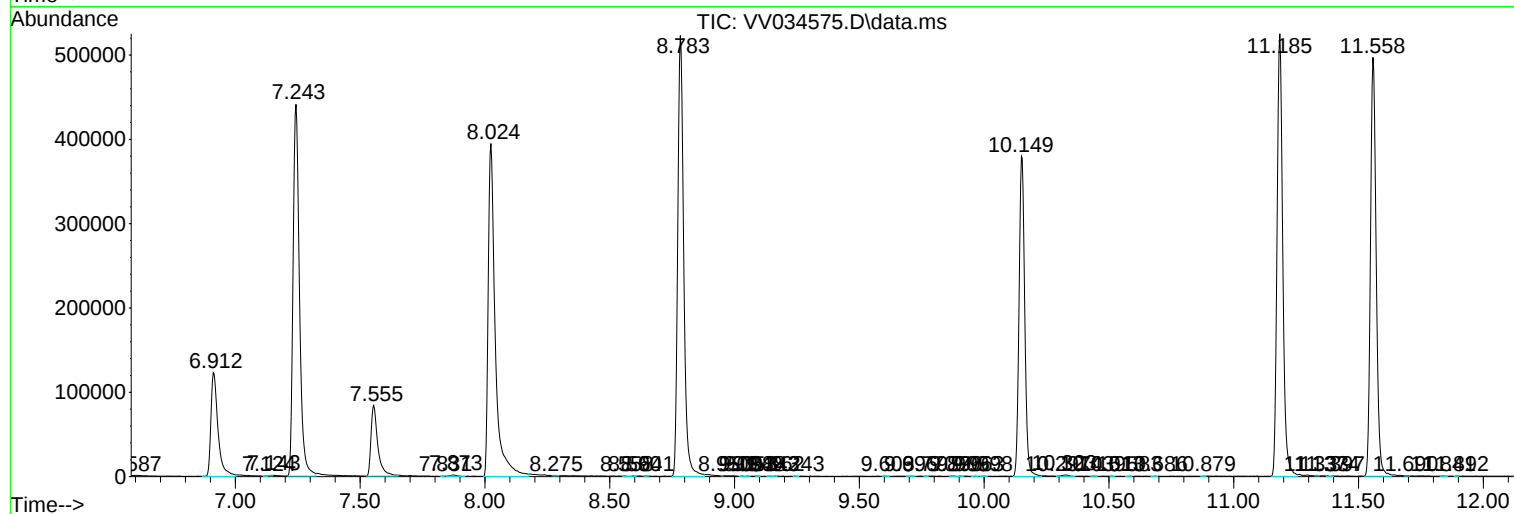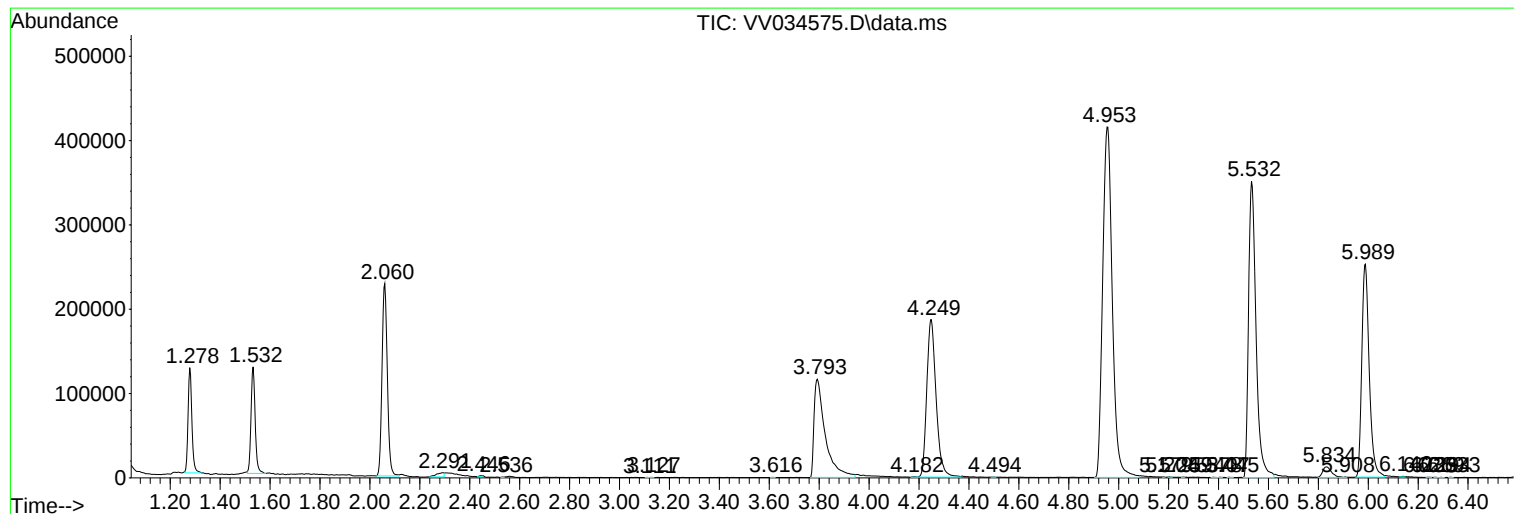

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034575.D
Acq On : 13 Mar 2024 15:16
Operator : SY/MD
Sample : P1739-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034575.D
Acq On : 13 Mar 2024 15:16
Operator : SY/MD
Sample : P1739-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
