

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034576.D
 Acq On : 13 Mar 2024 15:40
 Operator : SY/MD
 Sample : P1739-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034576.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	130819	137895	11.73%	1.480%
2	1.532	146	153	163	rBV	129786	146742	12.48%	1.575%
3	2.060	307	317	331	rBV	240007	350865	29.84%	3.765%
4	2.687	509	512	514	rBV2	302	181	0.02%	0.002%
5	2.760	531	535	538	rBV2	227	167	0.01%	0.002%
6	2.886	571	574	576	rBV2	147	93	0.01%	0.001%
7	2.979	601	603	606	rBV	112	80	0.01%	0.001%
8	3.018	613	615	616	rBV	144	57	0.00%	0.001%
9	3.066	628	630	636	rVB	241	133	0.01%	0.001%
10	3.108	640	643	646	rBV	237	173	0.01%	0.002%
11	3.162	658	660	662	rBV	163	54	0.00%	0.001%
12	3.217	671	677	680	rBV2	235	251	0.02%	0.003%
13	3.288	698	699	700	rBV	158	36	0.00%	0.000%
14	3.391	728	731	733	rBV	147	80	0.01%	0.001%
15	3.426	736	742	746	rBV2	194	218	0.02%	0.002%
16	3.532	770	775	776	rBV	212	173	0.01%	0.002%
17	3.564	783	785	786	rBV	113	47	0.00%	0.001%
18	3.638	804	808	810	rBV	192	128	0.01%	0.001%
19	3.693	822	825	827	rBV	174	101	0.01%	0.001%
20	3.709	827	830	835	rVB2	275	221	0.02%	0.002%
21	3.735	836	838	840	rBV	169	61	0.01%	0.001%
22	3.757	843	845	847	rBV2	127	72	0.01%	0.001%
23	3.789	847	855	891	rBV	122740	360710	30.67%	3.871%
24	4.246	982	997	1030	rBV	202007	512981	43.62%	5.505%
25	4.590	1102	1104	1106	rBV2	358	188	0.02%	0.002%
26	4.690	1131	1135	1136	rBV2	283	195	0.02%	0.002%
27	4.770	1155	1160	1164	rBV2	312	360	0.03%	0.004%
28	4.953	1201	1217	1254	rBV2	439793	1175929	100.00%	12.620%
29	5.346	1337	1339	1344	rVB2	533	338	0.03%	0.004%
30	5.368	1344	1346	1349	rBV	220	131	0.01%	0.001%
31	5.397	1352	1355	1356	rBV	114	52	0.00%	0.001%
32	5.410	1357	1359	1362	rVV2	230	91	0.01%	0.001%
33	5.439	1366	1368	1369	rBV2	265	93	0.01%	0.001%
34	5.458	1373	1374	1375	rBV	204	51	0.00%	0.001%
35	5.477	1376	1380	1381	rBV	197	121	0.01%	0.001%
36	5.532	1386	1397	1435	rBV	350673	725921	61.73%	7.790%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034576.D
 Acq On : 13 Mar 2024 15:40
 Operator : SY/MD
 Sample : P1739-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.831	1479	1490	1515	rVB7	16946	44287	3.77%	0.475%
38	5.989	1526	1539	1568	rBV2	266851	557336	47.40%	5.981%
39	6.230	1610	1614	1617	rBV2	328	303	0.03%	0.003%
40	6.259	1620	1623	1624	rBV	223	132	0.01%	0.001%
41	6.378	1655	1660	1663	rBV2	215	188	0.02%	0.002%
42	6.403	1663	1668	1669	rBV	254	170	0.01%	0.002%
43	6.452	1679	1683	1686	rBV	253	194	0.02%	0.002%
44	6.526	1704	1706	1707	rBV	149	41	0.00%	0.000%
45	6.571	1718	1720	1721	rBV	253	124	0.01%	0.001%
46	6.728	1767	1769	1771	rBV2	251	131	0.01%	0.001%
47	6.911	1814	1826	1863	rBV	132421	257874	21.93%	2.767%
48	7.140	1888	1897	1898	rBV3	1159	1347	0.11%	0.014%
49	7.191	1911	1913	1914	rBV	315	173	0.01%	0.002%
50	7.243	1918	1929	1962	rVV	473882	840040	71.44%	9.015%
51	7.555	2016	2026	2051	rBV	93218	171008	14.54%	1.835%
52	7.786	2097	2098	2107	rVB2	409	345	0.03%	0.004%
53	7.825	2107	2110	2111	rBV	172	73	0.01%	0.001%
54	7.834	2111	2113	2115	rBV	160	63	0.01%	0.001%
55	7.873	2117	2125	2126	rBV3	1198	1298	0.11%	0.014%
56	7.927	2137	2142	2144	rBV	180	150	0.01%	0.002%
57	7.956	2150	2151	2152	rBV	142	44	0.00%	0.000%
58	8.024	2163	2172	2220	rBV	434931	828962	70.49%	8.896%
59	8.423	2294	2296	2301	rBV3	450	353	0.03%	0.004%
60	8.493	2313	2318	2325	rBV4	500	534	0.05%	0.006%
61	8.571	2340	2342	2350	rVB2	361	278	0.02%	0.003%
62	8.606	2350	2353	2356	rBV3	441	267	0.02%	0.003%
63	8.673	2371	2374	2378	rBV3	295	221	0.02%	0.002%
64	8.696	2378	2381	2387	rBV2	387	463	0.04%	0.005%
65	8.783	2397	2408	2432	rBV	528778	863908	73.47%	9.271%
66	9.011	2477	2479	2483	rVB2	343	229	0.02%	0.002%
67	9.030	2483	2485	2487	rBV2	116	45	0.00%	0.000%
68	9.046	2487	2490	2494	rBV2	218	179	0.02%	0.002%
69	9.130	2514	2516	2517	rBV2	120	54	0.00%	0.001%
70	9.207	2536	2540	2542	rBV2	353	200	0.02%	0.002%
71	9.220	2542	2544	2548	rVB	259	124	0.01%	0.001%
72	9.316	2573	2574	2576	rVB	345	107	0.01%	0.001%
73	9.342	2580	2582	2586	rVB2	536	258	0.02%	0.003%
74	9.362	2586	2588	2589	rBV	183	78	0.01%	0.001%
75	9.487	2622	2627	2629	rBV	201	154	0.01%	0.002%
76	9.571	2646	2653	2656	rBV2	255	344	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034576.D
 Acq On : 13 Mar 2024 15:40
 Operator : SY/MD
 Sample : P1739-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	9.625	2668	2670	2672	rBV	237	103	0.01%	0.001%
78	9.638	2672	2674	2675	rBV	304	99	0.01%	0.001%
79	9.773	2713	2716	2720	rVB2	281	158	0.01%	0.002%
80	9.792	2720	2722	2725	rBV	150	63	0.01%	0.001%
81	9.825	2728	2732	2733	rBV2	198	122	0.01%	0.001%
82	9.866	2742	2745	2747	rBV	279	152	0.01%	0.002%
83	10.001	2786	2787	2788	rBV	145	36	0.00%	0.000%
84	10.152	2822	2834	2853	rBV	410700	646076	54.94%	6.933%
85	10.442	2919	2924	2927	rBV	265	292	0.02%	0.003%
86	10.484	2934	2937	2944	rVB3	386	332	0.03%	0.004%
87	10.641	2984	2986	2989	rBV	265	143	0.01%	0.002%
88	10.738	3011	3016	3020	rBV2	253	224	0.02%	0.002%
89	11.066	3115	3118	3129	rVB2	309	372	0.03%	0.004%
90	11.185	3144	3155	3181	rBV	515613	828731	70.47%	8.894%
91	11.419	3226	3228	3233	rBV2	189	127	0.01%	0.001%
92	11.474	3242	3245	3249	rVB2	278	233	0.02%	0.003%
93	11.558	3260	3271	3298	rBV	541332	851876	72.44%	9.142%
94	12.059	3423	3427	3429	rBV2	363	289	0.02%	0.003%
95	12.107	3439	3442	3446	rBV2	248	219	0.02%	0.002%
96	12.529	3565	3573	3577	rBV2	369	513	0.04%	0.006%
97	12.953	3701	3705	3710	rBV2	319	336	0.03%	0.004%
98	13.371	3832	3835	3837	rBV	345	172	0.01%	0.002%
99	13.789	3963	3965	3966	rBV	323	128	0.01%	0.001%
100	14.593	4213	4215	4218	rBV	745	364	0.03%	0.004%




Sum of corrected areas: 9318228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034576.D
Acq On : 13 Mar 2024 15:40
Operator : SY/MD
Sample : P1739-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

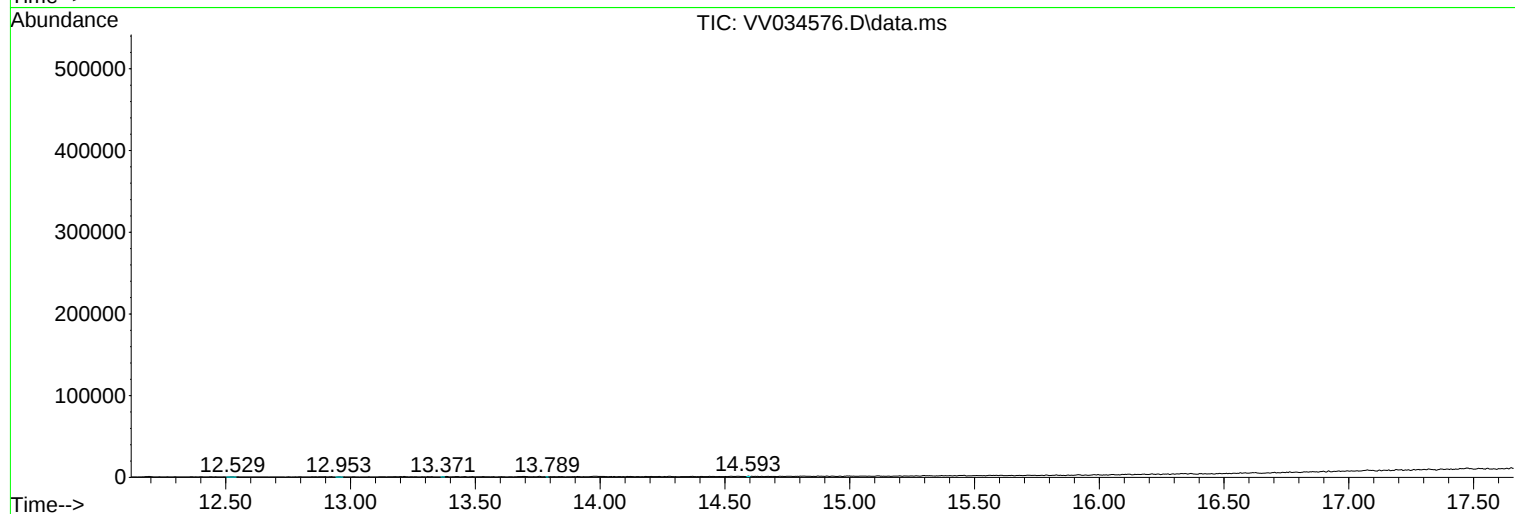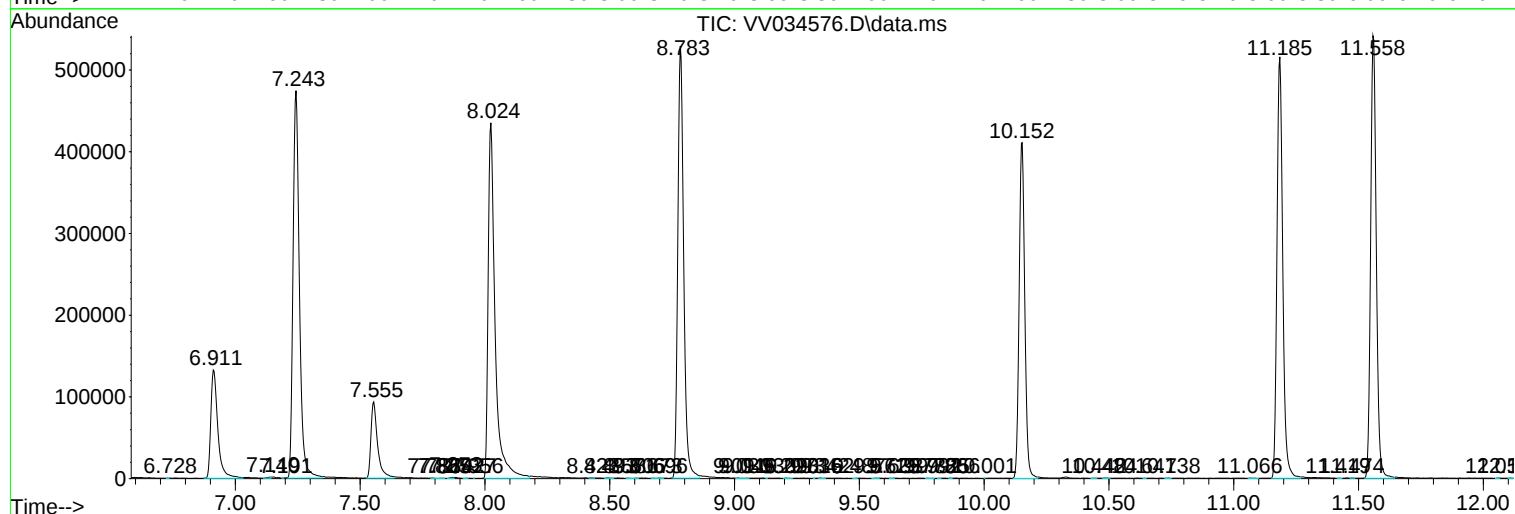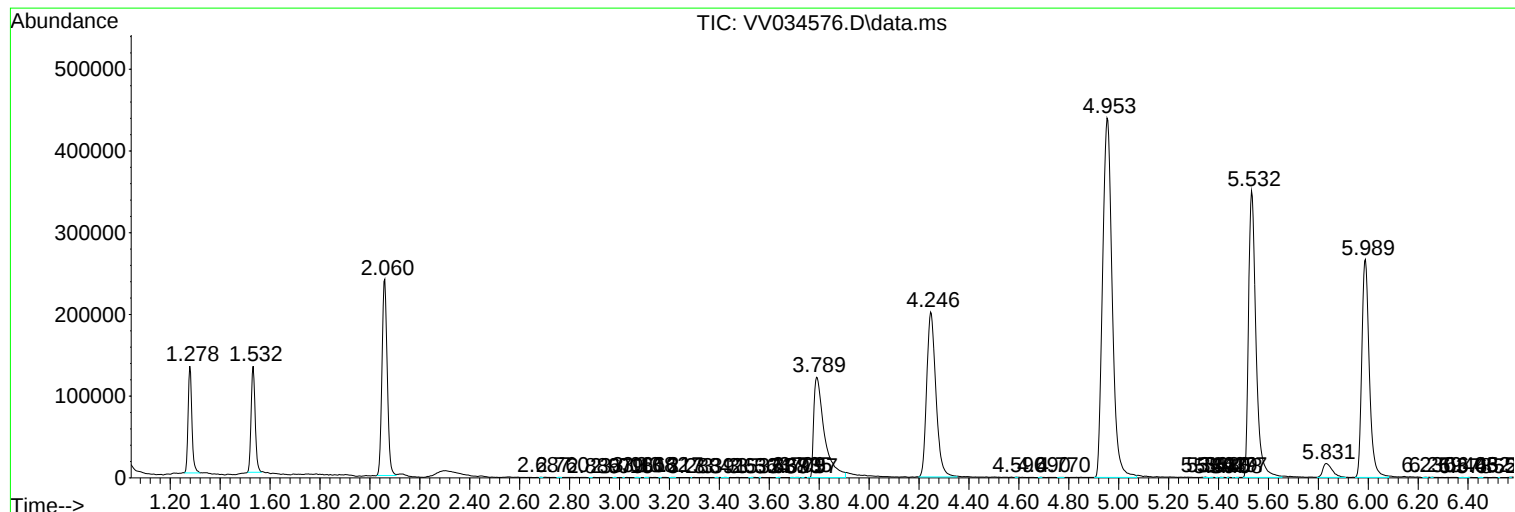

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034576.D
Acq On : 13 Mar 2024 15:40
Operator : SY/MD
Sample : P1739-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034576.D
Acq On : 13 Mar 2024 15:40
Operator : SY/MD
Sample : P1739-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc