

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034577.D
 Acq On : 13 Mar 2024 16:04
 Operator : SY/MD
 Sample : P1739-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034577.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	95	rVB	122334	130820	12.05%	1.457%
2	1.532	146	153	166	rBV	120451	141838	13.07%	1.580%
3	2.060	306	317	334	rBV2	247225	385416	35.50%	4.294%
4	2.809	547	550	553	rBV	140	132	0.01%	0.001%
5	3.011	611	613	614	rBV	160	49	0.00%	0.001%
6	3.076	631	633	636	rVB	206	104	0.01%	0.001%
7	3.105	636	642	643	rBV	540	513	0.05%	0.006%
8	3.208	672	674	679	rBV2	319	234	0.02%	0.003%
9	3.262	690	691	693	rVB	296	105	0.01%	0.001%
10	3.455	747	751	754	rBV2	248	170	0.02%	0.002%
11	3.561	783	784	785	rVB	141	27	0.00%	0.000%
12	3.577	785	789	792	rBV2	210	181	0.02%	0.002%
13	3.674	814	819	822	rBV2	304	253	0.02%	0.003%
14	3.690	822	824	826	rBV	134	67	0.01%	0.001%
15	3.722	831	834	836	rBV	207	143	0.01%	0.002%
16	3.757	841	845	847	rBV2	189	99	0.01%	0.001%
17	3.796	848	857	901	rBV	116009	389981	35.92%	4.345%
18	4.246	983	997	1027	rBV	180812	463820	42.73%	5.167%
19	4.519	1071	1082	1100	rVB4	6821	16560	1.53%	0.184%
20	4.744	1149	1152	1154	rBV	386	179	0.02%	0.002%
21	4.767	1154	1159	1161	rBV	257	230	0.02%	0.003%
22	4.860	1185	1188	1196	rBV3	265	309	0.03%	0.003%
23	4.896	1196	1199	1200	rBV	275	139	0.01%	0.002%
24	4.953	1202	1217	1249	rBV3	403440	1085592	100.00%	12.094%
25	5.455	1371	1373	1378	rVB2	376	235	0.02%	0.003%
26	5.532	1386	1397	1429	rBV	348449	723468	66.64%	8.060%
27	5.834	1479	1491	1517	rBV7	27350	68136	6.28%	0.759%
28	5.986	1526	1538	1573	rBV	247896	516834	47.61%	5.758%
29	6.227	1611	1613	1618	rVB2	270	186	0.02%	0.002%
30	6.272	1623	1627	1631	rBV2	409	405	0.04%	0.005%
31	6.336	1643	1647	1650	rBV2	188	161	0.01%	0.002%
32	6.359	1653	1654	1655	rBV	193	41	0.00%	0.000%
33	6.429	1673	1676	1677	rBV	149	75	0.01%	0.001%
34	6.532	1706	1708	1711	rBV	190	72	0.01%	0.001%
35	6.587	1719	1725	1726	rBV	971	758	0.07%	0.008%
36	6.789	1786	1788	1791	rVB2	212	85	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034577.D
 Acq On : 13 Mar 2024 16:04
 Operator : SY/MD
 Sample : P1739-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.805	1791	1793	1794	rBV2	166	55	0.01%	0.001%
38	6.873	1813	1814	1816	rVB	171	61	0.01%	0.001%
39	6.915	1816	1827	1851	rBV	121775	237798	21.90%	2.649%
40	7.137	1890	1896	1899	rBV4	1616	1837	0.17%	0.020%
41	7.243	1918	1929	1955	rBV	440645	768024	70.75%	8.556%
42	7.555	2016	2026	2053	rBV	86033	159102	14.66%	1.772%
43	7.799	2101	2102	2104	rVB	317	91	0.01%	0.001%
44	7.873	2118	2125	2135	rVB3	1271	2136	0.20%	0.024%
45	7.937	2143	2145	2146	rBV3	168	58	0.01%	0.001%
46	8.024	2163	2172	2216	rBV	406598	777372	71.61%	8.660%
47	8.686	2373	2378	2380	rBV2	272	291	0.03%	0.003%
48	8.783	2397	2408	2435	rBV	527022	874289	80.54%	9.740%
49	9.079	2498	2500	2504	rBV	280	134	0.01%	0.001%
50	9.146	2519	2521	2525	rVB2	395	192	0.02%	0.002%
51	9.169	2525	2528	2532	rBV2	186	139	0.01%	0.002%
52	9.207	2538	2540	2543	rBV2	245	122	0.01%	0.001%
53	9.262	2555	2557	2558	rBV2	171	73	0.01%	0.001%
54	9.410	2601	2603	2604	rBV	186	43	0.00%	0.000%
55	9.493	2626	2629	2633	rBV3	271	229	0.02%	0.003%
56	9.760	2709	2712	2713	rBV	168	94	0.01%	0.001%
57	10.001	2785	2787	2790	rVB	284	124	0.01%	0.001%
58	10.153	2822	2834	2858	rBV	385286	615807	56.73%	6.860%
59	10.323	2884	2887	2897	rVB5	1490	1781	0.16%	0.020%
60	10.574	2962	2965	2967	rBV	131	94	0.01%	0.001%
61	10.677	2996	2997	3001	rVB2	191	95	0.01%	0.001%
62	10.850	3049	3051	3055	rBV	157	72	0.01%	0.001%
63	11.059	3113	3116	3119	rVB	287	138	0.01%	0.002%
64	11.133	3137	3139	3140	rBV2	136	70	0.01%	0.001%
65	11.185	3144	3155	3179	rBV	529639	828544	76.32%	9.230%
66	11.365	3208	3211	3214	rBV3	557	459	0.04%	0.005%
67	11.561	3260	3272	3292	rBV	483149	778092	71.67%	8.668%
68	12.014	3409	3413	3416	rBV2	478	298	0.03%	0.003%
69	12.870	3675	3679	3681	rBV3	452	339	0.03%	0.004%
70	13.107	3750	3753	3755	rBV	342	279	0.03%	0.003%
71	13.339	3823	3825	3827	rBV	359	180	0.02%	0.002%
72	14.233	4101	4103	4105	rBV	468	228	0.02%	0.003%




Sum of corrected areas: 8976157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034577.D
Acq On : 13 Mar 2024 16:04
Operator : SY/MD
Sample : P1739-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

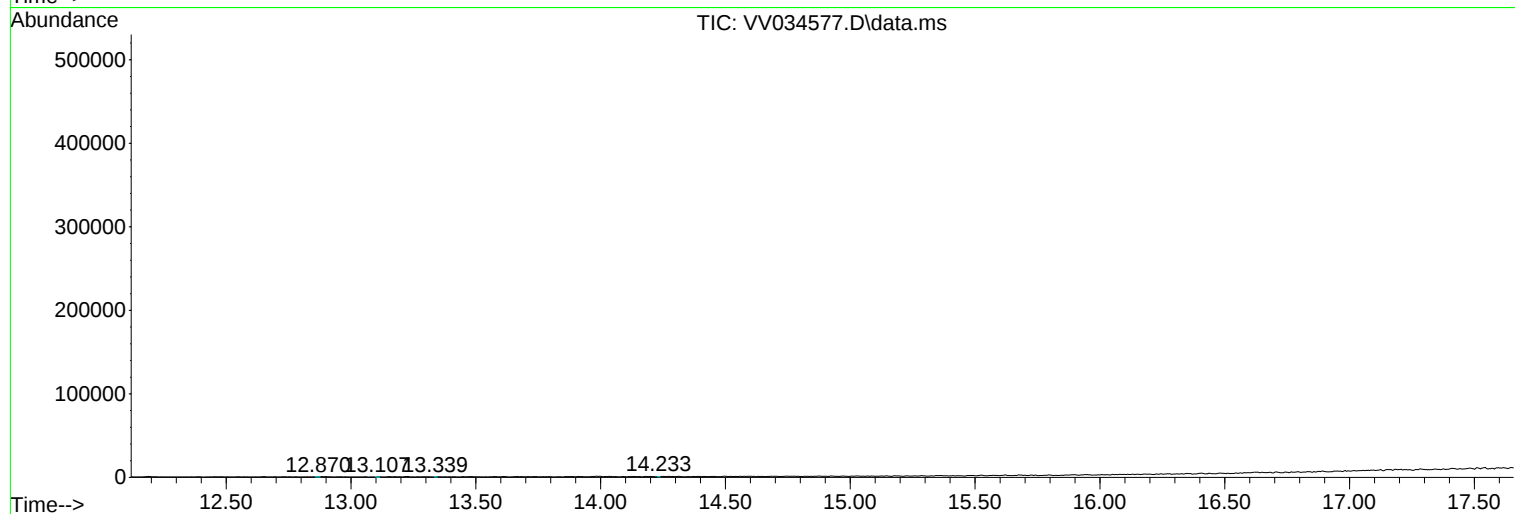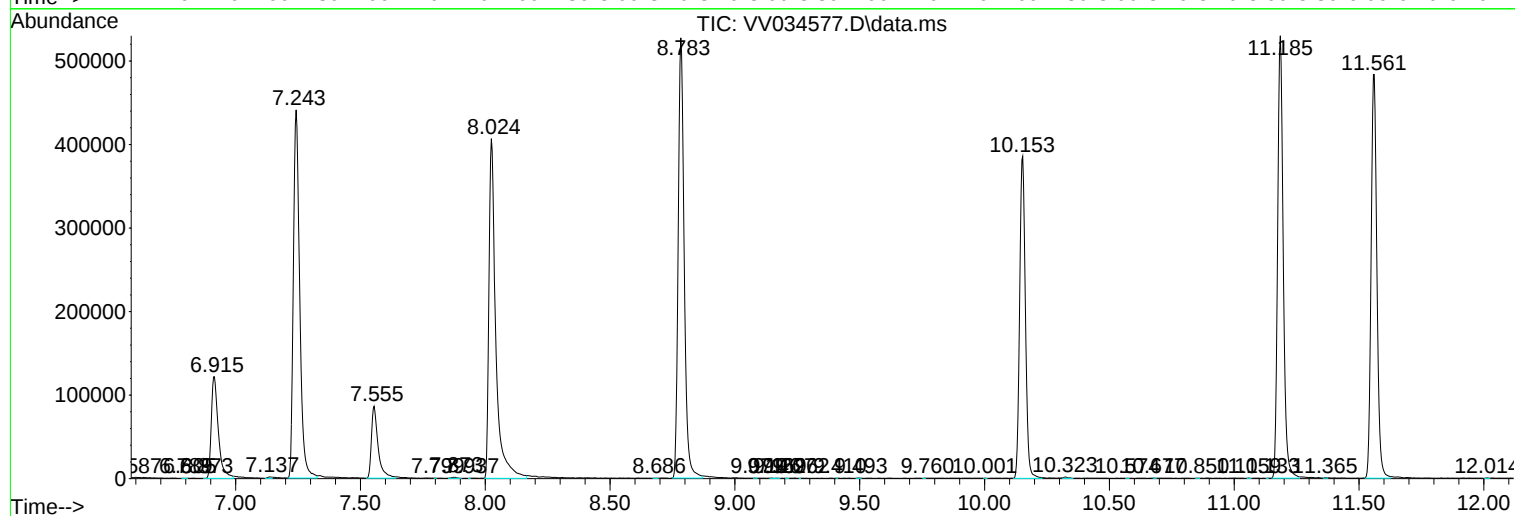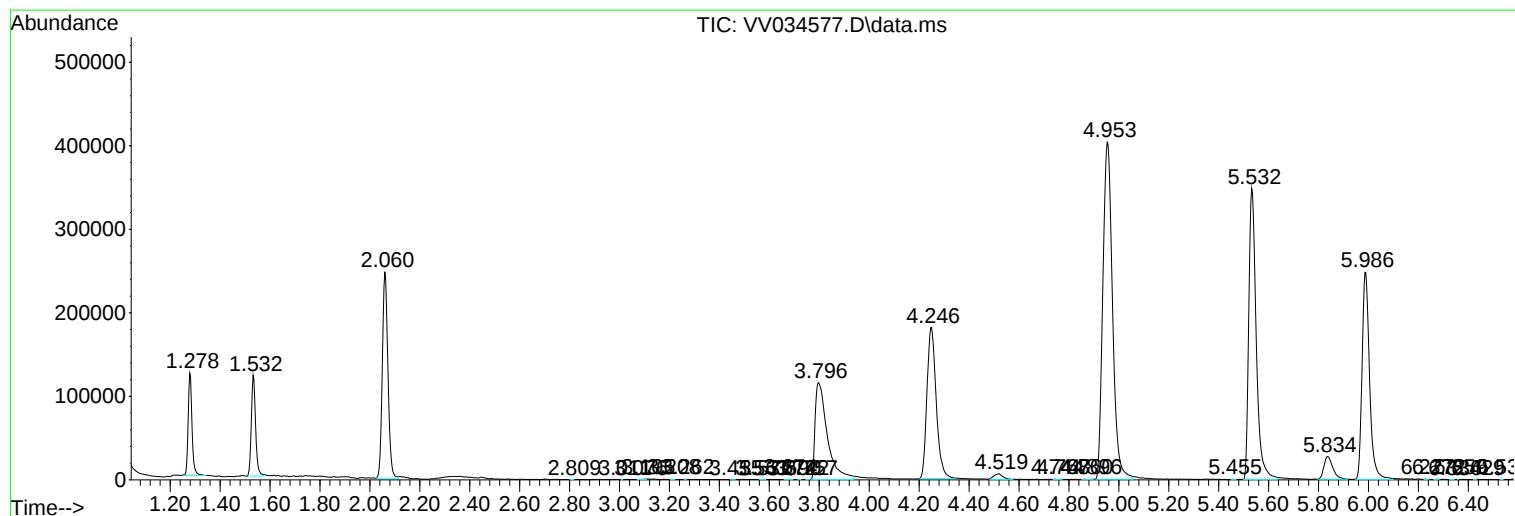

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034577.D
Acq On : 13 Mar 2024 16:04
Operator : SY/MD
Sample : P1739-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034577.D
Acq On : 13 Mar 2024 16:04
Operator : SY/MD
Sample : P1739-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
