

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034579.D
 Acq On : 13 Mar 2024 16:52
 Operator : SY/MD
 Sample : P1739-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	123979	131600	12.05%	1.489%
2	1.532	146	153	171	rVB	122088	140798	12.89%	1.594%
3	2.060	307	317	335	rBV	218245	322447	29.51%	3.649%
4	2.237	369	372	373	rBV	566	321	0.03%	0.004%
5	2.352	405	408	423	rVB	9901	9642	0.88%	0.109%
6	2.516	457	459	461	rBV	284	132	0.01%	0.001%
7	2.597	482	484	485	rBV	224	106	0.01%	0.001%
8	2.642	496	498	503	rBV2	180	116	0.01%	0.001%
9	2.748	528	531	534	rBV2	283	198	0.02%	0.002%
10	2.799	544	547	549	rBV2	130	88	0.01%	0.001%
11	2.815	549	552	554	rBV	224	138	0.01%	0.002%
12	2.870	565	569	571	rBV	281	200	0.02%	0.002%
13	2.921	583	585	586	rBV	164	75	0.01%	0.001%
14	2.960	593	597	600	rBV2	189	178	0.02%	0.002%
15	3.024	615	617	621	rVB	229	137	0.01%	0.002%
16	3.047	621	624	626	rBV2	143	92	0.01%	0.001%
17	3.169	658	662	666	rBV	172	178	0.02%	0.002%
18	3.214	673	676	680	rBV	226	189	0.02%	0.002%
19	3.259	685	690	694	rBV	156	197	0.02%	0.002%
20	3.282	694	697	705	rVB2	267	296	0.03%	0.003%
21	3.346	715	717	720	rBV2	136	76	0.01%	0.001%
22	3.436	742	745	750	rBV2	298	218	0.02%	0.002%
23	3.474	755	757	761	rVB2	225	139	0.01%	0.002%
24	3.497	761	764	767	rBV	179	126	0.01%	0.001%
25	3.664	813	816	819	rBV	159	114	0.01%	0.001%
26	3.706	826	829	831	rBV2	180	131	0.01%	0.001%
27	3.793	847	856	896	rBV	111848	332706	30.45%	3.766%
28	4.249	981	998	1038	rBV	181775	471185	43.13%	5.333%
29	4.712	1138	1142	1145	rBV2	310	243	0.02%	0.003%
30	4.728	1145	1147	1149	rVB	144	57	0.01%	0.001%
31	4.748	1149	1153	1159	rBV2	374	439	0.04%	0.005%
32	4.783	1161	1164	1165	rBV	215	119	0.01%	0.001%
33	4.815	1170	1174	1179	rBV3	301	316	0.03%	0.004%
34	4.844	1179	1183	1186	rVB	372	276	0.03%	0.003%
35	4.870	1187	1191	1196	rBV3	242	225	0.02%	0.003%
36	4.953	1202	1217	1254	rBV2	404202	1092557	100.00%	12.366%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031324\
 Data File : VW034579.D
 Acq On : 13 Mar 2024 16:52
 Operator : SY/MD
 Sample : P1739-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.352	1339	1341	1343	rVB2	556	240	0.02%	0.003%
38	5.371	1343	1347	1348	rBV	275	140	0.01%	0.002%
39	5.439	1361	1368	1370	rVB2	320	364	0.03%	0.004%
40	5.532	1386	1397	1432	rBV	348611	724375	66.30%	8.198%
41	5.834	1479	1491	1506	rBV5	12800	27622	2.53%	0.313%
42	5.989	1526	1539	1576	rBV	250131	522913	47.86%	5.918%
43	6.214	1607	1609	1610	rBV	333	154	0.01%	0.002%
44	6.252	1619	1621	1626	rVB2	369	245	0.02%	0.003%
45	6.381	1659	1661	1663	rBV	300	149	0.01%	0.002%
46	6.468	1683	1688	1691	rBV	239	211	0.02%	0.002%
47	6.551	1709	1714	1716	rBV2	163	151	0.01%	0.002%
48	6.574	1717	1721	1722	rBV2	460	291	0.03%	0.003%
49	6.709	1760	1763	1767	rVV3	248	157	0.01%	0.002%
50	6.725	1767	1768	1770	rVB3	246	52	0.00%	0.001%
51	6.760	1776	1779	1783	rBV2	340	369	0.03%	0.004%
52	6.915	1816	1827	1852	rBV	123137	240049	21.97%	2.717%
53	7.146	1891	1899	1901	rBV3	993	1520	0.14%	0.017%
54	7.243	1918	1929	1963	rBV	435702	776414	71.06%	8.787%
55	7.555	2017	2026	2055	rBV	86240	158615	14.52%	1.795%
56	7.770	2089	2093	2095	rBV	274	190	0.02%	0.002%
57	7.796	2099	2101	2103	rBV2	167	62	0.01%	0.001%
58	7.805	2103	2104	2105	rBV	239	51	0.00%	0.001%
59	7.825	2108	2110	2111	rBV	95	49	0.00%	0.001%
60	7.850	2115	2118	2119	rBV2	394	212	0.02%	0.002%
61	7.953	2147	2150	2151	rBV	199	94	0.01%	0.001%
62	8.024	2163	2172	2219	rBV	404800	773910	70.83%	8.759%
63	8.510	2321	2323	2324	rBV	207	108	0.01%	0.001%
64	8.532	2327	2330	2333	rVB	335	243	0.02%	0.003%
65	8.593	2346	2349	2351	rBV3	177	121	0.01%	0.001%
66	8.674	2372	2374	2378	rVB	274	125	0.01%	0.001%
67	8.696	2379	2381	2385	rVB2	532	309	0.03%	0.003%
68	8.715	2385	2387	2388	rBV	145	66	0.01%	0.001%
69	8.783	2397	2408	2437	rBV	533197	868977	79.54%	9.835%
70	9.011	2477	2479	2484	rVB3	411	208	0.02%	0.002%
71	9.053	2486	2492	2495	rBV2	431	291	0.03%	0.003%
72	9.108	2506	2509	2510	rBV	187	120	0.01%	0.001%
73	9.117	2510	2512	2513	rVV	170	53	0.00%	0.001%
74	9.265	2555	2558	2561	rBV2	196	136	0.01%	0.002%
75	9.323	2573	2576	2579	rVB	214	166	0.02%	0.002%
76	9.375	2591	2592	2596	rVB	278	126	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034579.D
 Acq On : 13 Mar 2024 16:52
 Operator : SY/MD
 Sample : P1739-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	9.403	2597	2601	2603	rBV	194	148	0.01%	0.002%
78	9.493	2625	2629	2630	rBV2	289	182	0.02%	0.002%
79	9.619	2665	2668	2674	rVB	281	229	0.02%	0.003%
80	9.645	2674	2676	2681	rBV	234	246	0.02%	0.003%
81	9.699	2690	2693	2699	rVB2	353	283	0.03%	0.003%
82	9.796	2721	2723	2727	rBV2	184	116	0.01%	0.001%
83	9.831	2731	2734	2737	rBV2	131	99	0.01%	0.001%
84	9.866	2743	2745	2750	rVB2	386	176	0.02%	0.002%
85	10.024	2791	2794	2796	rBV2	186	125	0.01%	0.001%
86	10.072	2805	2809	2810	rBV	229	154	0.01%	0.002%
87	10.153	2821	2834	2858	rBV	387800	612657	56.08%	6.934%
88	10.326	2882	2888	2896	rVB3	1159	1773	0.16%	0.020%
89	10.355	2896	2897	2902	rVB2	176	96	0.01%	0.001%
90	10.429	2916	2920	2923	rBV	189	176	0.02%	0.002%
91	10.461	2928	2930	2931	rBV	199	65	0.01%	0.001%
92	10.702	3003	3005	3007	rVV2	191	76	0.01%	0.001%
93	10.719	3007	3010	3015	rVB2	232	197	0.02%	0.002%
94	10.918	3069	3072	3075	rBV2	269	223	0.02%	0.003%
95	11.124	3134	3136	3138	rBV	179	68	0.01%	0.001%
96	11.185	3144	3155	3177	rBV	526396	821221	75.17%	9.295%
97	11.397	3218	3221	3227	rVB3	610	445	0.04%	0.005%
98	11.561	3260	3272	3301	rBV	488448	790337	72.34%	8.945%
99	12.300	3499	3502	3507	rBV2	279	284	0.03%	0.003%
100	14.921	4314	4317	4319	rBV2	580	413	0.04%	0.005%




Sum of corrected areas: 8835492

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034579.D
Acq On : 13 Mar 2024 16:52
Operator : SY/MD
Sample : P1739-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

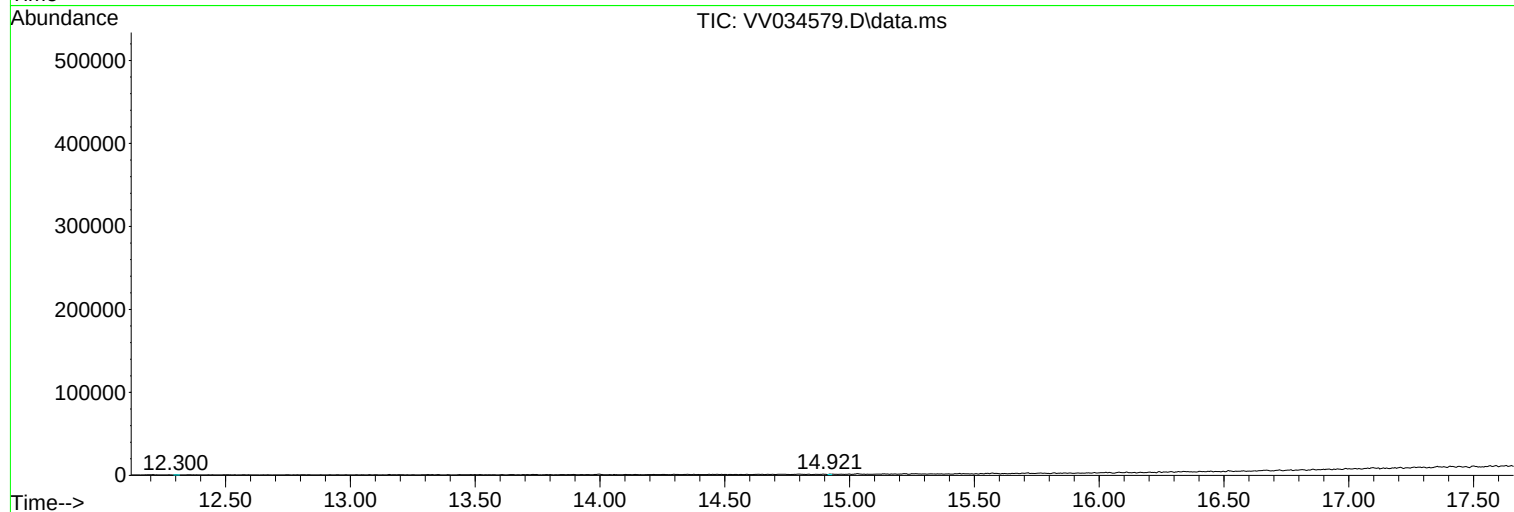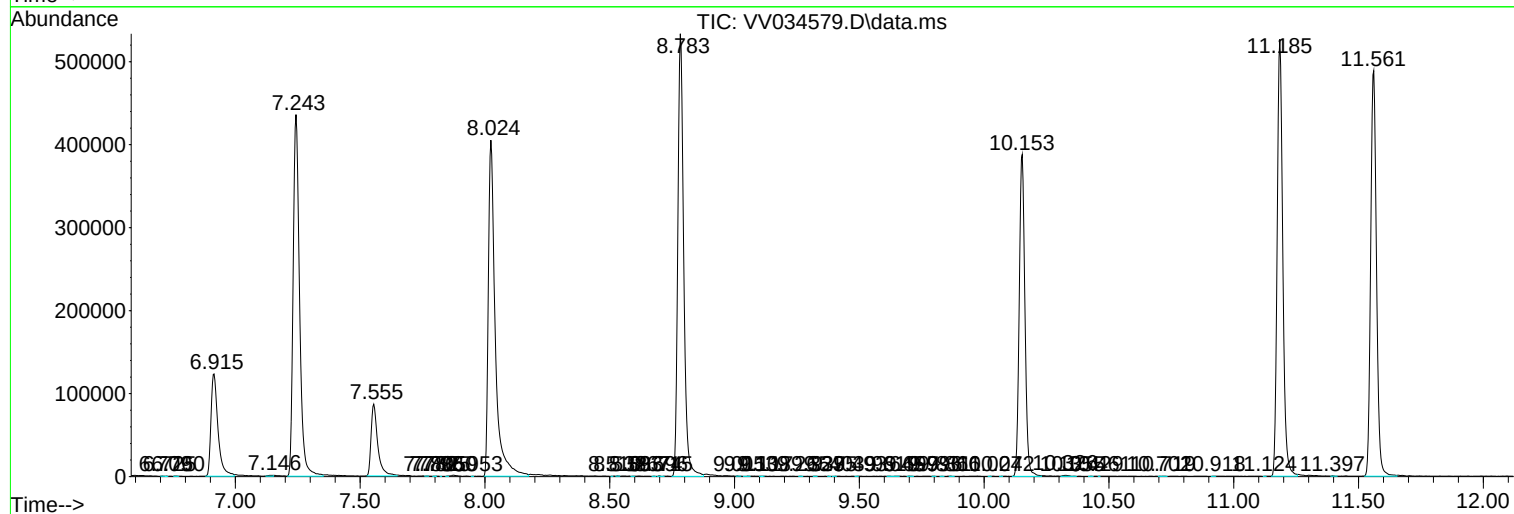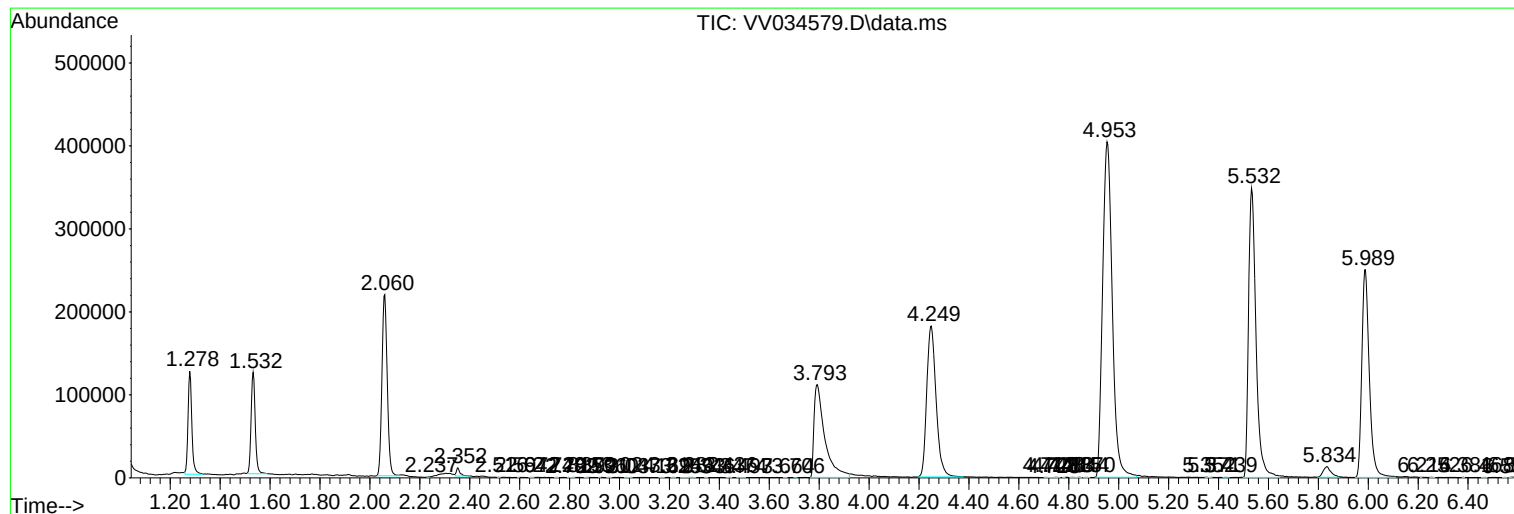

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034579.D
Acq On : 13 Mar 2024 16:52
Operator : SY/MD
Sample : P1739-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034579.D
Acq On : 13 Mar 2024 16:52
Operator : SY/MD
Sample : P1739-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc