

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034582.D
 Acq On : 13 Mar 2024 18:04
 Operator : SY/MD
 Sample : P1739-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034582.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	110856	119600	11.54%	1.401%
2	1.532	146	153	165	rVB	113845	129444	12.49%	1.516%
3	2.060	307	317	334	rBV	208984	303664	29.31%	3.557%
4	2.262	369	380	381	rBV4	1936	2367	0.23%	0.028%
5	2.532	462	464	465	rBV	117	50	0.00%	0.001%
6	2.571	470	476	479	rBV3	360	402	0.04%	0.005%
7	2.680	508	510	511	rVB	166	48	0.00%	0.001%
8	2.700	511	516	517	rBV2	278	240	0.02%	0.003%
9	2.851	560	563	566	rBV	145	105	0.01%	0.001%
10	2.886	571	574	580	rVV2	175	200	0.02%	0.002%
11	2.909	580	581	583	rVB	150	39	0.00%	0.000%
12	3.056	624	627	630	rVB2	303	197	0.02%	0.002%
13	3.073	630	632	634	rVB2	57	21	0.00%	0.000%
14	3.082	634	635	636	rBV2	139	41	0.00%	0.000%
15	3.095	636	639	642	rVB	189	115	0.01%	0.001%
16	3.175	661	664	666	rBV	207	148	0.01%	0.002%
17	3.208	671	674	679	rVB2	222	197	0.02%	0.002%
18	3.249	684	687	692	rVB2	110	109	0.01%	0.001%
19	3.282	692	697	699	rBV2	162	150	0.01%	0.002%
20	3.343	711	716	718	rBV2	138	104	0.01%	0.001%
21	3.420	737	740	742	rBV2	112	72	0.01%	0.001%
22	3.513	764	769	770	rBV2	124	108	0.01%	0.001%
23	3.526	770	773	775	rVV	95	65	0.01%	0.001%
24	3.593	793	794	796	rBV	120	53	0.01%	0.001%
25	3.677	817	820	821	rBV	97	55	0.01%	0.001%
26	3.696	823	826	827	rBV	127	81	0.01%	0.001%
27	3.793	847	856	899	rBV	107293	325048	31.37%	3.808%
28	4.246	984	997	1026	rVB2	175286	440965	42.56%	5.166%
29	4.516	1079	1081	1085	rVB2	468	245	0.02%	0.003%
30	4.748	1148	1153	1154	rBV2	135	131	0.01%	0.002%
31	4.790	1161	1166	1169	rBV3	473	489	0.05%	0.006%
32	4.851	1180	1185	1187	rBV2	425	404	0.04%	0.005%
33	4.954	1201	1217	1249	rBV2	387222	1036041	100.00%	12.136%
34	5.259	1309	1312	1313	rBV	288	163	0.02%	0.002%
35	5.275	1315	1317	1319	rBV2	298	121	0.01%	0.001%
36	5.462	1370	1375	1376	rBV	168	143	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034582.D
 Acq On : 13 Mar 2024 18:04
 Operator : SY/MD
 Sample : P1739-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1431	rBV	348648	719741	69.47%	8.431%
38	5.838	1479	1492	1512	rBV6	26499	65232	6.30%	0.764%
39	5.989	1523	1539	1563	rBV	238003	499357	48.20%	5.850%
40	6.301	1633	1636	1641	rBV	417	269	0.03%	0.003%
41	6.458	1680	1685	1687	rBV2	185	122	0.01%	0.001%
42	6.507	1697	1700	1701	rBV	191	86	0.01%	0.001%
43	6.519	1702	1704	1705	rVB	131	36	0.00%	0.000%
44	6.584	1718	1724	1726	rBV3	646	621	0.06%	0.007%
45	6.834	1799	1802	1805	rBV	280	176	0.02%	0.002%
46	6.857	1805	1809	1812	rBV	182	135	0.01%	0.002%
47	6.915	1816	1827	1849	rBV	116289	227282	21.94%	2.662%
48	7.095	1880	1883	1885	rBV2	340	230	0.02%	0.003%
49	7.146	1892	1899	1905	rBV4	1299	2262	0.22%	0.026%
50	7.243	1916	1929	1962	rBV	412154	735198	70.96%	8.612%
51	7.555	2016	2026	2051	rBV	79216	150026	14.48%	1.757%
52	7.757	2087	2089	2091	rBV2	387	128	0.01%	0.001%
53	7.867	2117	2123	2124	rBV2	922	692	0.07%	0.008%
54	7.966	2151	2154	2156	rBV	128	72	0.01%	0.001%
55	7.992	2160	2162	2163	rBV	168	53	0.01%	0.001%
56	8.024	2163	2172	2218	rBV	389468	749186	72.31%	8.776%
57	8.580	2340	2345	2348	rBV	363	362	0.03%	0.004%
58	8.696	2379	2381	2382	rBV	189	90	0.01%	0.001%
59	8.709	2382	2385	2388	rVB2	231	182	0.02%	0.002%
60	8.725	2388	2390	2392	rBV2	222	150	0.01%	0.002%
61	8.783	2397	2408	2446	rBV	523684	865648	83.55%	10.140%
62	9.114	2510	2511	2514	rVB	133	52	0.01%	0.001%
63	9.194	2532	2536	2540	rBV2	211	204	0.02%	0.002%
64	9.217	2541	2543	2548	rVB	328	164	0.02%	0.002%
65	9.252	2548	2554	2560	rBV2	279	349	0.03%	0.004%
66	9.281	2561	2563	2566	rBV	172	113	0.01%	0.001%
67	9.301	2566	2569	2571	rBV2	152	80	0.01%	0.001%
68	9.339	2578	2581	2583	rBV	262	143	0.01%	0.002%
69	9.375	2590	2592	2594	rBV2	96	61	0.01%	0.001%
70	9.400	2599	2600	2601	rVV2	131	28	0.00%	0.000%
71	9.420	2603	2606	2610	rVB2	169	114	0.01%	0.001%
72	9.519	2635	2637	2638	rBV2	211	101	0.01%	0.001%
73	9.539	2641	2643	2647	rVB	273	115	0.01%	0.001%
74	9.590	2655	2659	2662	rBV	198	148	0.01%	0.002%
75	9.735	2698	2704	2706	rBV2	242	270	0.03%	0.003%
76	9.789	2719	2721	2722	rVB2	208	59	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034582.D
 Acq On : 13 Mar 2024 18:04
 Operator : SY/MD
 Sample : P1739-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	9.863	2741	2744	2748	rBV2	286	166	0.02%	0.002%
78	10.043	2796	2800	2801	rBV2	252	168	0.02%	0.002%
79	10.153	2822	2834	2854	rBV	373047	588231	56.78%	6.891%
80	10.420	2914	2917	2919	rBV2	164	104	0.01%	0.001%
81	10.539	2952	2954	2957	rVB	158	43	0.00%	0.001%
82	11.130	3135	3138	3141	rBV2	257	155	0.01%	0.002%
83	11.185	3144	3155	3181	rBV	519224	815180	78.68%	9.549%
84	11.410	3223	3225	3228	rBV3	336	149	0.01%	0.002%
85	11.474	3242	3245	3246	rBV	284	153	0.01%	0.002%
86	11.516	3251	3258	3260	rBV2	340	389	0.04%	0.005%
87	11.558	3260	3271	3298	rBV	466531	749877	72.38%	8.784%
88	12.699	3624	3626	3629	rBV	203	146	0.01%	0.002%
89	12.940	3695	3701	3703	rBV2	301	358	0.03%	0.004%
90	13.040	3730	3732	3733	rVB	228	62	0.01%	0.001%
91	13.136	3757	3762	3766	rBV3	409	431	0.04%	0.005%
92	13.198	3778	3781	3784	rBV3	290	198	0.02%	0.002%
93	13.780	3961	3962	3964	rBV	358	118	0.01%	0.001%




Sum of corrected areas: 8536690

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034582.D
Acq On : 13 Mar 2024 18:04
Operator : SY/MD
Sample : P1739-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

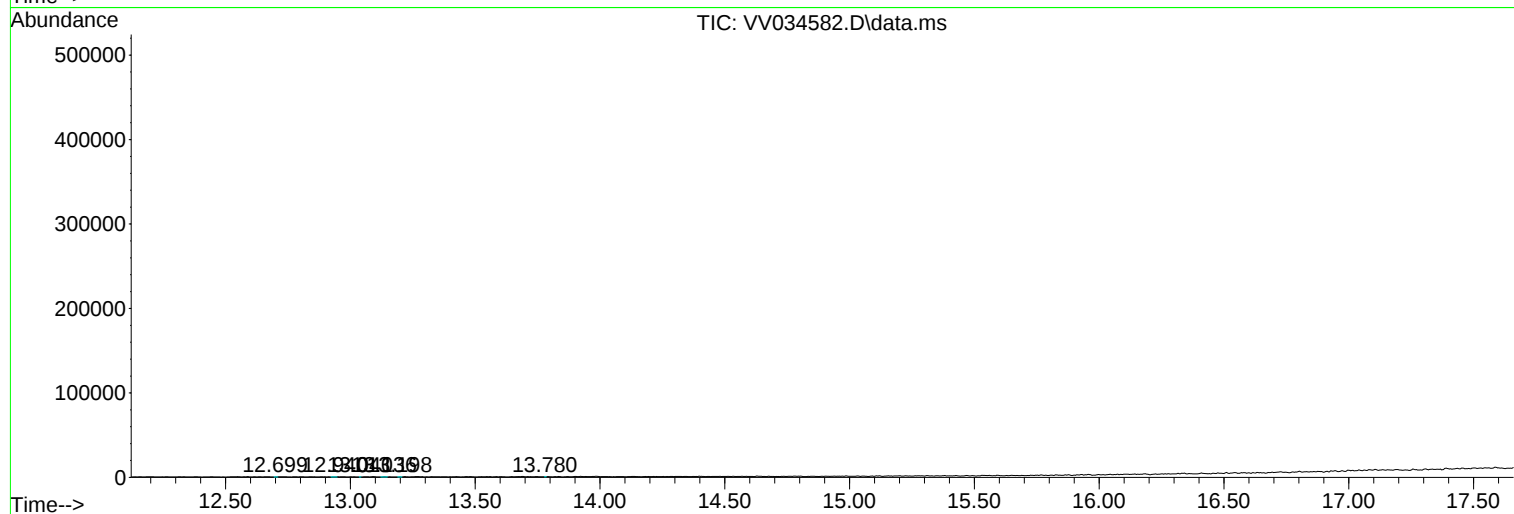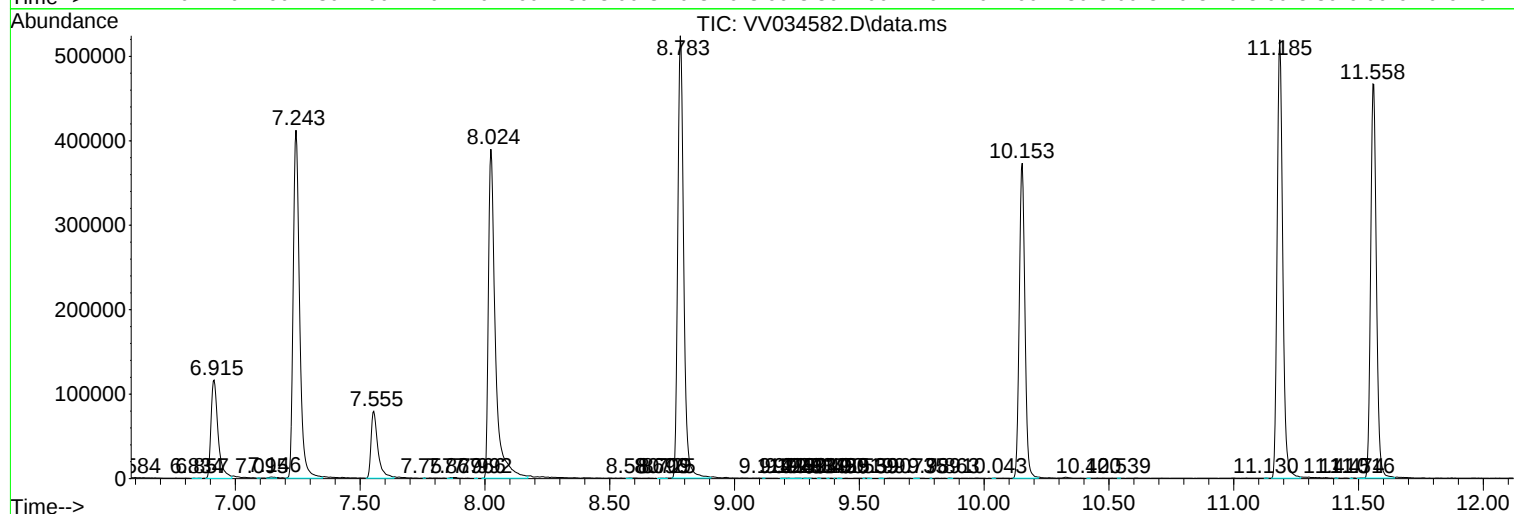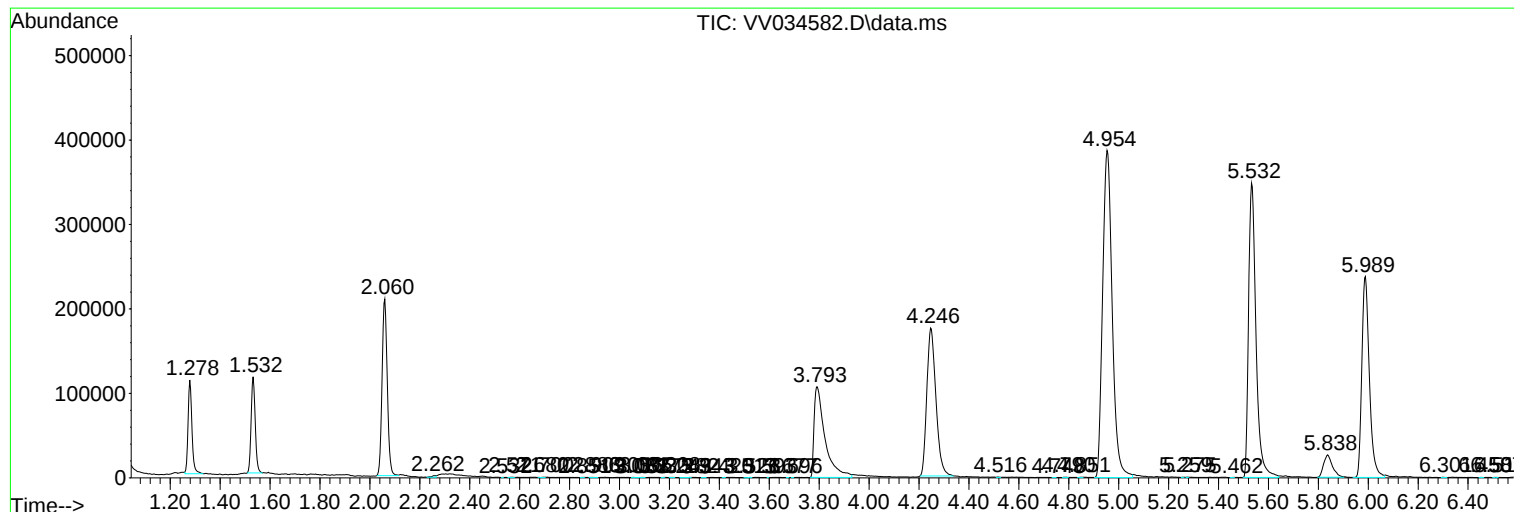

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034582.D
Acq On : 13 Mar 2024 18:04
Operator : SY/MD
Sample : P1739-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034582.D
Acq On : 13 Mar 2024 18:04
Operator : SY/MD
Sample : P1739-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
