

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034584.D
 Acq On : 13 Mar 2024 18:51
 Operator : SY/MD
 Sample : P1739-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034584.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	95777	103846	10.48%	1.276%
2	1.532	146	153	166	rVB	102272	116654	11.77%	1.434%
3	2.056	307	316	328	rBV	179129	257091	25.94%	3.160%
4	2.606	485	487	491	rBV	381	245	0.02%	0.003%
5	2.706	516	518	521	rBV2	341	199	0.02%	0.002%
6	3.011	610	613	615	rBV	187	122	0.01%	0.001%
7	3.092	636	638	641	rBV	191	121	0.01%	0.001%
8	3.175	661	664	667	rBV	184	124	0.01%	0.002%
9	3.339	712	715	718	rBV2	190	165	0.02%	0.002%
10	3.394	730	732	735	rVB	204	100	0.01%	0.001%
11	3.410	735	737	740	rBV	151	93	0.01%	0.001%
12	3.474	753	757	759	rBV	254	191	0.02%	0.002%
13	3.609	796	799	801	rBV2	175	104	0.01%	0.001%
14	3.709	827	830	834	rVB2	128	88	0.01%	0.001%
15	3.793	848	856	896	rBV	107252	325585	32.84%	4.002%
16	4.246	983	997	1026	rBV2	167697	429230	43.30%	5.276%
17	4.661	1121	1126	1129	rBV2	314	312	0.03%	0.004%
18	4.693	1133	1136	1137	rBV	193	128	0.01%	0.002%
19	4.722	1143	1145	1147	rBV2	218	87	0.01%	0.001%
20	4.738	1148	1150	1154	rVB	331	184	0.02%	0.002%
21	4.761	1154	1157	1160	rBV	247	152	0.02%	0.002%
22	4.953	1200	1217	1248	rBV2	366748	991280	100.00%	12.184%
23	5.249	1306	1309	1313	rVB3	363	254	0.03%	0.003%
24	5.291	1319	1322	1325	rBV2	232	179	0.02%	0.002%
25	5.352	1337	1341	1345	rBV3	437	461	0.05%	0.006%
26	5.368	1345	1346	1348	rVV	341	124	0.01%	0.002%
27	5.384	1349	1351	1354	rVB3	250	142	0.01%	0.002%
28	5.455	1370	1373	1375	rBV2	213	145	0.01%	0.002%
29	5.532	1384	1397	1430	rBV	329932	691824	69.79%	8.503%
30	5.834	1480	1491	1519	rVB7	20017	52928	5.34%	0.651%
31	5.989	1526	1539	1565	rBV	229179	478196	48.24%	5.878%
32	6.201	1603	1605	1607	rBV2	369	112	0.01%	0.001%
33	6.378	1658	1660	1663	rVB	226	109	0.01%	0.001%
34	6.397	1663	1666	1669	rBV	235	114	0.01%	0.001%
35	6.413	1669	1671	1674	rVV2	172	117	0.01%	0.001%
36	6.429	1674	1676	1680	rVB2	142	91	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034584.D
 Acq On : 13 Mar 2024 18:51
 Operator : SY/MD
 Sample : P1739-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.478	1689	1691	1696	rBV2	145	104	0.01%	0.001%
38	6.587	1719	1725	1727	rBV3	892	736	0.07%	0.009%
39	6.754	1775	1777	1778	rBV3	216	93	0.01%	0.001%
40	6.915	1817	1827	1860	rBV	113384	222386	22.43%	2.733%
41	7.243	1915	1929	1955	rBV	383279	681271	68.73%	8.374%
42	7.555	2017	2026	2064	rBV	80107	151699	15.30%	1.865%
43	7.838	2111	2114	2117	rBV2	307	147	0.01%	0.002%
44	7.857	2117	2120	2121	rBV	432	192	0.02%	0.002%
45	8.024	2163	2172	2211	rBV	387109	752273	75.89%	9.246%
46	8.452	2302	2305	2310	rVB2	282	201	0.02%	0.002%
47	8.477	2311	2313	2315	rBV2	280	165	0.02%	0.002%
48	8.571	2340	2342	2343	rBV	265	88	0.01%	0.001%
49	8.580	2343	2345	2349	rVB2	432	252	0.03%	0.003%
50	8.722	2388	2389	2391	rBV	251	122	0.01%	0.001%
51	8.783	2397	2408	2431	rBV	507184	830552	83.79%	10.208%
52	9.059	2491	2494	2498	rBV	276	249	0.03%	0.003%
53	9.185	2530	2533	2539	rBV2	262	219	0.02%	0.003%
54	9.249	2550	2553	2557	rBV	287	189	0.02%	0.002%
55	9.329	2576	2578	2581	rBV	180	112	0.01%	0.001%
56	9.410	2601	2603	2606	rVB2	211	127	0.01%	0.002%
57	9.426	2606	2608	2611	rVB2	182	109	0.01%	0.001%
58	9.458	2611	2618	2624	rBV2	296	400	0.04%	0.005%
59	9.487	2624	2627	2629	rBV2	369	211	0.02%	0.003%
60	9.503	2629	2632	2634	rVB2	244	141	0.01%	0.002%
61	9.725	2700	2701	2703	rBV	275	103	0.01%	0.001%
62	9.793	2718	2722	2726	rBV	253	179	0.02%	0.002%
63	9.863	2742	2744	2747	rVB2	273	102	0.01%	0.001%
64	9.883	2747	2750	2753	rVB2	168	93	0.01%	0.001%
65	9.963	2773	2775	2778	rBV	285	175	0.02%	0.002%
66	10.030	2793	2796	2799	rBV2	257	147	0.01%	0.002%
67	10.153	2820	2834	2854	rBV	363229	581401	58.65%	7.146%
68	10.281	2872	2874	2877	rBV	162	97	0.01%	0.001%
69	10.365	2897	2900	2903	rBV2	185	131	0.01%	0.002%
70	10.384	2904	2906	2908	rBV2	224	87	0.01%	0.001%
71	10.600	2971	2973	2976	rVB	283	116	0.01%	0.001%
72	10.799	3031	3035	3036	rBV2	170	117	0.01%	0.001%
73	10.866	3052	3056	3059	rBV2	490	352	0.04%	0.004%
74	11.001	3095	3098	3100	rBV	158	110	0.01%	0.001%
75	11.185	3144	3155	3178	rBV	490344	764465	77.12%	9.396%
76	11.384	3213	3217	3219	rBV2	311	209	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034584.D
 Acq On : 13 Mar 2024 18:51
 Operator : SY/MD
 Sample : P1739-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	11.448	3234	3237	3238	rBV	260	128	0.01%	0.002%
78	11.561	3260	3272	3291	rBV	432531	686042	69.21%	8.432%
79	11.808	3346	3349	3351	rBV2	348	219	0.02%	0.003%
80	11.985	3399	3404	3406	rBV2	259	197	0.02%	0.002%
81	12.059	3424	3427	3434	rVB2	333	317	0.03%	0.004%
82	12.101	3434	3440	3446	rBV	345	387	0.04%	0.005%
83	12.259	3487	3489	3492	rVB2	249	116	0.01%	0.001%
84	12.416	3535	3538	3544	rVB2	469	471	0.05%	0.006%
85	12.442	3544	3546	3547	rBV	164	87	0.01%	0.001%
86	12.458	3549	3551	3554	rVB2	262	163	0.02%	0.002%
87	12.606	3592	3597	3599	rBV2	354	360	0.04%	0.004%
88	12.641	3605	3608	3617	rBV2	240	231	0.02%	0.003%
89	12.805	3655	3659	3663	rBV2	346	328	0.03%	0.004%
90	13.127	3755	3759	3764	rBV	493	388	0.04%	0.005%
91	13.275	3803	3805	3806	rBV	287	86	0.01%	0.001%
92	13.458	3859	3862	3864	rBV2	413	276	0.03%	0.003%
93	13.577	3896	3899	3900	rBV2	224	110	0.01%	0.001%
94	13.638	3915	3918	3922	rVB3	487	386	0.04%	0.005%
95	13.911	4000	4003	4005	rBV2	442	276	0.03%	0.003%
96	13.979	4017	4024	4028	rBV5	674	988	0.10%	0.012%
97	14.091	4058	4059	4063	rBV2	265	187	0.02%	0.002%
98	14.226	4098	4101	4107	rVB3	769	682	0.07%	0.008%
99	14.252	4107	4109	4110	rBV	297	126	0.01%	0.002%
100	14.345	4133	4138	4148	rVB7	1978	2556	0.26%	0.031%




Sum of corrected areas: 8135926

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034584.D
Acq On : 13 Mar 2024 18:51
Operator : SY/MD
Sample : P1739-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

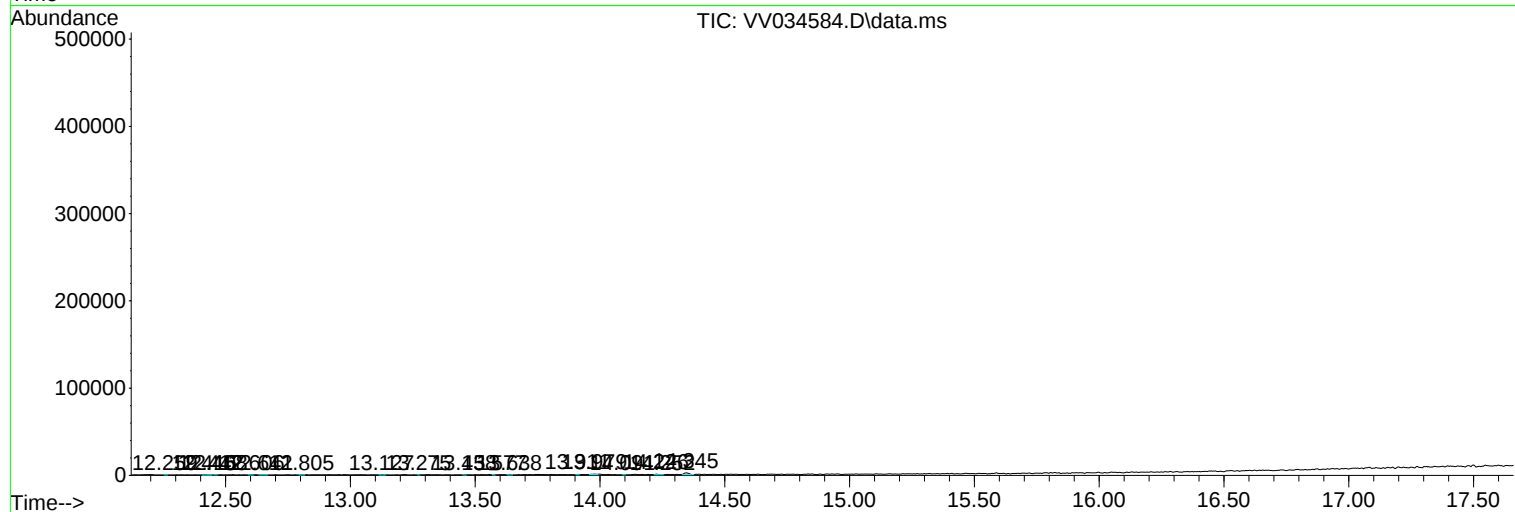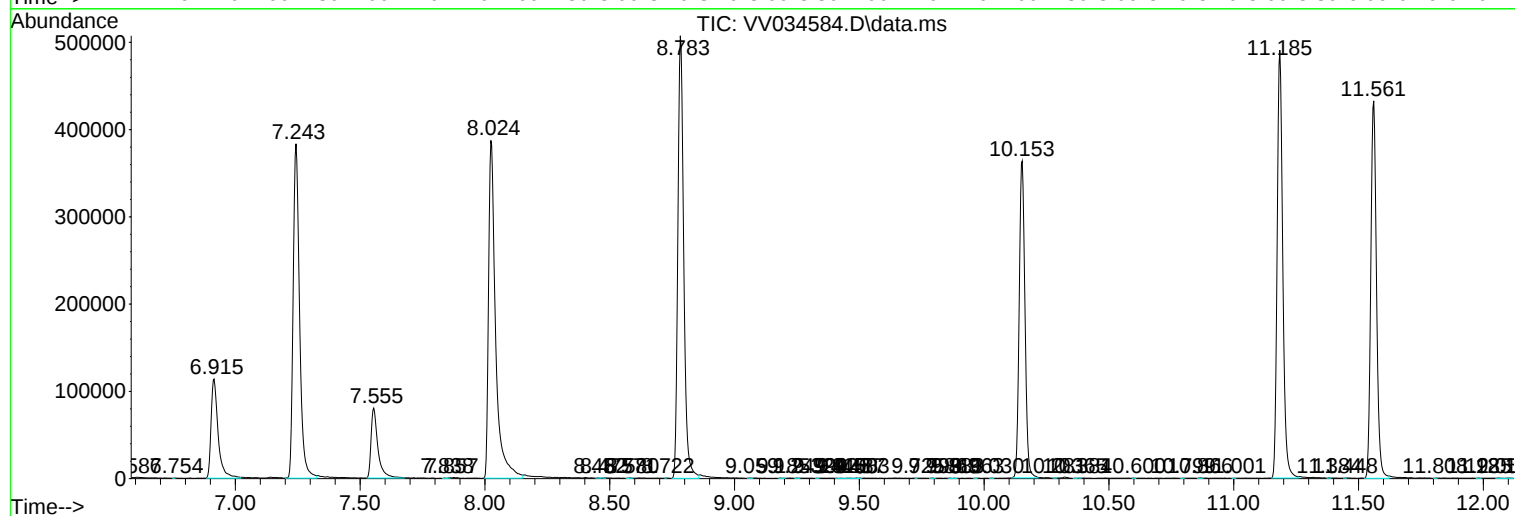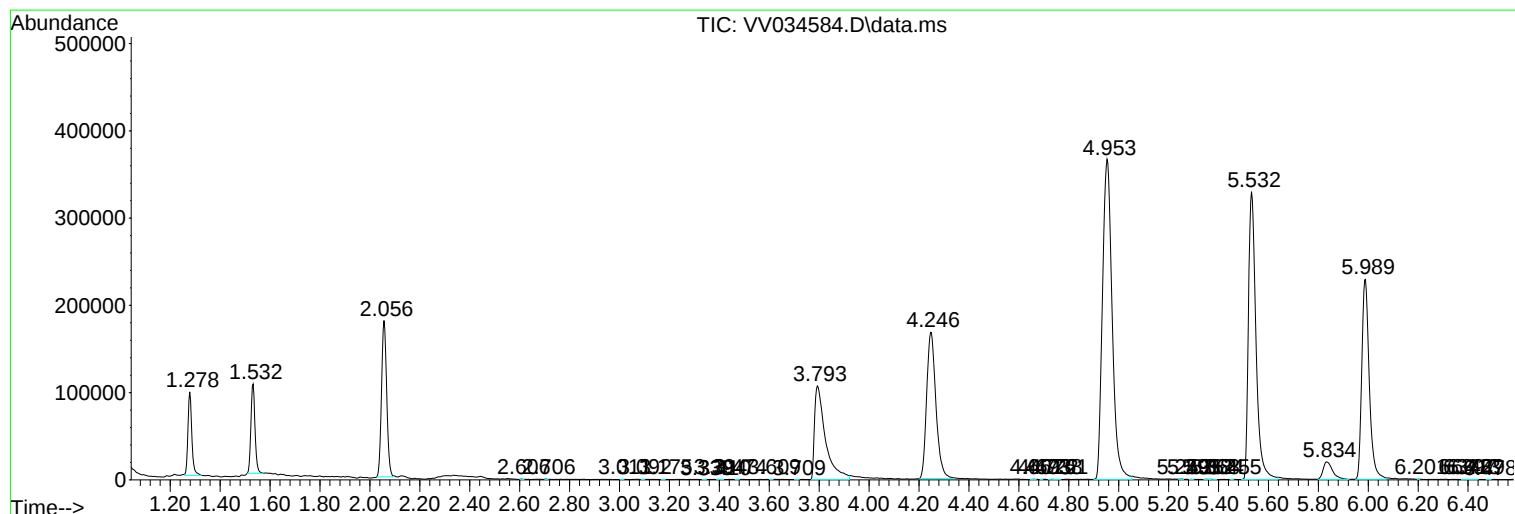

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034584.D
Acq On : 13 Mar 2024 18:51
Operator : SY/MD
Sample : P1739-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034584.D
Acq On : 13 Mar 2024 18:51
Operator : SY/MD
Sample : P1739-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc