

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034586.D
 Acq On : 13 Mar 2024 19:39
 Operator : SY/MD
 Sample : P1739-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	111222	119183	4.38%	1.015%
2	1.529	146	152	167	rVB	112309	130707	4.80%	1.113%
3	2.063	307	318	333	rBV2	281067	471106	17.31%	4.013%
4	2.253	365	377	403	rBV2	6702	25471	0.94%	0.217%
5	2.445	430	437	438	rBV3	1190	1154	0.04%	0.010%
6	2.699	512	516	520	rVV4	956	763	0.03%	0.007%
7	2.735	526	527	534	rVB2	188	154	0.01%	0.001%
8	2.941	588	591	593	rBV2	141	90	0.00%	0.001%
9	2.986	601	605	607	rBV	233	176	0.01%	0.001%
10	3.079	631	634	636	rBV2	211	134	0.00%	0.001%
11	3.111	637	644	645	rBV4	2187	2086	0.08%	0.018%
12	3.188	664	668	670	rBV2	226	166	0.01%	0.001%
13	3.233	678	682	685	rBV2	278	166	0.01%	0.001%
14	3.333	711	713	715	rVB2	299	92	0.00%	0.001%
15	3.349	715	718	722	rBV2	174	152	0.01%	0.001%
16	3.535	772	776	778	rBV	202	164	0.01%	0.001%
17	3.664	812	816	819	rBV2	178	115	0.00%	0.001%
18	3.716	829	832	834	rBV2	160	101	0.00%	0.001%
19	3.748	837	842	844	rBV2	197	144	0.01%	0.001%
20	3.806	845	860	898	rBV2	152723	573345	21.07%	4.884%
21	4.249	982	998	1034	rBV	176368	455377	16.73%	3.879%
22	4.513	1065	1080	1099	rBV	46828	120139	4.42%	1.023%
23	4.613	1109	1111	1115	rVB4	284	146	0.01%	0.001%
24	4.645	1119	1121	1125	rVB3	393	222	0.01%	0.002%
25	4.680	1130	1132	1134	rBV	191	117	0.00%	0.001%
26	4.703	1138	1139	1143	rVB2	180	79	0.00%	0.001%
27	4.725	1143	1146	1149	rBV2	299	259	0.01%	0.002%
28	4.786	1162	1165	1166	rBV	191	106	0.00%	0.001%
29	4.799	1168	1169	1173	rVB3	264	134	0.00%	0.001%
30	4.857	1184	1187	1189	rVB2	245	129	0.00%	0.001%
31	4.953	1202	1217	1251	rBV2	386646	1037542	38.13%	8.839%
32	5.275	1314	1317	1320	rBV2	412	282	0.01%	0.002%
33	5.317	1327	1330	1333	rBV2	344	240	0.01%	0.002%
34	5.355	1340	1342	1346	rVB	411	159	0.01%	0.001%
35	5.410	1351	1359	1360	rBV	281	282	0.01%	0.002%
36	5.455	1369	1373	1379	rBV3	258	276	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034586.D
 Acq On : 13 Mar 2024 19:39
 Operator : SY/MD
 Sample : P1739-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1434	rBV	354651	732958	26.94%	6.244%
38	5.828	1476	1489	1526	rBV	1378658	2721127	100.00%	23.181%
39	5.989	1528	1539	1567	rVB	237486	486749	17.89%	4.147%
40	6.342	1646	1649	1651	rBV	380	199	0.01%	0.002%
41	6.413	1669	1671	1674	rBV	185	88	0.00%	0.001%
42	6.445	1678	1681	1682	rBV	193	91	0.00%	0.001%
43	6.516	1699	1703	1710	rVB2	242	302	0.01%	0.003%
44	6.558	1710	1716	1718	rBV2	123	124	0.00%	0.001%
45	6.590	1718	1726	1733	rBV4	1130	1976	0.07%	0.017%
46	6.850	1801	1807	1813	rBV2	156	233	0.01%	0.002%
47	6.915	1816	1827	1855	rBV	112909	219701	8.07%	1.872%
48	7.243	1917	1929	1964	rBV	396099	712953	26.20%	6.074%
49	7.487	2003	2005	2008	rBV3	485	266	0.01%	0.002%
50	7.555	2017	2026	2055	rBV	76251	141918	5.22%	1.209%
51	7.735	2079	2082	2085	rBV3	389	315	0.01%	0.003%
52	7.786	2093	2098	2101	rBV5	829	989	0.04%	0.008%
53	7.879	2117	2127	2131	rBV4	1526	2241	0.08%	0.019%
54	7.931	2141	2143	2146	rVB	421	174	0.01%	0.001%
55	8.024	2163	2172	2216	rBV	393422	744180	27.35%	6.340%
56	8.484	2311	2315	2319	rBV3	243	311	0.01%	0.003%
57	8.583	2342	2346	2348	rBV2	345	255	0.01%	0.002%
58	8.612	2353	2355	2357	rBV2	229	101	0.00%	0.001%
59	8.625	2357	2359	2363	rBV3	246	166	0.01%	0.001%
60	8.722	2383	2389	2395	rBV2	338	422	0.02%	0.004%
61	8.783	2398	2408	2432	rBV	511702	855078	31.42%	7.284%
62	9.040	2486	2488	2490	rVB2	332	174	0.01%	0.001%
63	9.079	2496	2500	2501	rBV2	199	112	0.00%	0.001%
64	9.198	2533	2537	2540	rBV2	162	164	0.01%	0.001%
65	9.284	2561	2564	2566	rBV2	248	121	0.00%	0.001%
66	9.413	2601	2604	2609	rBV2	171	142	0.01%	0.001%
67	9.490	2626	2628	2631	rBV2	169	78	0.00%	0.001%
68	9.529	2637	2640	2643	rBV	317	205	0.01%	0.002%
69	9.590	2657	2659	2661	rVB	258	109	0.00%	0.001%
70	9.609	2661	2665	2668	rBV2	180	147	0.01%	0.001%
71	9.628	2668	2671	2675	rBV	328	189	0.01%	0.002%
72	9.722	2698	2700	2703	rBV2	120	75	0.00%	0.001%
73	9.905	2755	2757	2761	rBV	270	154	0.01%	0.001%
74	9.966	2772	2776	2777	rBV	210	134	0.00%	0.001%
75	10.040	2794	2799	2804	rVB2	183	235	0.01%	0.002%
76	10.075	2804	2810	2813	rBV	304	293	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034586.D
 Acq On : 13 Mar 2024 19:39
 Operator : SY/MD
 Sample : P1739-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.153	2820	2834	2860	rBV	377427	586603	21.56%	4.997%
78	10.323	2878	2887	2897	rBV7	2039	3590	0.13%	0.031%
79	10.416	2912	2916	2918	rBV	241	183	0.01%	0.002%
80	10.715	3007	3009	3015	rVB2	223	148	0.01%	0.001%
81	11.114	3126	3133	3136	rBV4	1159	1263	0.05%	0.011%
82	11.133	3136	3139	3142	rVB2	386	226	0.01%	0.002%
83	11.185	3144	3155	3176	rBV	529074	826424	30.37%	7.040%
84	11.487	3246	3249	3251	rBV	356	230	0.01%	0.002%
85	11.561	3260	3272	3292	rBV	467902	742096	27.27%	6.322%
86	11.818	3349	3352	3355	rBV2	344	251	0.01%	0.002%
87	11.898	3374	3377	3380	rBV	220	156	0.01%	0.001%
88	12.194	3464	3469	3483	rVB3	1664	2733	0.10%	0.023%
89	12.300	3496	3502	3511	rBV6	2214	3502	0.13%	0.030%
90	12.497	3560	3563	3567	rVB2	276	180	0.01%	0.002%
91	12.593	3589	3593	3596	rBV2	371	323	0.01%	0.003%
92	12.680	3618	3620	3626	rVB	357	204	0.01%	0.002%
93	12.741	3637	3639	3641	rBV	188	105	0.00%	0.001%
94	13.124	3754	3758	3761	rBV	438	295	0.01%	0.003%
95	13.140	3761	3763	3765	rBV	205	85	0.00%	0.001%
96	13.439	3854	3856	3861	rBV2	363	281	0.01%	0.002%
97	13.635	3916	3917	3921	rVB	409	227	0.01%	0.002%
98	13.683	3927	3932	3939	rBV3	1943	2703	0.10%	0.023%
99	14.050	4044	4046	4050	rBV	422	276	0.01%	0.002%
100	14.403	4154	4156	4157	rBV	341	120	0.00%	0.001%




Sum of corrected areas: 11738411

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034586.D
Acq On : 13 Mar 2024 19:39
Operator : SY/MD
Sample : P1739-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

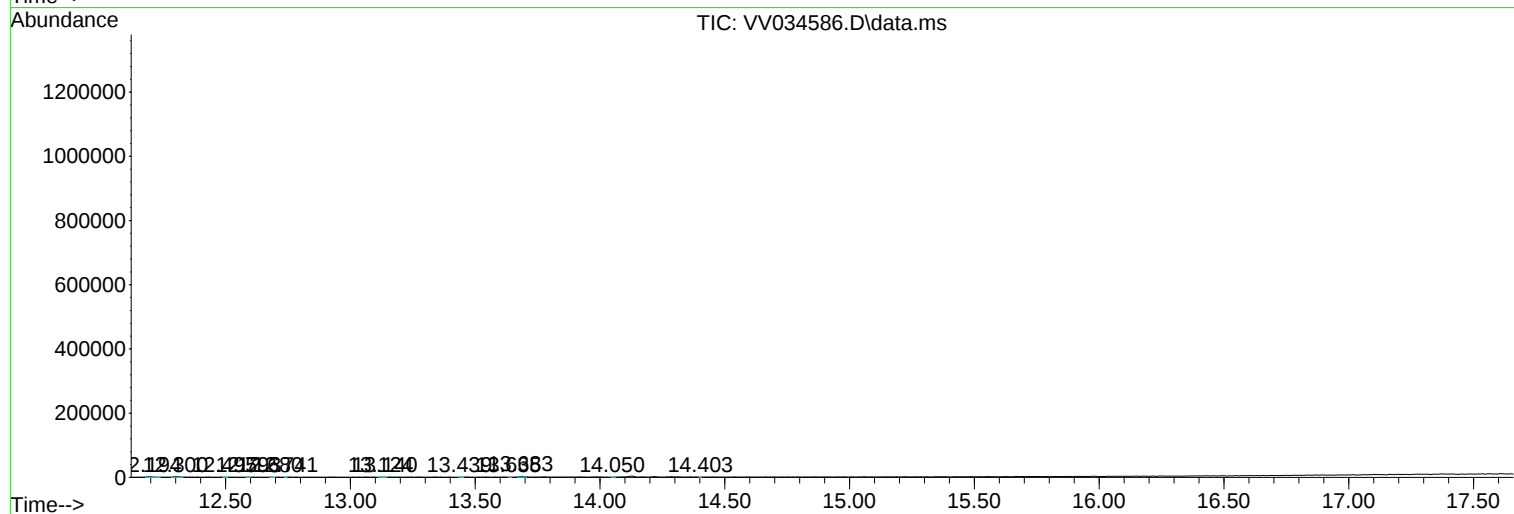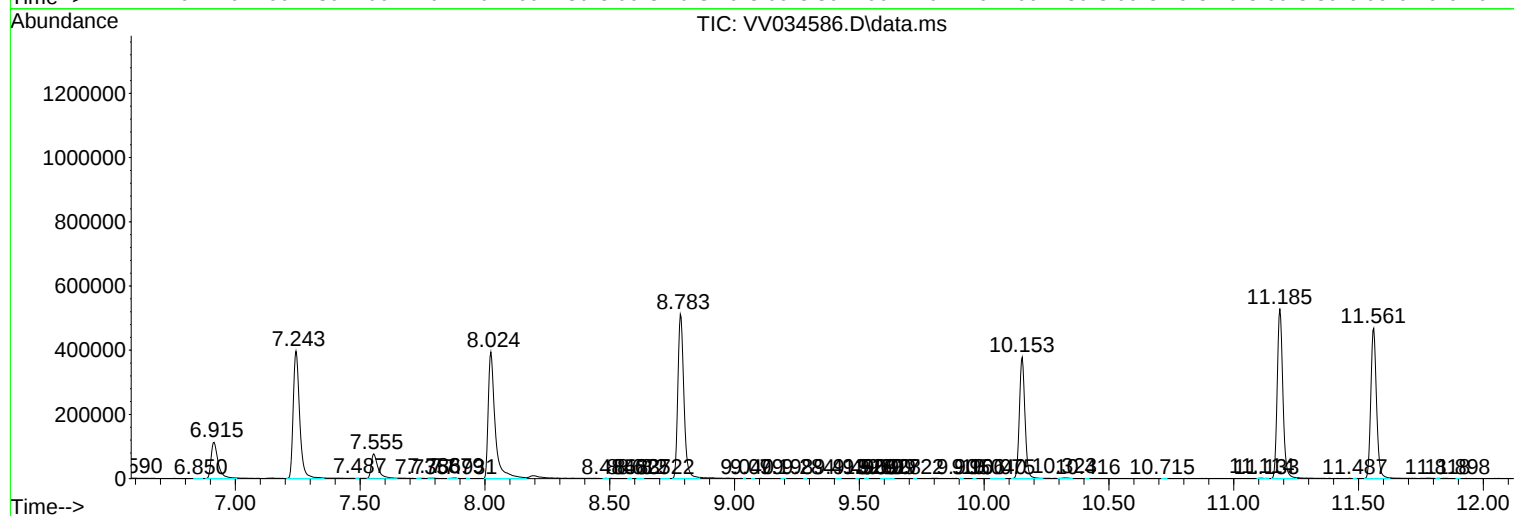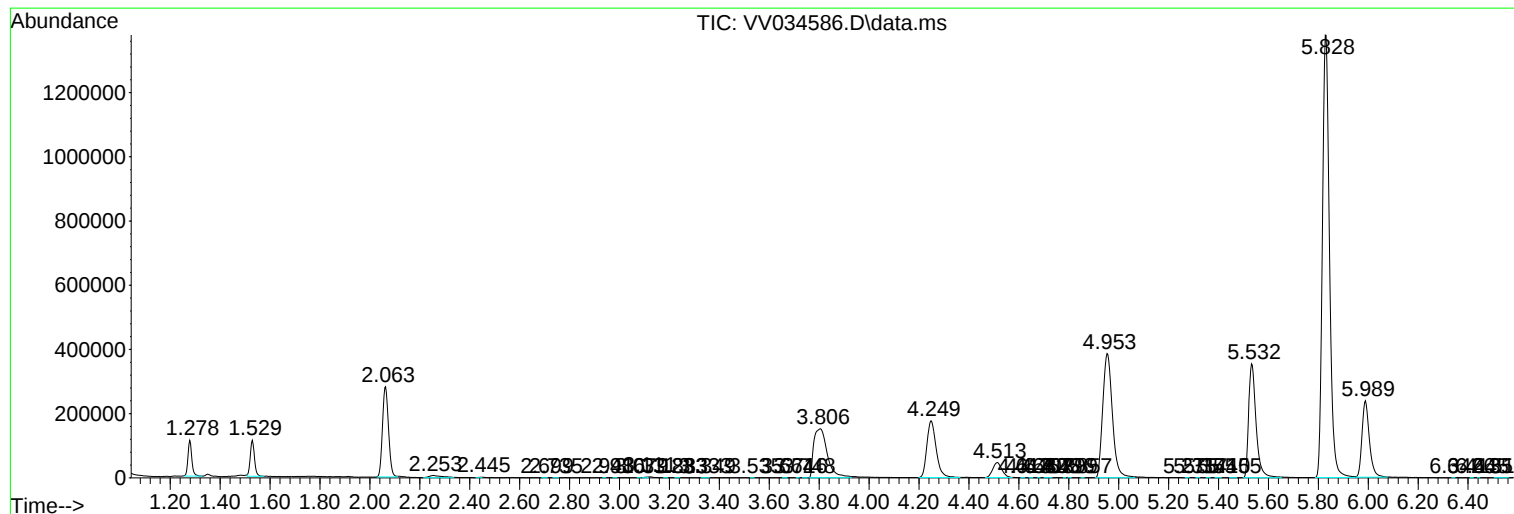

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034586.D
Acq On : 13 Mar 2024 19:39
Operator : SY/MD
Sample : P1739-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034586.D
Acq On : 13 Mar 2024 19:39
Operator : SY/MD
Sample : P1739-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------