
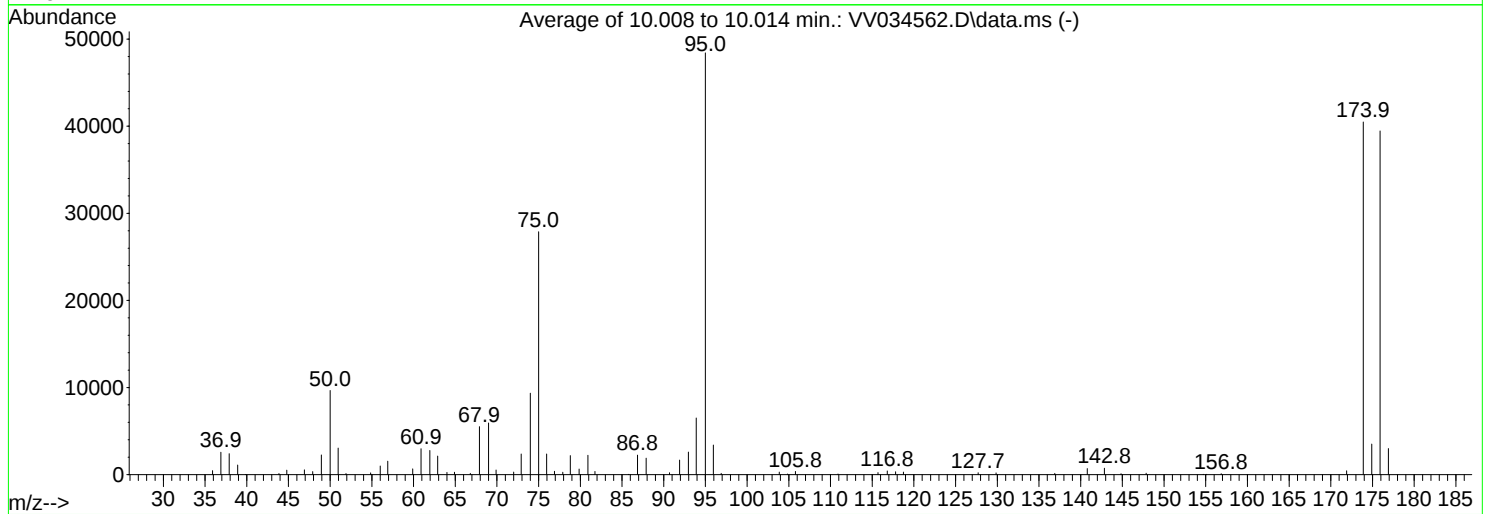


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034562.D
Acq On : 13 Mar 2024 09:06
Operator : SY/MD
Sample : BFB267
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB267

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis
Last Update : Sat Mar 16 00:58:04 2024

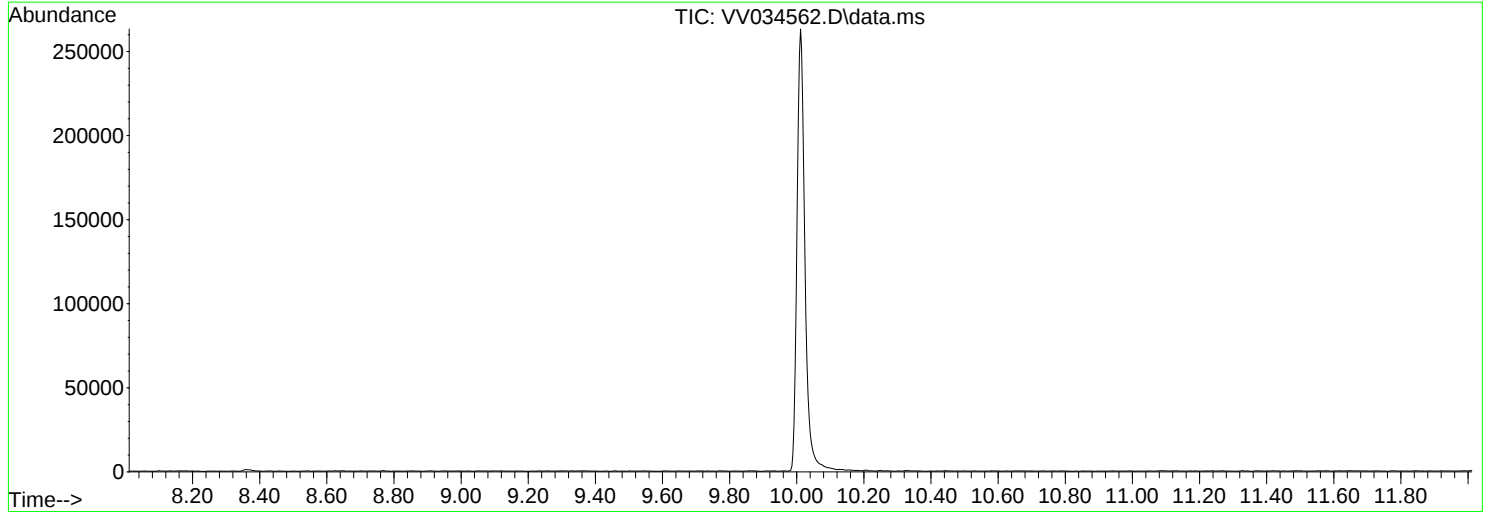

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	9657	PASS
75	95	30	80	57.6	27883	PASS
95	95	100	100	100.0	48421	PASS
96	95	5	9	7.0	3402	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.6	40475	PASS
175	174	5	9	8.7	3506	PASS
176	174	95	105	97.5	39461	PASS
177	176	5	10	7.6	2995	PASS

m/z	Abundance
39.80	208.0
43.80	369.0

Instrument :
MSVOA_V
ClientSampleId :
BFB267

m/z	Abundance
35.90	459.0
36.90	2695.0
37.90	2466.0
38.90	1090.0
39.90	222.0
44.00	572.0
44.80	516.0
46.90	473.0
47.90	292.0
49.00	2196.0
50.00	9669.0
51.00	3032.0
51.90	136.0
54.80	218.0
56.00	890.0
56.90	1523.0
59.90	676.0
60.90	3118.0
61.90	2799.0
62.90	2309.0
64.00	233.0
65.00	261.0
66.80	158.0
67.90	5369.0
69.00	5678.0
69.90	569.0
72.00	329.0
72.90	2269.0
74.00	9244.0
75.00	27440.0
75.90	2245.0
76.90	405.0
77.90	281.0
78.80	2106.0
79.90	627.0
80.90	2276.0
81.80	383.0
86.90	2198.0
87.90	1820.0
90.70	235.0
91.90	1812.0
92.90	2401.0
93.90	6749.0
95.00	46848.0
95.90	3362.0
96.90	159.0
103.80	276.0
105.80	384.0
110.90	104.0
115.70	218.0
116.80	411.0
117.80	319.0
118.70	298.0
127.70	184.0
129.90	212.0
136.90	120.0
140.80	659.0
142.90	776.0
144.90	110.0
147.80	154.0
156.80	103.0
171.90	450.0
173.90	38448.0
174.90	3511.0
175.90	37440.0
176.90	2915.0

Instrument :
MSVOA_V
ClientSampleId :
BFB267

m/z	Abundance
35.90	488.0
36.90	2655.0
37.90	2485.0
38.90	1150.0
40.00	200.0
44.00	486.0
44.80	544.0
46.90	545.0
47.90	379.0
48.90	2325.0
50.00	9928.0
50.90	3147.0
51.90	128.0
54.90	222.0
56.00	1053.0
56.90	1558.0
59.90	665.0
60.90	3110.0
62.00	2889.0
62.90	2160.0
64.00	264.0
64.90	281.0
66.80	144.0
67.90	5720.0
69.00	6234.0
69.90	542.0
72.00	312.0
72.90	2444.0
74.00	9630.0
75.00	29000.0
76.00	2470.0
76.90	412.0
77.90	290.0
78.80	2270.0
79.80	640.0
80.90	2251.0
81.70	375.0
86.90	2291.0
87.90	1944.0
90.70	217.0
91.90	1738.0
92.90	2712.0
93.90	6665.0
95.00	50104.0
96.00	3477.0
96.90	160.0
103.90	293.0
104.80	117.0
105.80	395.0
110.90	110.0
115.70	258.0
116.80	444.0
117.80	347.0
118.80	312.0
127.70	220.0
129.90	202.0
136.90	149.0
140.80	734.0
142.90	730.0
144.80	106.0
147.90	180.0
155.10	105.0
156.90	108.0
171.90	451.0
173.90	41808.0
174.90	3569.0
175.90	40944.0
176.90	3119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB267

m/z	Abundance
35.90	435.0
36.90	2384.0
37.90	2293.0
38.90	1048.0
40.00	232.0
43.80	408.0
44.80	486.0
46.90	639.0
47.90	396.0
48.90	2242.0
50.00	9373.0
50.90	2967.0
51.90	123.0
54.90	191.0
56.00	1053.0
56.90	1536.0
59.90	623.0
60.90	2677.0
61.90	2638.0
62.90	1939.0
64.00	284.0
64.80	271.0
66.80	143.0
67.90	5443.0
69.00	5901.0
69.90	490.0
72.00	252.0
72.90	2400.0
74.00	9166.0
75.00	27208.0
76.00	2396.0
76.90	335.0
77.90	243.0
78.80	2203.0
79.80	640.0
80.90	2124.0
81.80	355.0
85.80	114.0
86.80	2252.0
87.90	1934.0
90.70	184.0
91.90	1482.0
93.00	2634.0
93.90	6072.0
95.00	48312.0
96.00	3368.0
96.90	146.0
103.90	300.0
104.90	108.0
105.80	305.0
115.70	270.0
116.80	430.0
117.80	306.0
118.80	280.0
127.70	232.0
129.80	177.0
136.90	154.0
140.80	694.0
142.80	677.0
144.80	103.0
147.90	173.0
154.70	103.0
156.90	121.0
171.90	426.0
173.90	41168.0
174.90	3438.0
175.90	40000.0
176.90	2951.0

Instrument :
MSVOA_V
ClientSampleId :
BFB267