

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031422\
 Data File : VV024983.D
 Acq On : 14 Mar 2022 13:27
 Operator : SY/MD
 Sample : N1880-17
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	97	rVB	206372	209400	15.33%	1.940%
2	1.571	157	165	184	rVB	165469	186433	13.65%	1.727%
3	2.047	309	313	314	rBV3	465	291	0.02%	0.003%
4	2.111	322	333	374	rVB2	342556	531285	38.91%	4.923%
5	2.294	388	390	393	rVB2	352	233	0.02%	0.002%
6	2.355	402	409	411	rBV2	270	302	0.02%	0.003%
7	2.510	453	457	462	rVB2	850	753	0.06%	0.007%
8	2.590	478	482	488	rVB2	414	357	0.03%	0.003%
9	2.629	488	494	497	rBV	176	195	0.01%	0.002%
10	2.732	522	526	534	rVB2	294	378	0.03%	0.004%
11	2.770	534	538	540	rBV	324	225	0.02%	0.002%
12	2.802	545	548	554	rVB2	262	240	0.02%	0.002%
13	2.847	554	562	567	rBV2	296	375	0.03%	0.003%
14	3.198	665	671	673	rBV2	443	397	0.03%	0.004%
15	3.268	686	693	696	rBV2	288	339	0.02%	0.003%
16	3.539	772	777	782	rVB2	215	262	0.02%	0.002%
17	3.847	861	873	877	rBV2	225	405	0.03%	0.004%
18	3.899	877	889	934	rBV	84864	316815	23.20%	2.935%
19	4.227	988	991	997	rVB3	423	314	0.02%	0.003%
20	4.349	1012	1029	1058	rBV	219593	539382	39.50%	4.998%
21	4.609	1097	1110	1129	rVB2	5268	13214	0.97%	0.122%
22	5.047	1227	1246	1288	rBV2	531542	1365586	100.00%	12.653%
23	5.207	1294	1296	1300	rBV3	301	206	0.02%	0.002%
24	5.368	1343	1346	1349	rVB	343	211	0.02%	0.002%
25	5.400	1349	1356	1357	rBV2	399	478	0.04%	0.004%
26	5.558	1397	1405	1408	rBV2	249	286	0.02%	0.003%
27	5.616	1408	1423	1457	rBV	358173	710215	52.01%	6.580%
28	5.911	1501	1515	1547	rBV2	451388	913838	66.92%	8.467%
29	6.069	1551	1564	1587	rBV	301731	602307	44.11%	5.581%
30	6.207	1603	1607	1608	rBV3	271	207	0.02%	0.002%
31	6.252	1619	1621	1625	rVB2	341	209	0.02%	0.002%
32	6.278	1626	1629	1633	rVB3	331	207	0.02%	0.002%
33	6.513	1696	1702	1706	rVB2	291	251	0.02%	0.002%
34	6.696	1754	1759	1761	rBV3	281	217	0.02%	0.002%
35	6.738	1768	1772	1777	rBV2	173	212	0.02%	0.002%
36	6.928	1827	1831	1834	rBV	214	190	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031422\
 Data File : VV024983.D
 Acq On : 14 Mar 2022 13:27
 Operator : SY/MD
 Sample : N1880-17
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.985	1838	1849	1871	rBV	161745	290333	21.26%	2.690%
38	7.108	1885	1887	1897	rVB3	557	618	0.05%	0.006%
39	7.188	1909	1912	1916	rBV2	497	421	0.03%	0.004%
40	7.313	1938	1951	1971	rBV	626167	1090603	79.86%	10.105%
41	7.503	2008	2010	2017	rVV3	319	302	0.02%	0.003%
42	7.622	2036	2047	2076	rBV	106247	184522	13.51%	1.710%
43	7.841	2111	2115	2120	rVB2	279	252	0.02%	0.002%
44	7.892	2125	2131	2134	rBV	297	291	0.02%	0.003%
45	7.944	2140	2147	2152	rVV2	309	496	0.04%	0.005%
46	8.088	2182	2192	2235	rVV	304687	591489	43.31%	5.480%
47	8.320	2262	2264	2270	rVB2	349	316	0.02%	0.003%
48	8.612	2350	2355	2365	rVB4	614	1046	0.08%	0.010%
49	8.664	2365	2371	2374	rBV2	189	199	0.01%	0.002%
50	8.760	2396	2401	2403	rBV	208	201	0.01%	0.002%
51	8.850	2418	2429	2457	rBV	545976	883687	64.71%	8.188%
52	9.075	2496	2499	2502	rBV2	255	219	0.02%	0.002%
53	9.117	2507	2512	2516	rBV3	267	276	0.02%	0.003%
54	9.149	2516	2522	2526	rBV2	559	636	0.05%	0.006%
55	9.252	2549	2554	2557	rBV2	195	204	0.01%	0.002%
56	9.297	2562	2568	2572	rBV2	166	225	0.02%	0.002%
57	9.551	2640	2647	2651	rBV2	322	393	0.03%	0.004%
58	9.860	2739	2743	2748	rBV2	240	269	0.02%	0.002%
59	9.908	2754	2758	2764	rVB	317	280	0.02%	0.003%
60	9.937	2764	2767	2772	rBV	272	201	0.01%	0.002%
61	10.124	2818	2825	2834	rBV4	2708	4181	0.31%	0.039%
62	10.214	2841	2853	2876	rBV	386736	595913	43.64%	5.521%
63	10.410	2910	2914	2920	rVB2	289	280	0.02%	0.003%
64	10.455	2924	2928	2932	rBV2	276	263	0.02%	0.002%
65	10.474	2932	2934	2939	rVB	333	190	0.01%	0.002%
66	10.548	2953	2957	2960	rVB	299	239	0.02%	0.002%
67	10.577	2960	2966	2971	rBV2	1140	1306	0.10%	0.012%
68	10.815	3037	3040	3044	rVB2	286	207	0.02%	0.002%
69	10.837	3044	3047	3049	rBV	275	192	0.01%	0.002%
70	10.914	3063	3071	3080	rBV4	2083	3082	0.23%	0.029%
71	11.030	3100	3107	3108	rBV2	217	254	0.02%	0.002%
72	11.149	3136	3144	3150	rVV4	1356	1830	0.13%	0.017%
73	11.246	3163	3174	3196	rBV	553299	831107	60.86%	7.701%
74	11.384	3213	3217	3218	rBV3	515	393	0.03%	0.004%
75	11.426	3223	3230	3239	rVB4	1876	2758	0.20%	0.026%
76	11.496	3250	3252	3260	rVB2	265	237	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031422\
 Data File : VV024983.D
 Acq On : 14 Mar 2022 13:27
 Operator : SY/MD
 Sample : N1880-17
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

77	11.541	3260	3266	3268	rBV2	419	328	0.02%	0.003%
78	11.622	3279	3291	3312	rVV	588620	899433	65.86%	8.334%
79	11.786	3338	3342	3348	rVB3	726	842	0.06%	0.008%
80	11.847	3357	3361	3366	rVB3	442	421	0.03%	0.004%
81	11.953	3391	3394	3402	rVB2	218	263	0.02%	0.002%
82	12.242	3482	3484	3490	rVB3	196	217	0.02%	0.002%
83	12.545	3574	3578	3581	rBV2	252	235	0.02%	0.002%
84	12.580	3586	3589	3594	rVV2	340	374	0.03%	0.003%
85	12.625	3598	3603	3607	rVB	283	276	0.02%	0.003%
86	12.840	3664	3670	3675	rBV2	374	494	0.04%	0.005%
87	12.869	3675	3679	3681	rVV	311	261	0.02%	0.002%
88	12.992	3714	3717	3721	rBV2	304	214	0.02%	0.002%
89	13.156	3763	3768	3773	rBV	264	347	0.03%	0.003%
90	13.262	3797	3801	3807	rBV2	215	274	0.02%	0.003%
91	13.500	3872	3875	3878	rVB2	355	227	0.02%	0.002%
92	13.519	3878	3881	3885	rBV2	284	272	0.02%	0.003%
93	13.699	3934	3937	3941	rBV2	272	323	0.02%	0.003%
94	13.766	3956	3958	3963	rVB3	317	196	0.01%	0.002%
95	13.811	3968	3972	3975	rBV2	332	248	0.02%	0.002%
96	13.876	3990	3992	3998	rVB2	341	286	0.02%	0.003%
97	13.908	3998	4002	4004	rBV2	301	226	0.02%	0.002%
98	14.323	4128	4131	4134	rBV3	244	191	0.01%	0.002%
99	14.493	4181	4184	4189	rBV2	344	361	0.03%	0.003%
100	16.146	4694	4698	4701	rVB3	574	445	0.03%	0.004%


Sum of corrected areas: 10792880

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031422\
Data File : VV024983.D
Acq On : 14 Mar 2022 13:27
Operator : SY/MD
Sample : N1880-17
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CODE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

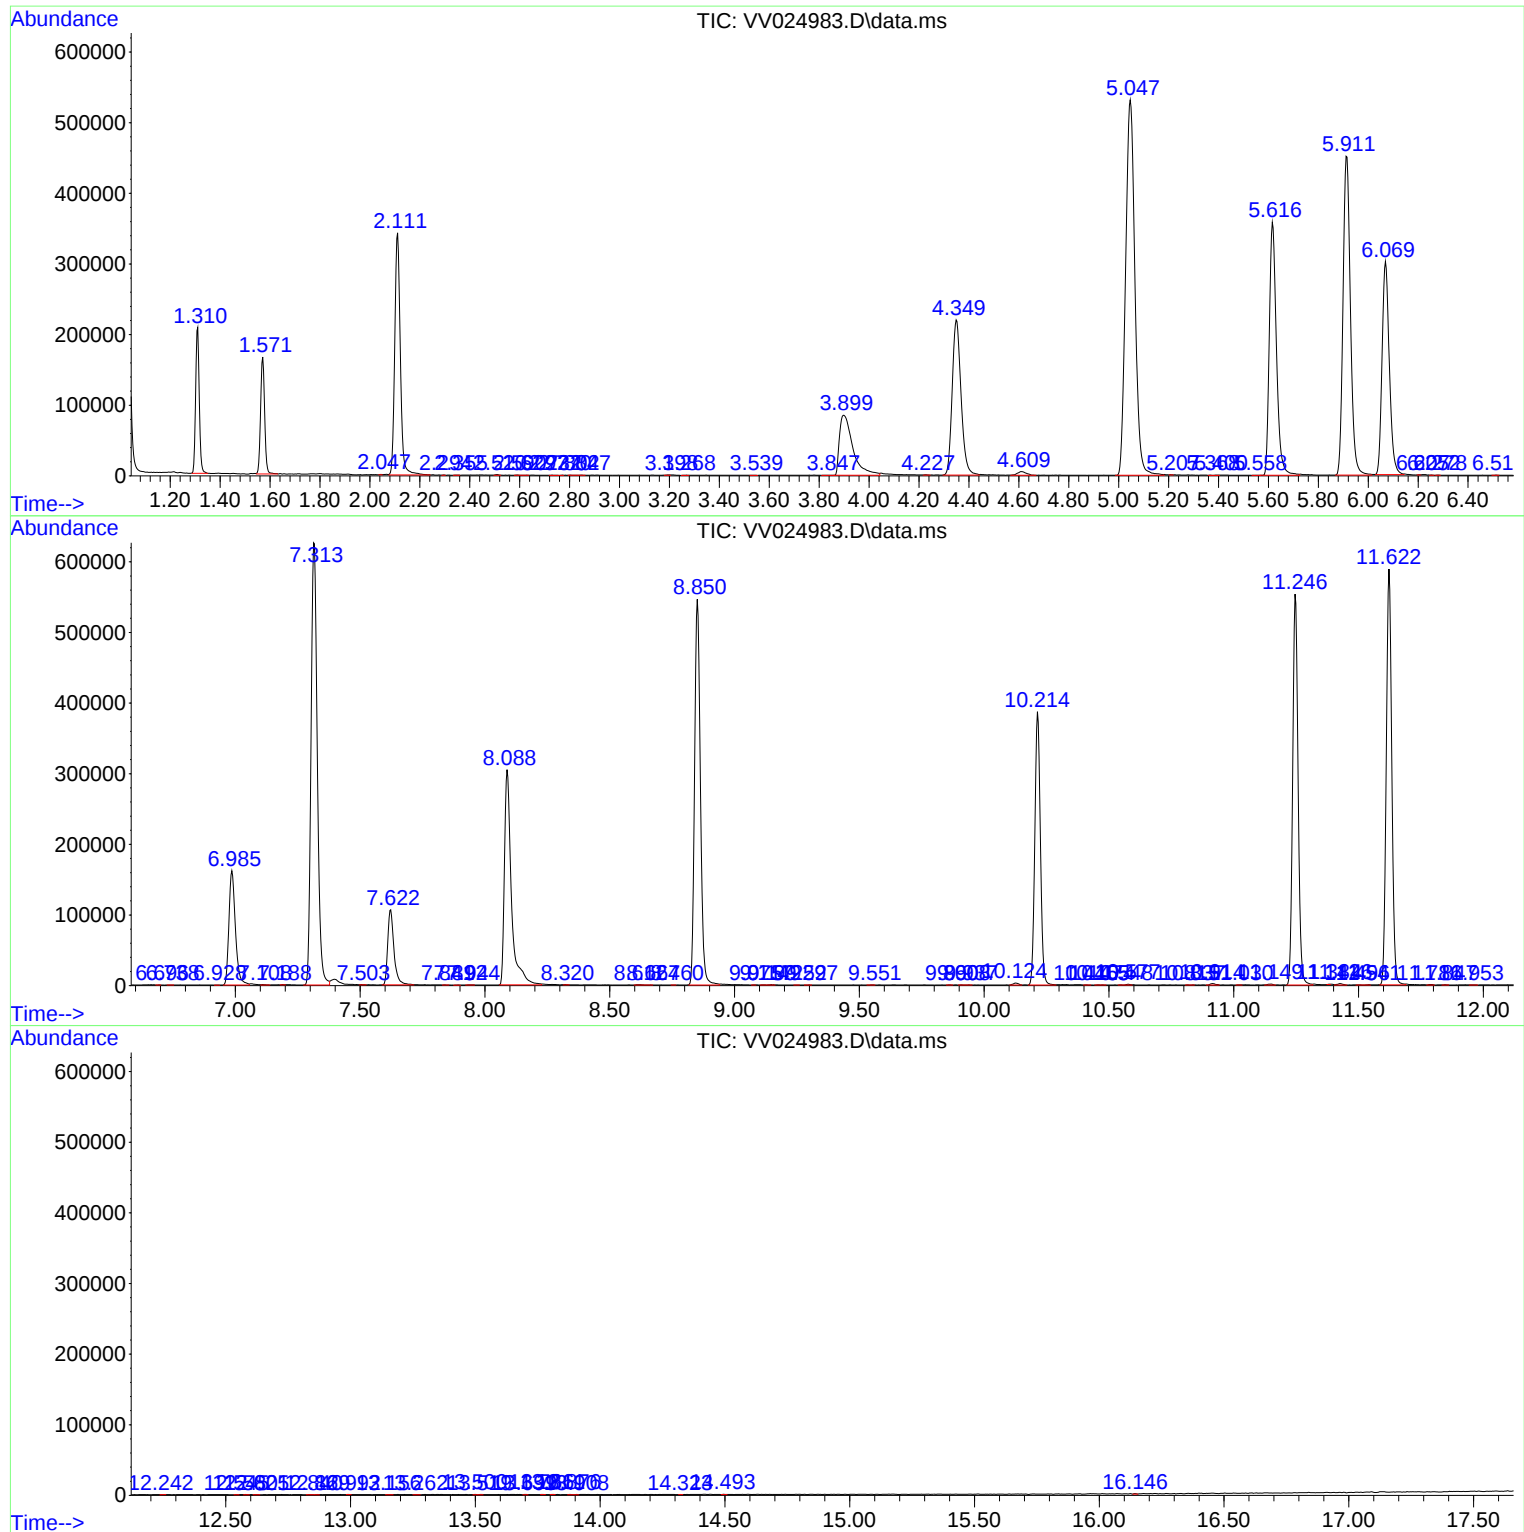

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031422\
Data File : VV024983.D
Acq On : 14 Mar 2022 13:27
Operator : SY/MD
Sample : N1880-17
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CODE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031422\
Data File : VV024983.D
Acq On : 14 Mar 2022 13:27
Operator : SY/MD
Sample : N1880-17
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------