


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031422\
 Data File : VV024975.D
 Acq On : 14 Mar 2022 09:01
 Operator : SY/MD
 Sample : BFB205
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB205

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis
 Last Update : Tue Mar 15 02:18:50 2022

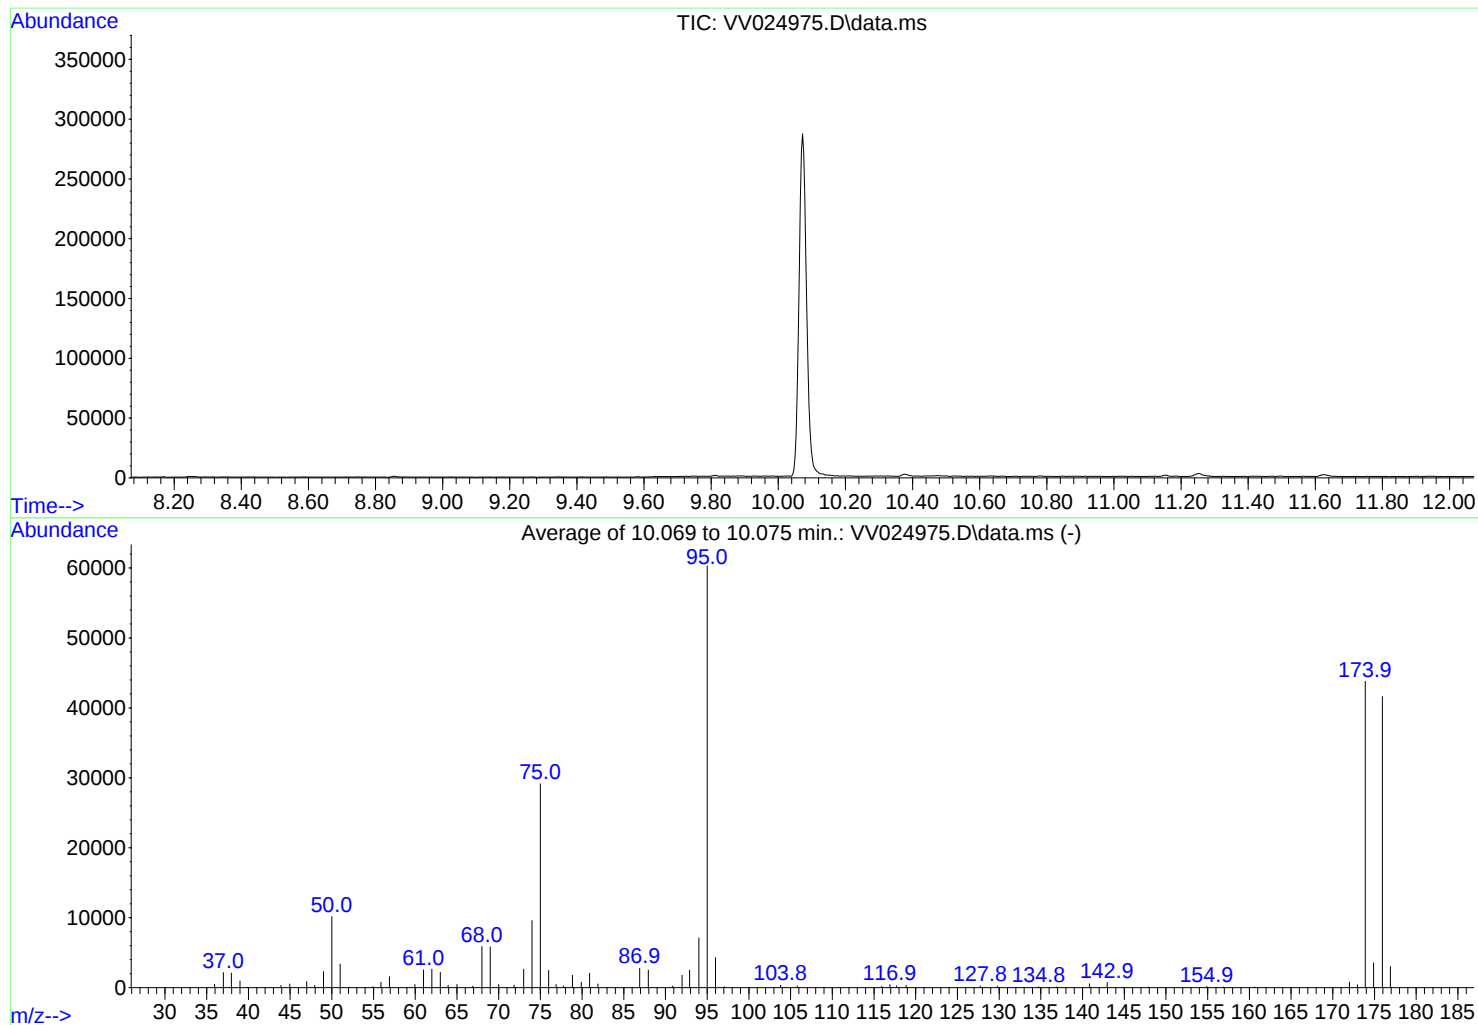

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	10163	PASS
75	95	30	80	48.3	29155	PASS
95	95	100	100	100.0	60312	PASS
96	95	5	9	7.1	4275	PASS
173	174	0.00	2	1.0	421	PASS
174	95	50	120	72.6	43784	PASS
175	174	5	9	8.1	3541	PASS
176	174	95	105	95.0	41616	PASS
177	176	5	10	7.3	3021	PASS

m/z	Abundance
36.00	549.0
37.90	240.0
39.90	493.0
43.90	246.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	1100.0
37.00	2139.0
38.00	2376.0
39.00	943.0
39.90	527.0
43.90	529.0
44.90	548.0
47.00	933.0
48.00	308.0
49.00	2274.0
50.00	10266.0
51.00	3434.0
55.00	173.0
55.90	782.0
56.90	1594.0
59.90	460.0
61.00	2505.0
62.00	2688.0
63.00	2078.0
63.90	364.0
65.00	414.0
66.90	217.0
68.00	5753.0
69.00	5743.0
70.00	478.0
71.80	364.0
73.00	2646.0
74.00	9600.0
75.00	29200.0
76.00	2591.0
76.90	456.0
77.80	269.0
78.80	1724.0
79.90	691.0
80.90	2077.0
81.90	495.0
86.90	2629.0
88.00	2429.0
90.90	248.0
92.00	1693.0
92.90	2473.0
94.00	7139.0
95.00	59784.0
96.00	4280.0
97.10	133.0
103.80	312.0
105.80	224.0
116.00	217.0
116.90	446.0
117.70	242.0
118.90	371.0
127.80	259.0
129.80	183.0
134.80	128.0
136.80	128.0
140.90	537.0
143.00	660.0
144.80	146.0
154.90	115.0
172.00	701.0
172.90	404.0
173.90	42200.0
174.90	3372.0
176.00	40136.0
176.90	2965.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
35.90	1038.0
37.00	2266.0
38.00	2413.0
39.00	983.0
40.00	555.0
43.90	573.0
45.00	535.0
47.00	954.0
47.90	344.0
49.00	2392.0
50.00	10511.0
51.00	3543.0
52.10	115.0
55.00	171.0
55.90	802.0
56.90	1612.0
59.90	458.0
61.00	2647.0
62.00	2661.0
63.00	2281.0
63.90	359.0
65.00	476.0
66.90	204.0
68.00	6131.0
69.00	6025.0
70.00	443.0
71.80	353.0
73.00	2714.0
74.00	9846.0
75.00	29952.0
76.00	2514.0
76.90	493.0
77.70	261.0
78.90	1801.0
79.90	805.0
80.90	2120.0
81.90	561.0
86.90	2856.0
87.90	2552.0
90.90	231.0
92.00	1836.0
92.90	2634.0
94.00	7399.0
95.00	62424.0
96.00	4419.0
97.00	147.0
103.80	353.0
105.80	259.0
116.00	218.0
116.90	456.0
117.70	262.0
118.80	348.0
127.70	247.0
129.80	222.0
134.80	132.0
136.80	128.0
140.80	542.0
142.90	743.0
145.00	150.0
147.90	117.0
154.90	181.0
156.90	128.0
160.60	126.0
172.00	812.0
172.90	437.0
173.90	45440.0
174.90	3715.0
175.90	43136.0
176.90	3169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
35.00	947.0
37.00	2074.0
38.00	2212.0
39.00	906.0
40.00	567.0
43.00	589.0
45.00	475.0
47.00	755.0
47.00	331.0
49.00	2197.0
50.00	9713.0
51.00	3145.0
52.00	133.0
54.00	130.0
55.00	797.0
56.00	1475.0
60.00	428.0
61.00	2470.0
62.00	2518.0
63.00	2139.0
64.00	303.0
65.00	516.0
66.00	173.0
68.00	5789.0
69.00	5715.0
70.00	425.0
71.00	351.0
73.00	2536.0
74.00	9285.0
75.00	28312.0
76.00	2312.0
76.00	453.0
77.00	243.0
78.00	225.0
78.00	1743.0
79.00	819.0
80.00	1975.0
81.00	544.0
86.00	122.0
86.00	2799.0
87.00	2544.0
90.00	202.0
92.00	1760.0
92.00	2384.0
94.00	6829.0
95.00	58728.0
96.00	4125.0
97.00	150.0
103.00	349.0
105.00	251.0
115.00	217.0
116.00	392.0
117.00	254.0
118.00	310.0
127.00	217.0
129.00	249.0
134.00	122.0
136.00	108.0
140.00	556.0
141.00	109.0
142.00	785.0
145.00	150.0
147.00	147.0
154.00	195.0
156.00	123.0
160.00	139.0
172.00	793.0
173.00	423.0
173.00	43712.0
174.00	3536.0
175.00	41576.0
176.00	2930.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205