
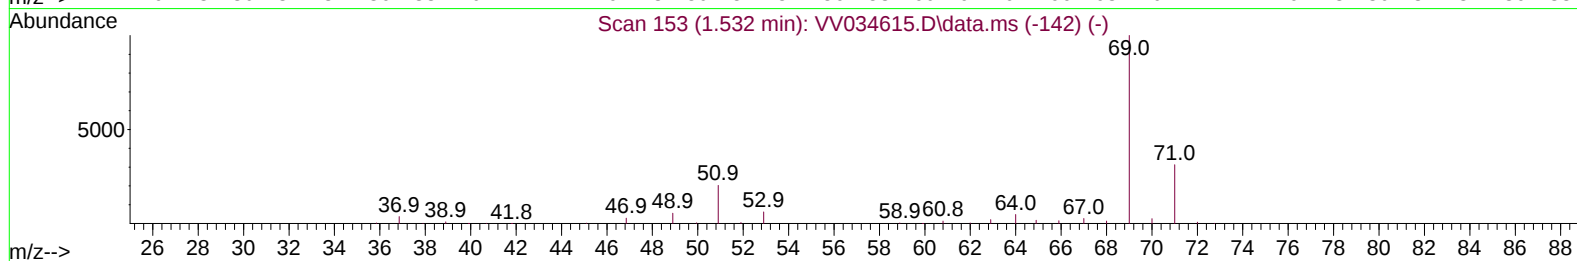
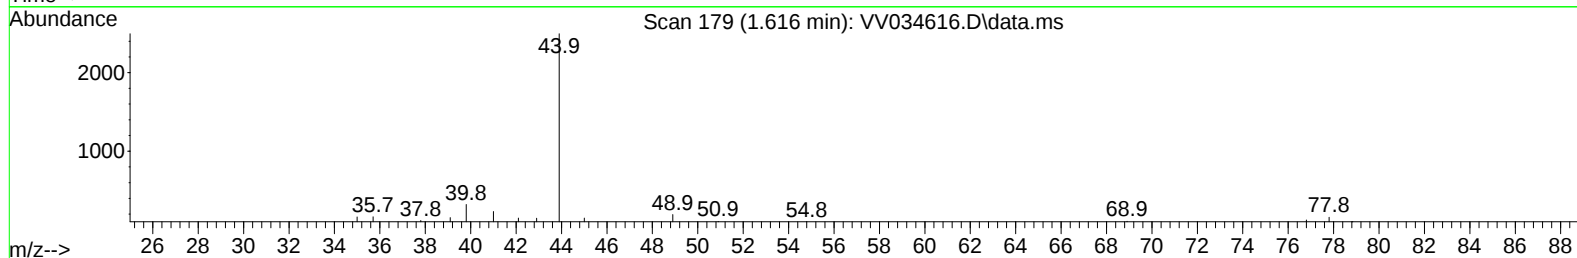


Data Path : Z:\voasrv\HPCHEM1\MSV0A_V\Data\VV031424\
Data File : VV034616.D
Acq On : 14 Mar 2024 20:38
Operator : SY/MD
Sample : VV0314WBL02
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Mar 15 06:40:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSV0A_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 06:40:01 2024
Response via : Initial Calibration

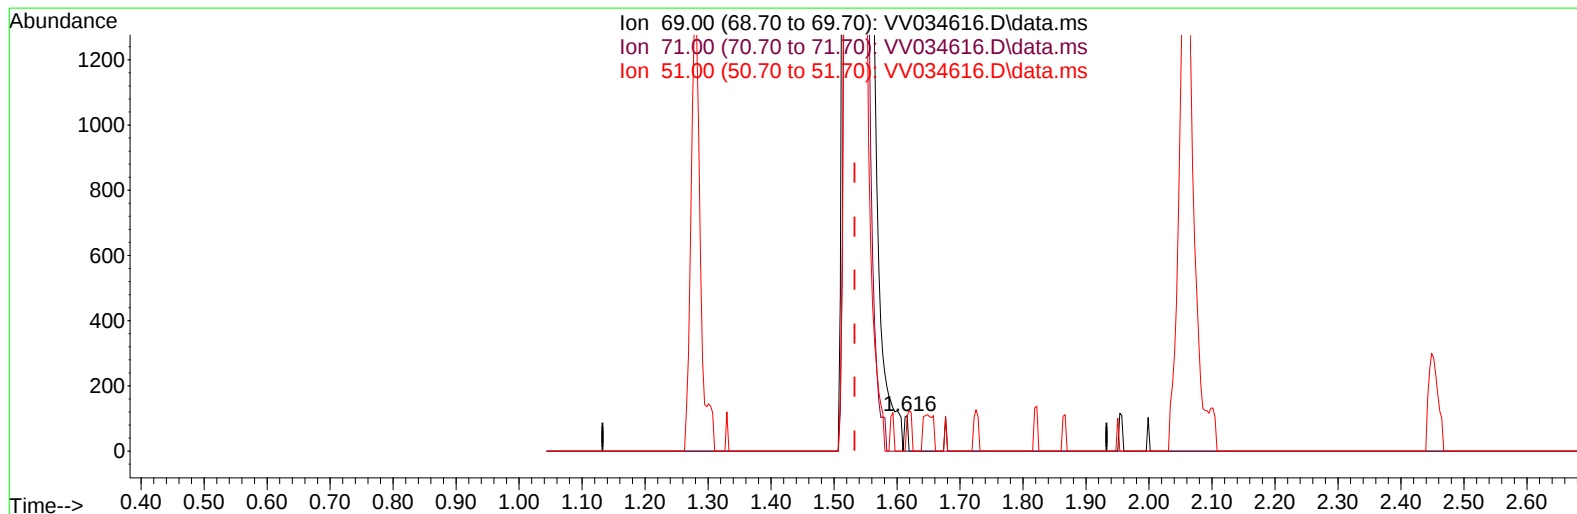

TIC: VV034616.D\data.ms

(7) Chloroethane-d5 (S)

1.616min (+ 0.084) 0.02 ug/L

response 41

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.00#
51.00	28.90	163.41#
0.00	0.00	0.00