

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034592.D
 Acq On : 14 Mar 2024 10:40
 Operator : SY/MD
 Sample : P1739-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 15 03:34:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 15 03:33:21 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	307651	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	288143	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	133676	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	134141	50.296	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery	= 100.600%		
7) Chloroethane-d5	1.529	69	111147	53.493	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery	= 106.980%		
11) 1,1-Dichloroethene-d2	2.056	65	61538	51.020	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery	= 102.040%		
21) 2-Butanone-d5	3.786	46	172983	96.989	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery	= 96.990%		
24) Chloroform-d	4.243	84	242700	51.468	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	= 102.940%		
26) 1,2-Dichloroethane-d4	4.937	65	163417	53.032	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	= 106.060%		
32) Benzene-d6	4.957	84	476322	54.773	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	= 109.540%		
36) 1,2-Dichloropropane-d6	5.985	67	145262	54.735	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery	= 109.460%		
41) Toluene-d8	7.239	98	418173	53.137	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery	= 106.280%		
43) trans-1,3-Dichloroprop...	7.551	79	65415	49.084	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery	= 98.160%		
47) 2-Hexanone-d5	8.021	63	127111	95.915	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery	= 95.910%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	178876	51.217	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery	= 102.440%		
66) 1,2-Dichlorobenzene-d4	11.558	152	149200	54.604	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery	= 109.200%		
Target Compounds						Qvalue
35) Methylcyclohexane	5.985	83	35151	9.095	ug/L #	18
61) 1,2,3-Trichloropropane	11.185	75	16796	6.582	ug/L #	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034592.D
Acq On : 14 Mar 2024 10:40
Operator : SY/MD
Sample : P1739-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 15 03:34:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 03:33:21 2024
Response via : Initial Calibration




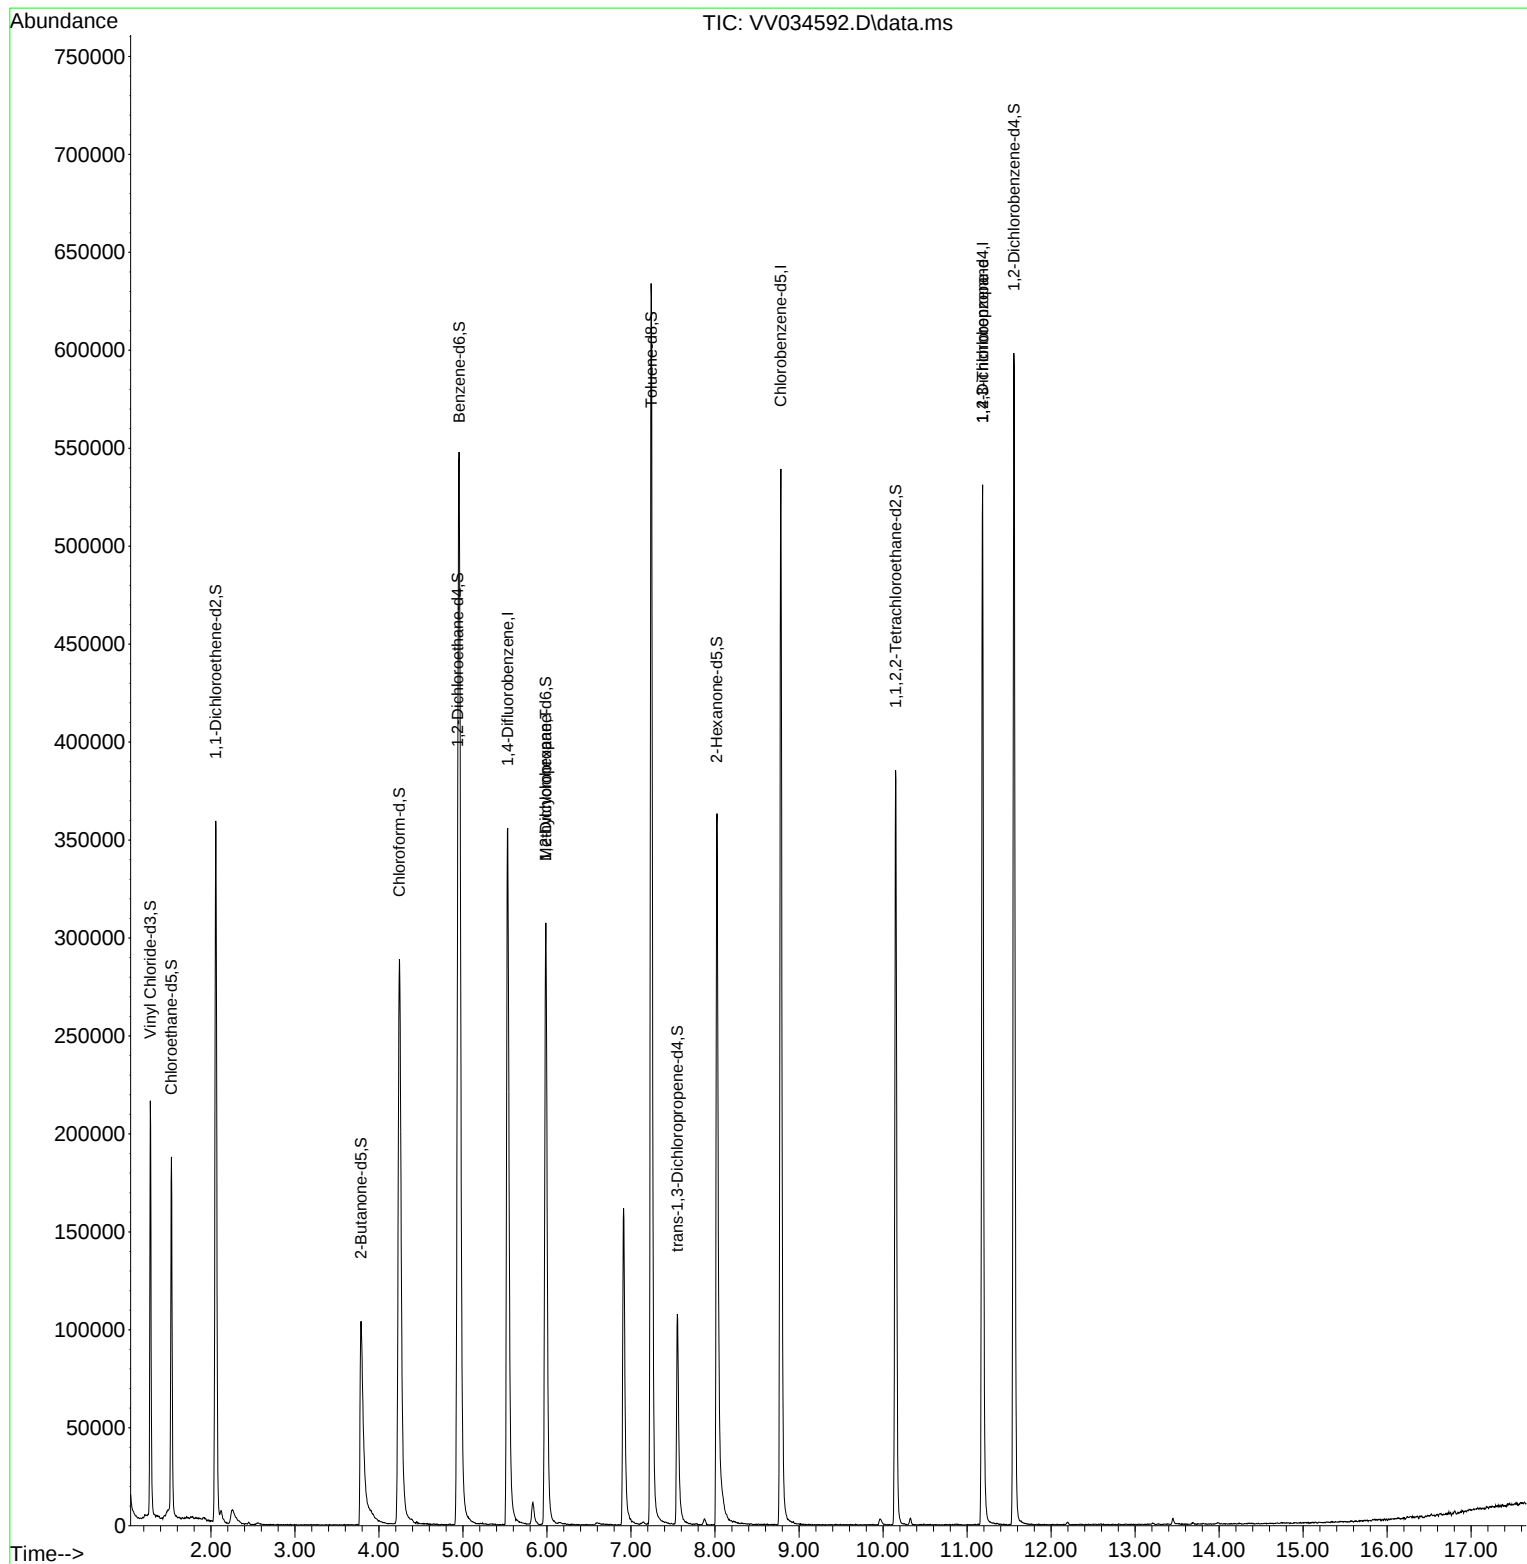


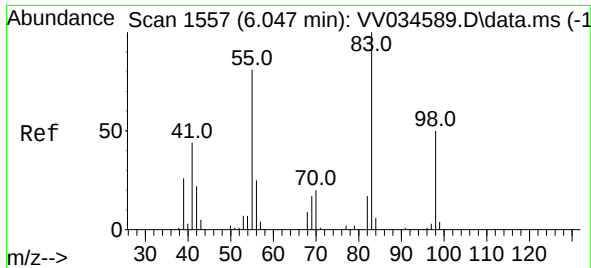

#35
Methylcyclohexane
Concen: 9.095 ug/L
RT: 5.985 min Scan# 1
Delta R.T. -0.061 min
Lab File: VV034592.D
Acq: 14 Mar 2024 10:40

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 83 Resp: 35151
Ion Ratio Lower Upper
83 100
55 0.0 62.6 94.0#
98 1.6 39.5 59.3#

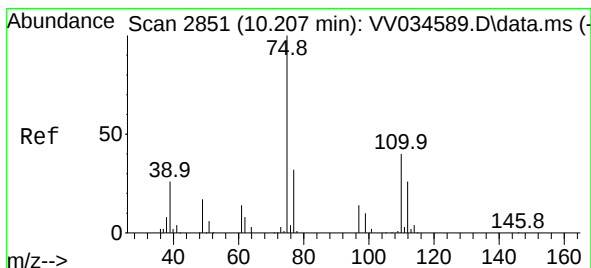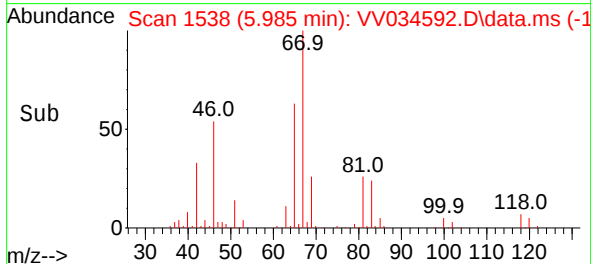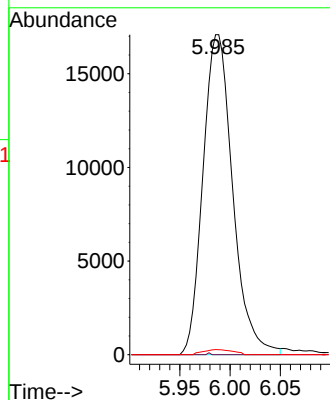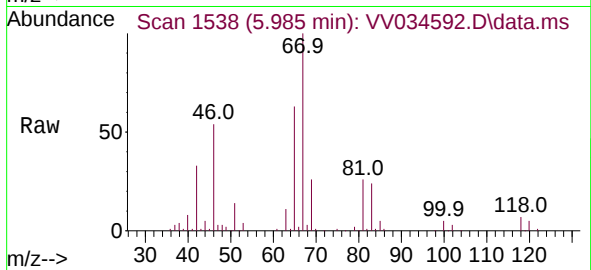

#61
1,2,3-Trichloropropane
Concen: 6.582 ug/L
RT: 11.185 min Scan# 3155
Delta R.T. 0.978 min
Lab File: VV034592.D
Acq: 14 Mar 2024 10:40

Tgt Ion: 75 Resp: 16796
Ion Ratio Lower Upper
75 100
77 37.6 25.9 38.9
110 3.1 33.1 49.7#

