

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034613.D
 Acq On : 14 Mar 2024 19:02
 Operator : SY/MD
 Sample : P1751-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 15 03:39:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 15 03:33:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	285587	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	270055	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	127048	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	110613	44.679	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.360%
7) Chloroethane-d5	1.532	69	93176	48.308	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.620%
11) 1,1-Dichloroethene-d2	2.060	65	50046	44.698	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.400%
21) 2-Butanone-d5	3.799	46	165660	100.059	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.060%
24) Chloroform-d	4.249	84	209444	47.847	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.700%
26) 1,2-Dichloroethane-d4	4.940	65	143151	50.044	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.080%
32) Benzene-d6	4.960	84	407619	50.013	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.020%
36) 1,2-Dichloropropane-d6	5.989	67	127734	51.354	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.700%
41) Toluene-d8	7.243	98	353578	47.938	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.880%
43) trans-1,3-Dichloroprop...	7.554	79	56808	45.481	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.960%
47) 2-Hexanone-d5	8.024	63	119034	95.836	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.840%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	164012	50.106	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.220%
66) 1,2-Dichlorobenzene-d4	11.561	152	133363	51.355	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.700%
Target Compounds						
15) Methyl Acetate	2.288	43	14118	5.545	ug/L	Qvalue # 53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034613.D
Acq On : 14 Mar 2024 19:02
Operator : SY/MD
Sample : P1751-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 15 03:39:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 03:33:21 2024
Response via : Initial Calibration

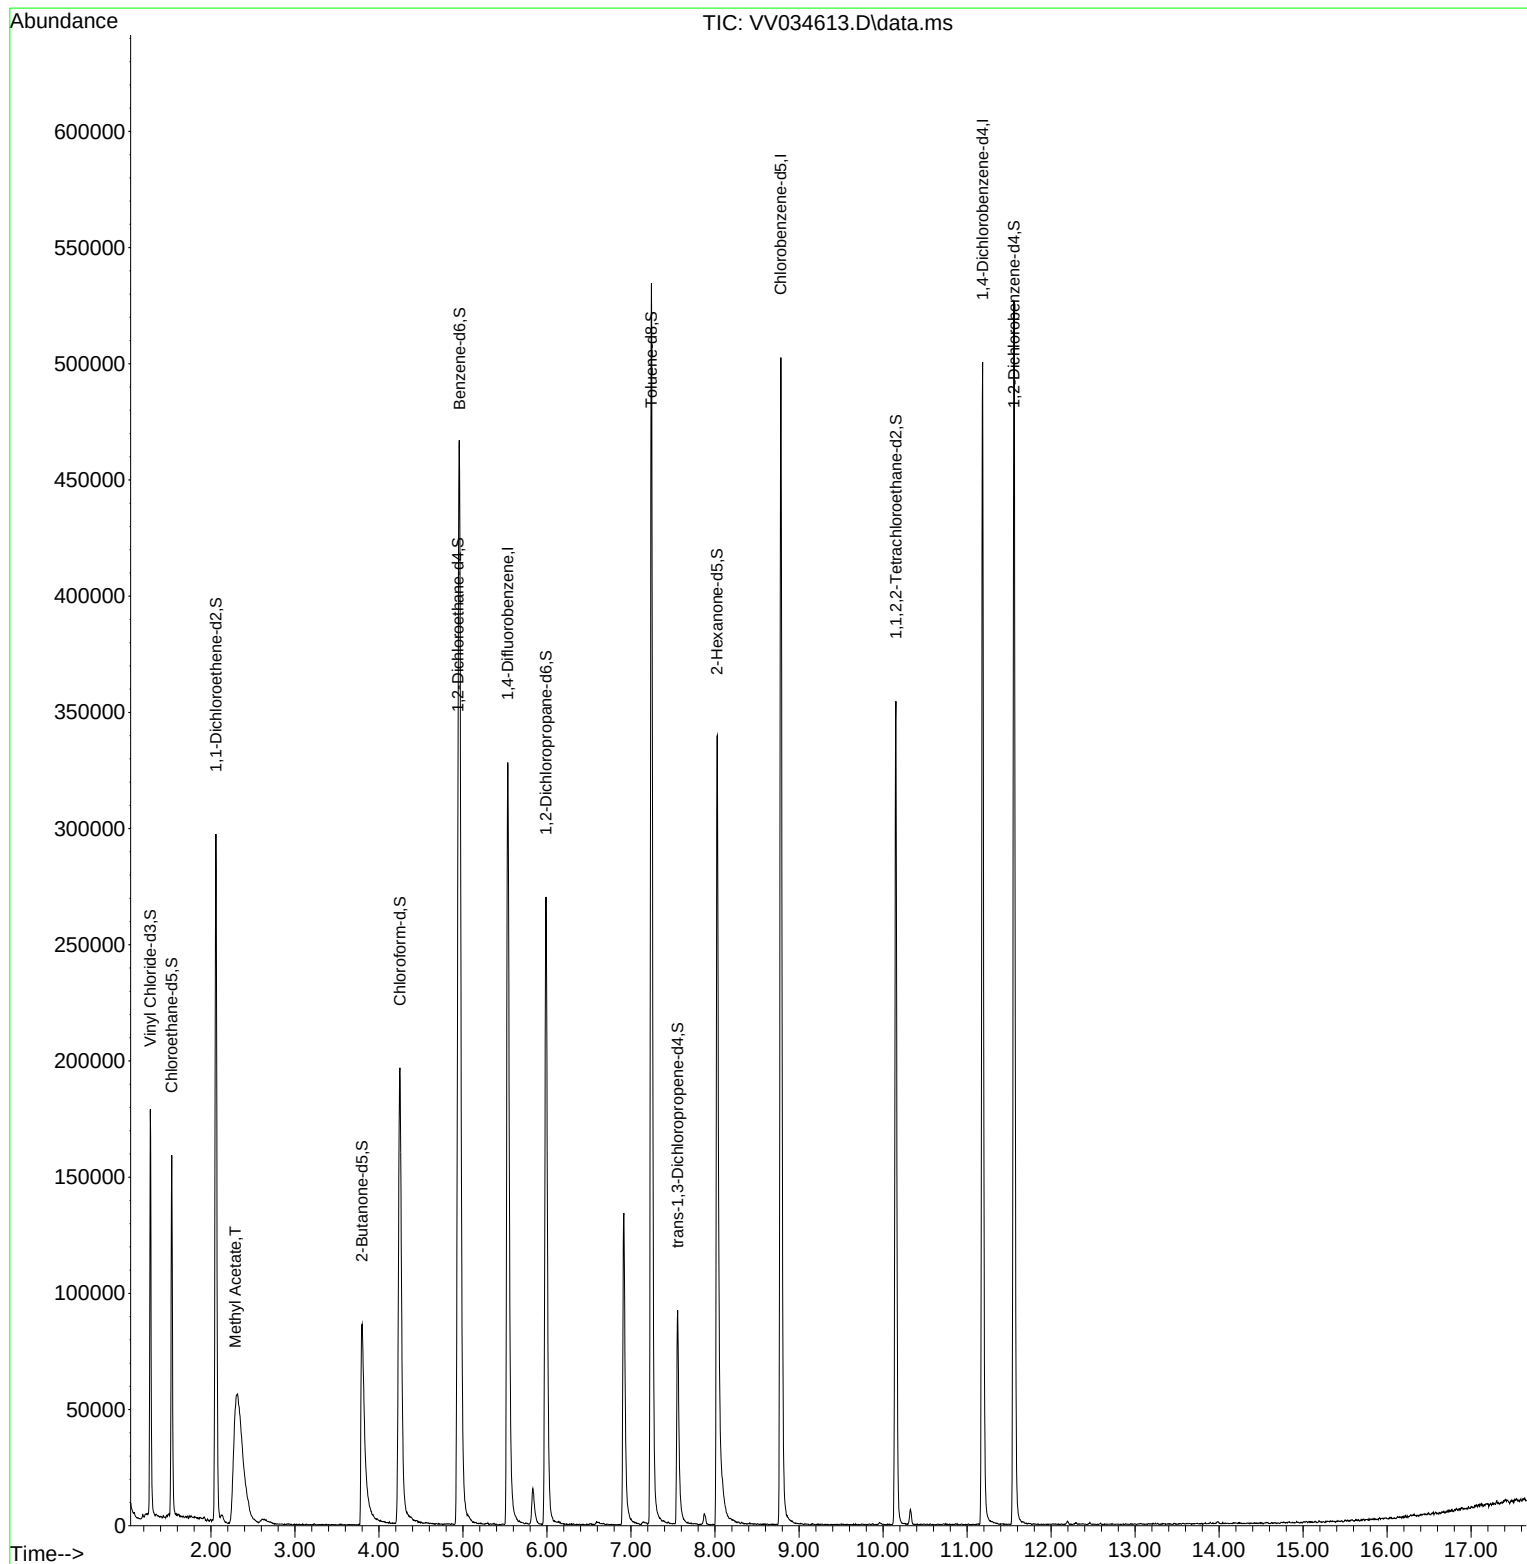

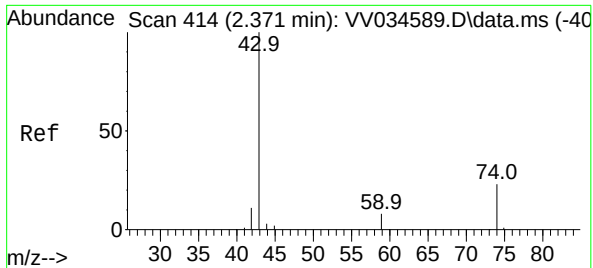

#15
Methyl Acetate
Concen: 5.545 ug/L
RT: 2.288 min Scan# 31
Delta R.T. -0.084 min
Lab File: VV034613.D
Acq: 14 Mar 2024 19:02

Instrument :
MSVOA_V
ClientSampleId :

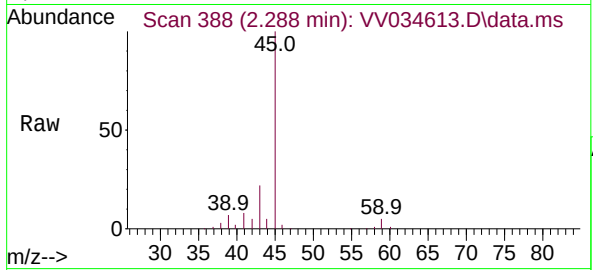

Tgt Ion: 43 Resp: 14118
Ion Ratio Lower Upper
43 100
74 0.0 17.8 26.8#

