
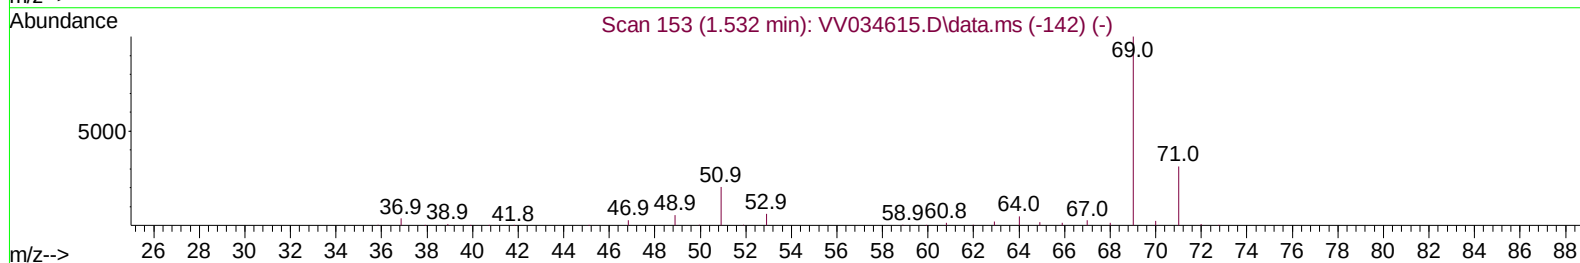
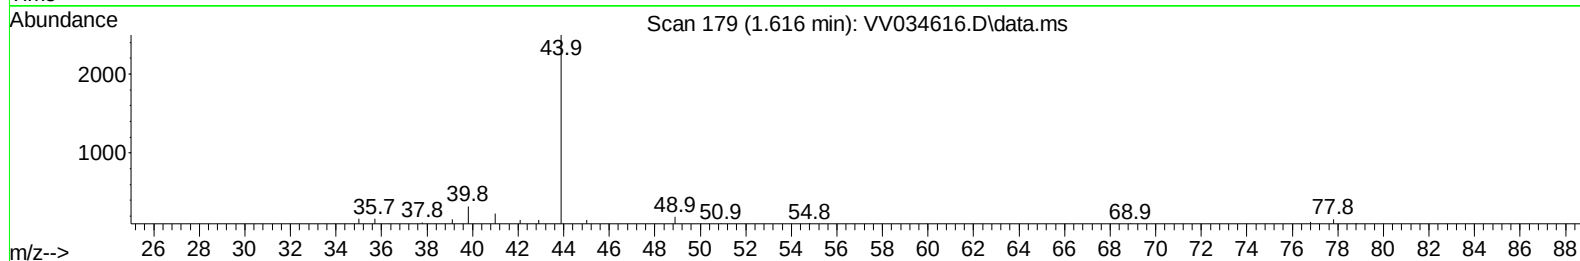


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034616.D
Acq On : 14 Mar 2024 20:38
Operator : SY/MD
Sample : VV0314WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Mar 15 06:40:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 06:40:01 2024
Response via : Initial Calibration

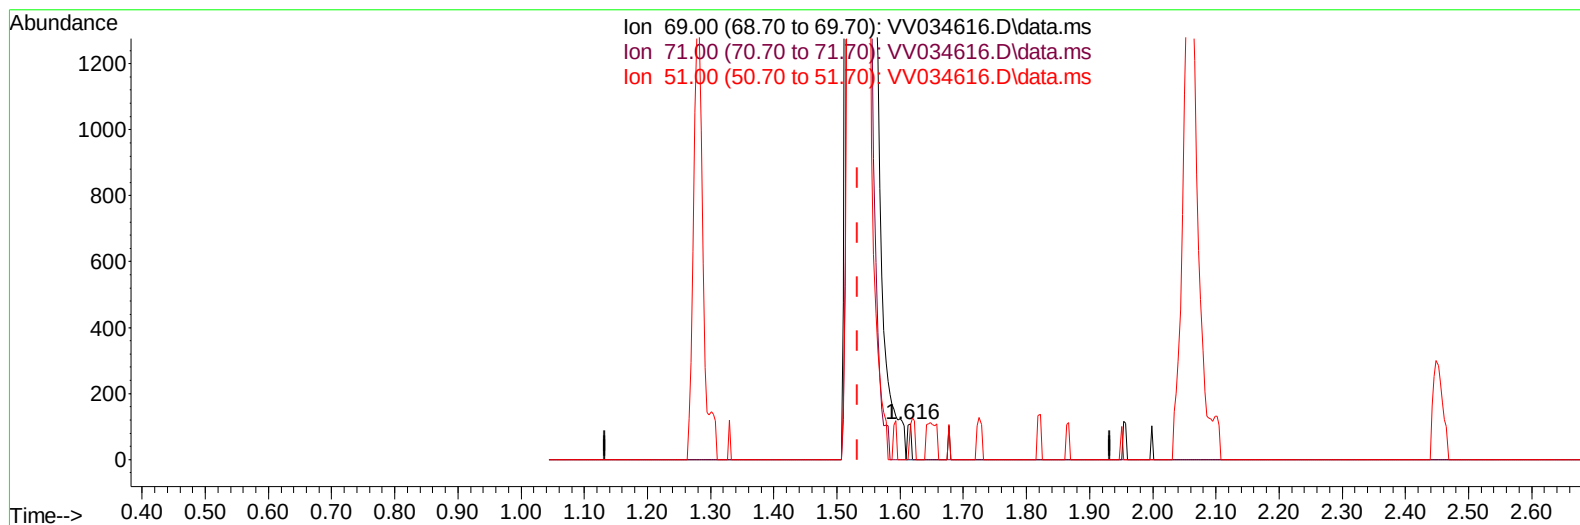




TIC: VV034616.D\data.ms

(7) Chloroethane-d5 (S)**1.616min (+ 0.084) 0.02 ug/L****response 41**

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.00#
51.00	28.90	163.41#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034616.D
Acq On : 14 Mar 2024 20:38
Operator : SY/MD
Sample : VV0314WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Mar 15 06:40:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 06:40:01 2024
Response via : Initial Calibration

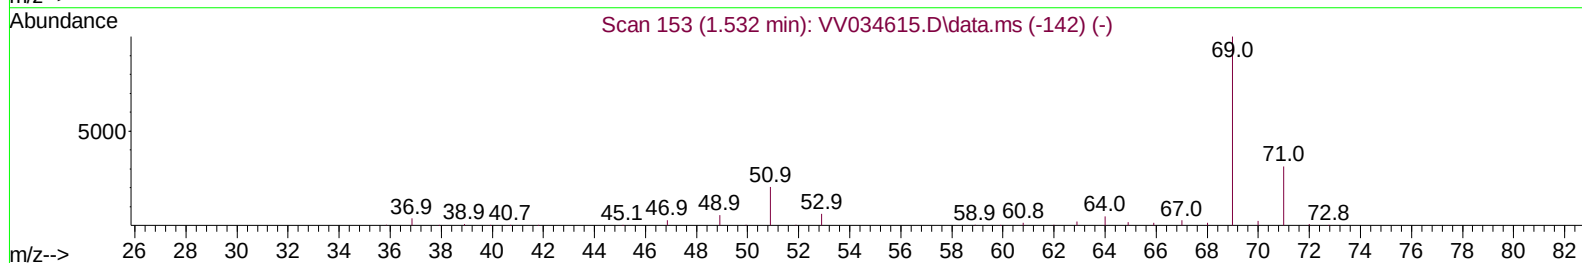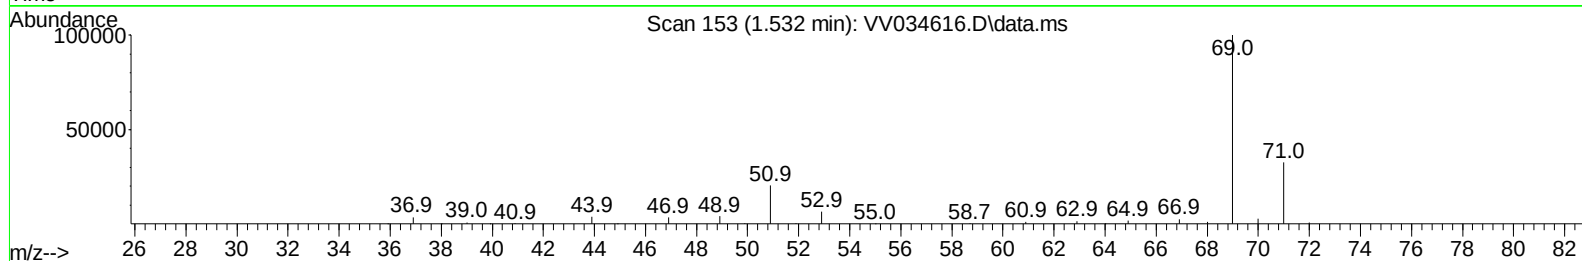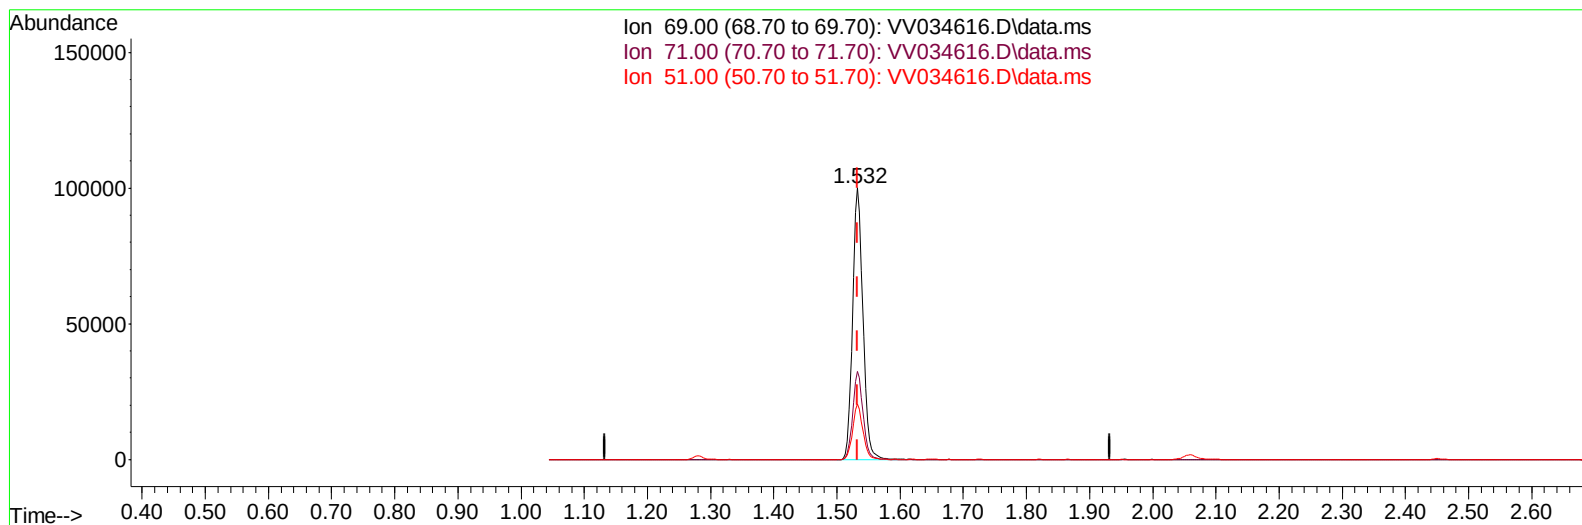

TIC: VV034616.D\data.ms

(7) Chloroethane-d5 (S)**1.532min (+ 0.000) 57.11 ug/L m****response 114205**

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.00#
51.00	28.90	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034616.D
 Acq On : 14 Mar 2024 20:38
 Operator : SY/MD
 Sample : VV0314WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Mar 15 06:40:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 15 06:40:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	296095	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	277156	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	131138	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	138641	54.012	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	108.020%	
7) Chloroethane-d5	1.532	69	114205m	57.110	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	114.220%	
11) 1,1-Dichloroethene-d2	2.056	65	60893	52.456	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	104.920%	
21) 2-Butanone-d5	3.796	46	188399	109.755	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	109.750%	
24) Chloroform-d	4.246	84	239594	52.792	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	105.580%	
26) 1,2-Dichloroethane-d4	4.941	65	163450	55.112	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	110.220%	
32) Benzene-d6	4.960	84	473972	56.664	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	113.320%	
36) 1,2-Dichloropropane-d6	5.986	67	146455	57.372	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	114.740%	
41) Toluene-d8	7.243	98	420459	55.546	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	111.100%	
43) trans-1,3-Dichloroprop...	7.555	79	62330	48.623	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	97.240%	
47) 2-Hexanone-d5	8.024	63	139437	109.386	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	109.390%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	189782	56.494	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	112.980%	
66) 1,2-Dichlorobenzene-d4	11.558	152	155119	57.869	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	115.740%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034616.D
Acq On : 14 Mar 2024 20:38
Operator : SY/MD
Sample : VV0314WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Mar 15 06:40:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 06:40:01 2024
Response via : Initial Calibration

