

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034600.D
 Acq On : 14 Mar 2024 13:51
 Operator : SY/MD
 Sample : P1739-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG9

Quant Time: Mar 15 03:36:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 15 03:33:21 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	293269	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	272944	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	132400	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	128407	50.507	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 101.020%		
7) Chloroethane-d5	1.529	69	105877	53.455	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 106.920%		
11) 1,1-Dichloroethene-d2	2.056	65	58917	51.243	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 102.480%		
21) 2-Butanone-d5	3.786	46	170694	100.399	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 100.400%		
24) Chloroform-d	4.249	84	229182	50.985	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 101.960%		
26) 1,2-Dichloroethane-d4	4.941	65	155955	53.092	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 106.180%		
32) Benzene-d6	4.960	84	450055	54.635	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 109.260%		
36) 1,2-Dichloropropane-d6	5.989	67	137281	54.608	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 109.220%		
41) Toluene-d8	7.243	98	393683	52.811	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 105.620%		
43) trans-1,3-Dichloroprop...	7.555	79	60941	48.273	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 96.540%		
47) 2-Hexanone-d5	8.024	63	123979	98.761	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 98.760%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	175930	53.178	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 106.360%		
66) 1,2-Dichlorobenzene-d4	11.561	152	147606	54.542	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 109.080%		
Target Compounds						
34) Trichloroethene	5.841	95	6753	2.804	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034600.D
Acq On : 14 Mar 2024 13:51
Operator : SY/MD
Sample : P1739-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG9


Quant Time: Mar 15 03:36:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 03:33:21 2024
Response via : Initial Calibration

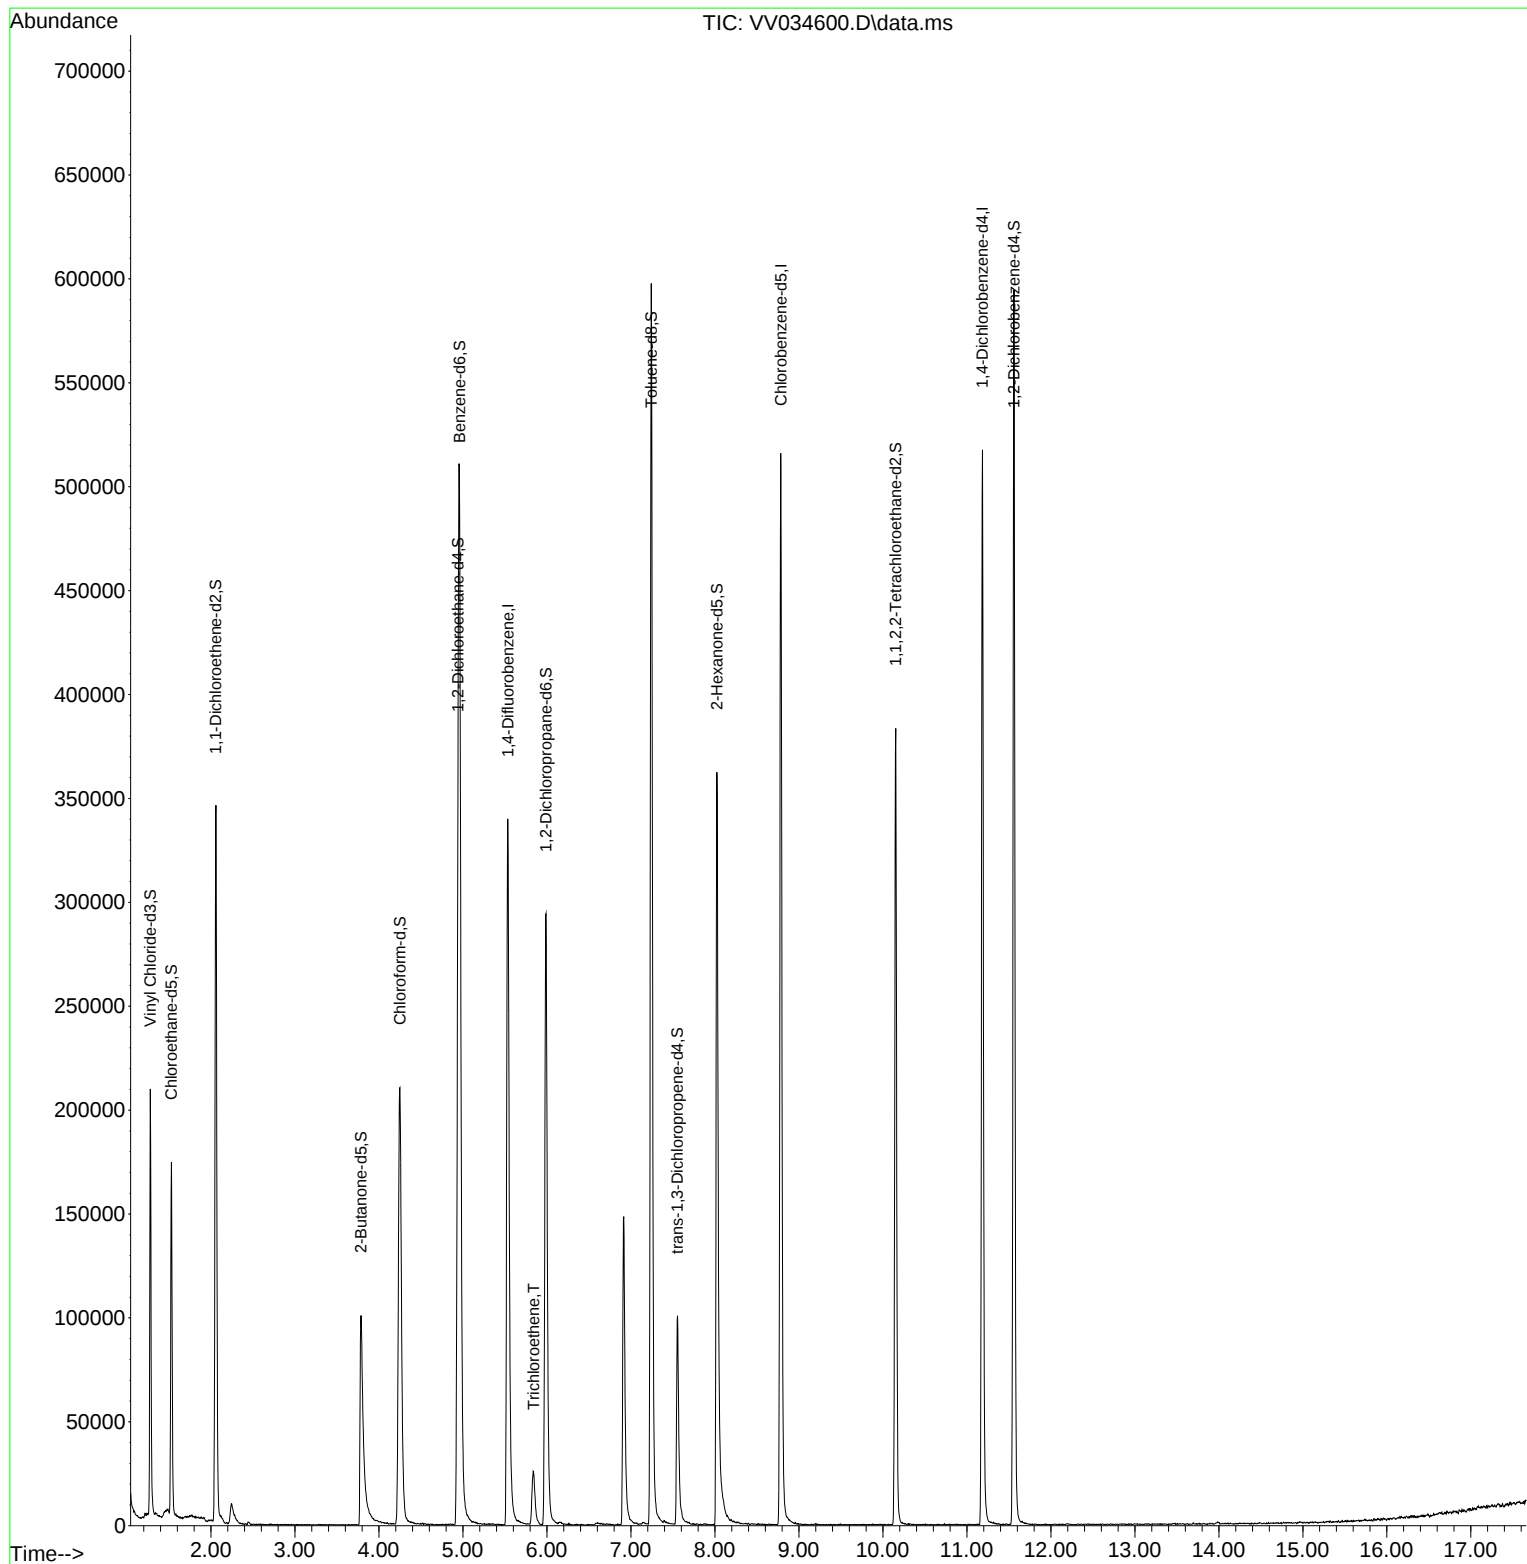

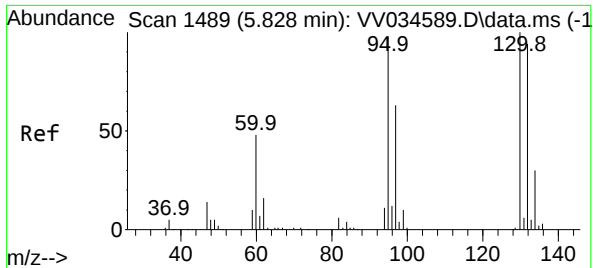

#34
 Trichloroethene
 Concen: 2.804 ug/L
 RT: 5.841 min Scan# 14
 Delta R.T. 0.013 min
 Lab File: VV034600.D
 Acq: 14 Mar 2024 13:51

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG9

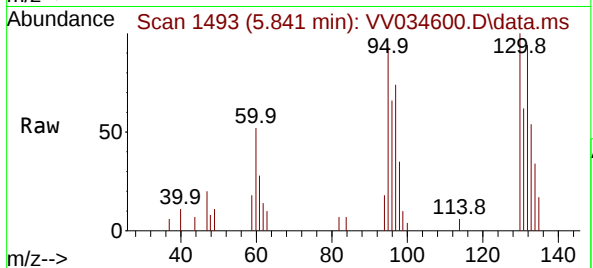

Tgt Ion: 95 Resp: 6753

Ion	Ratio	Lower	Upper
95	100		
97	79.6	44.7	83.1
132	101.4	65.3	121.3
130	107.6	69.1	128.3

