

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034604.D
 Acq On : 14 Mar 2024 15:27
 Operator : SY/MD
 Sample : P1740-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH4

Quant Time: Mar 15 03:37:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 15 03:33:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	294410	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	273208	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	133335	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	121681	47.676	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	95.360%		
7) Chloroethane-d5	1.532	69	102213	51.406	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	102.820%		
11) 1,1-Dichloroethene-d2	2.060	65	55467	48.055	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	96.100%		
21) 2-Butanone-d5	3.796	46	162849	95.413	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	95.410%		
24) Chloroform-d	4.249	84	215993	47.864	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.720%		
26) 1,2-Dichloroethane-d4	4.940	65	146652	49.731	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.460%		
32) Benzene-d6	4.960	84	429870	52.134	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.260%		
36) 1,2-Dichloropropane-d6	5.989	67	132181	52.529	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	105.060%		
41) Toluene-d8	7.243	98	375025	50.259	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.520%		
43) trans-1,3-Dichloroprop...	7.555	79	58597	46.372	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.740%		
47) 2-Hexanone-d5	8.024	63	114790	91.352	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.350%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	161218	48.684	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	97.360%		
66) 1,2-Dichlorobenzene-d4	11.558	152	139262	51.098	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.200%		
Target Compounds					Qvalue	
13) Acetone	2.134	43	9127	4.448	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034604.D
Acq On : 14 Mar 2024 15:27
Operator : SY/MD
Sample : P1740-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH4

Quant Time: Mar 15 03:37:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 03:33:21 2024
Response via : Initial Calibration

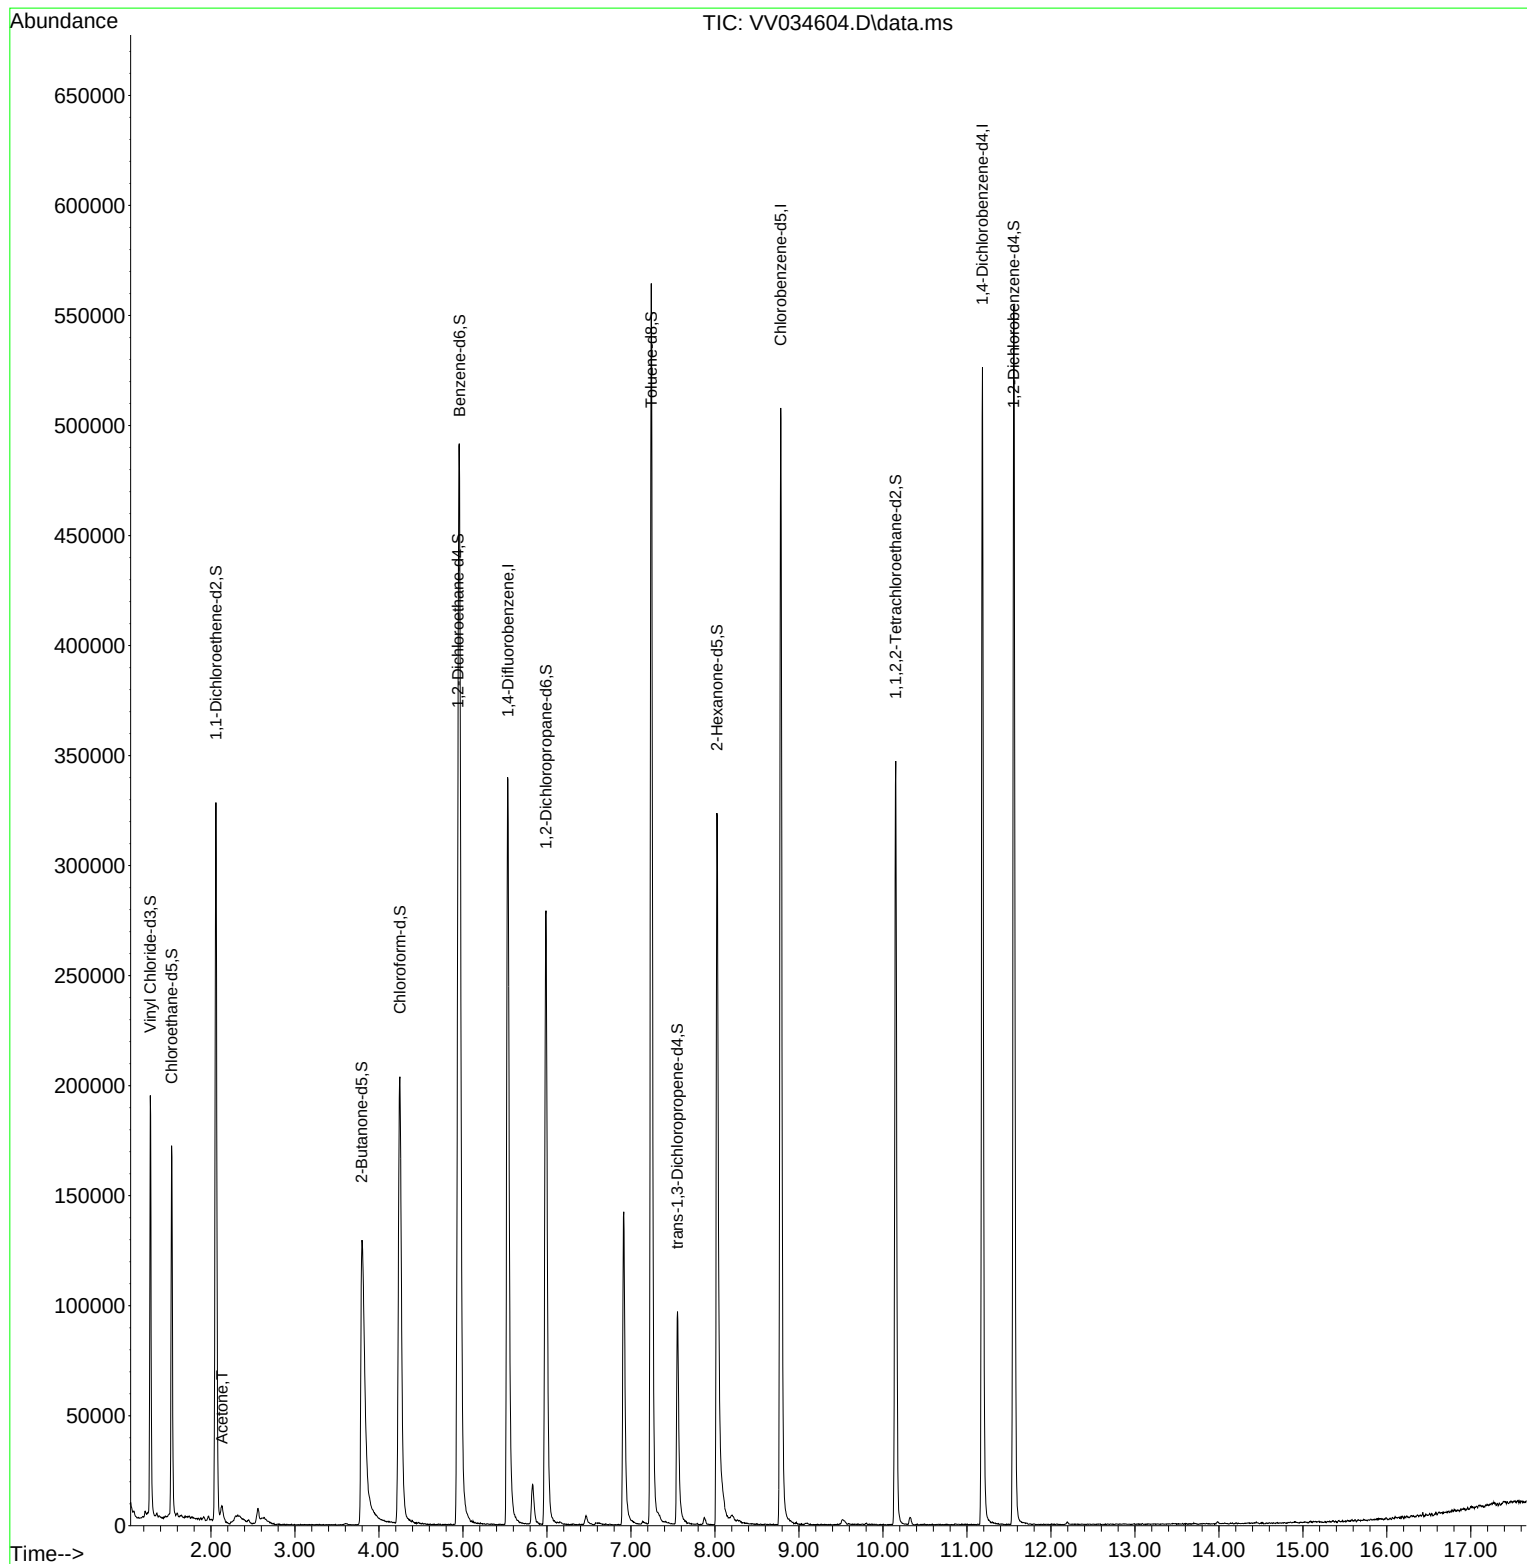

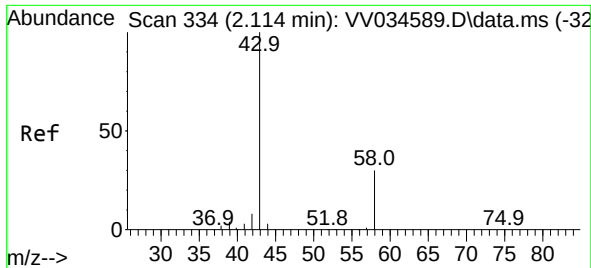

#13

Acetone

Concen: 4.448 ug/L

RT: 2.134 min Scan# 34

Delta R.T. 0.019 min

Lab File: VV034604.D


Acq: 14 Mar 2024 15:27

Instrument :

MSVOA_V

ClientSampleId :

C0GH4

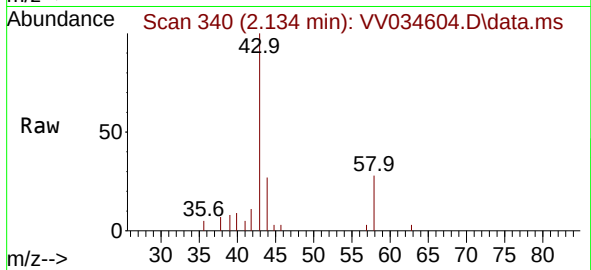

Tgt Ion: 43 Resp: 9127

Ion Ratio Lower Upper

43 100

58 32.2 0.0 57.2

