

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034625.D
 Acq On : 15 Mar 2024 00:37
 Operator : SY/MD
 Sample : P1751-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKX6

Quant Time: Mar 15 06:56:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 15 06:40:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	264925	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	250845	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	115552	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	93295	40.623	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.240%		
7) Chloroethane-d5	1.526	69	80560	45.025	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	90.040%		
11) 1,1-Dichloroethene-d2	2.056	65	43407	41.792	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.580%		
21) 2-Butanone-d5	3.789	46	172119	112.068	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	112.070%		
24) Chloroform-d	4.246	84	198440	48.869	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.740%		
26) 1,2-Dichloroethane-d4	4.940	65	141398	53.286	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	106.580%		
32) Benzene-d6	4.956	84	380933	50.318	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.640%		
36) 1,2-Dichloropropane-d6	5.989	67	121396	52.543	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	105.080%		
41) Toluene-d8	7.243	98	325859	47.564	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.120%		
43) trans-1,3-Dichloroprop...	7.554	79	53384	46.013	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.020%		
47) 2-Hexanone-d5	8.024	63	117955	102.240	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	102.240%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84	168674	55.477	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	110.960%		
66) 1,2-Dichlorobenzene-d4	11.561	152	122431	51.835	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.680%		
Target Compounds					Qvalue	
13) Acetone	2.117	43	401703	217.568	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034625.D
Acq On : 15 Mar 2024 00:37
Operator : SY/MD
Sample : P1751-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKX6

Quant Time: Mar 15 06:56:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 06:40:01 2024
Response via : Initial Calibration

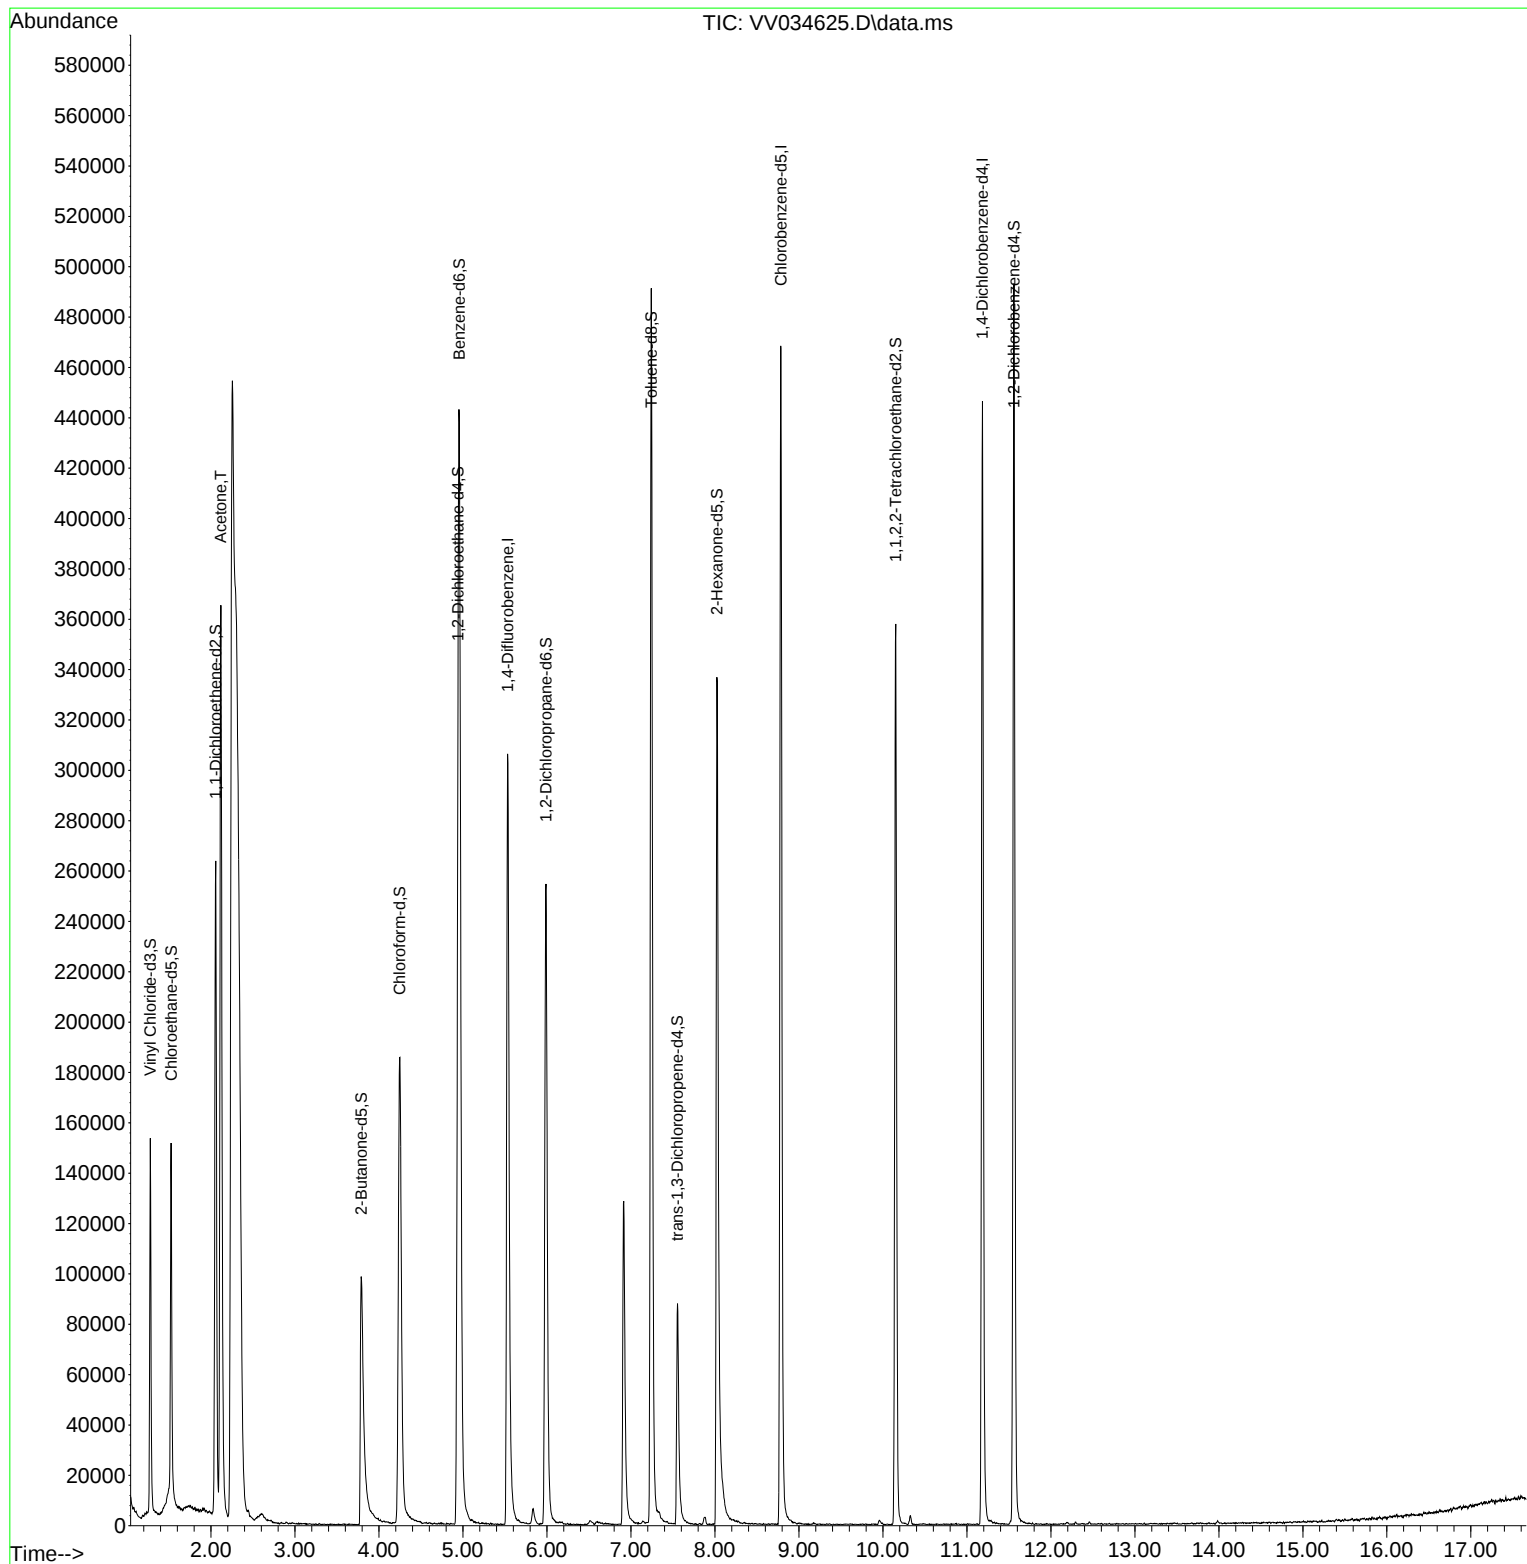

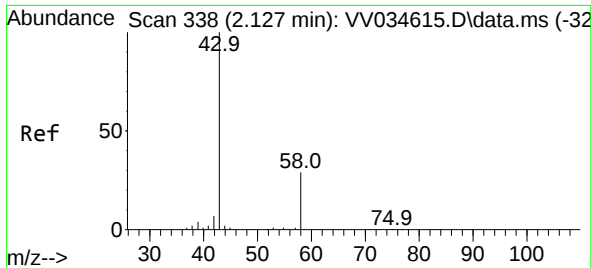

#13

Acetone

Concen: 217.568 ug/L

RT: 2.117 min Scan# 31

Delta R.T. -0.010 min

Lab File: VV034625.D

Acq: 15 Mar 2024 00:37

Instrument :

MSVOA_V

ClientSampleId :

YCKX6

Tgt Ion: 43 Resp: 401703

Ion Ratio Lower Upper

43 100

58 29.2 0.0 57.2

