

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031424\
 Data File : VW034626.D
 Acq On : 15 Mar 2024 01:00
 Operator : SY/MD
 Sample : P1751-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKX7

Quant Time: Mar 15 06:56:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 15 06:40:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	292823	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	271106	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	127745	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	113873	44.859	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	89.720%		
7) Chloroethane-d5	1.529	69	95351	48.214	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.420%		
11) 1,1-Dichloroethene-d2	2.056	65	53159	46.305	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.600%		
21) 2-Butanone-d5	3.789	46	171505	101.030	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.030%		
24) Chloroform-d	4.246	84	210786	46.964	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.920%		
26) 1,2-Dichloroethane-d4	4.941	65	145042	49.452	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.900%		
32) Benzene-d6	4.960	84	414009	50.600	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.200%		
36) 1,2-Dichloropropane-d6	5.985	67	128636	51.516	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	103.040%		
41) Toluene-d8	7.243	98	357833	48.327	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.660%		
43) trans-1,3-Dichloroprop...	7.555	79	52204	41.633	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.260%		
47) 2-Hexanone-d5	8.024	63	119758	96.045	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	96.050%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	170759	51.965	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	103.940%		
66) 1,2-Dichlorobenzene-d4	11.561	152	132574	50.772	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.540%		
Target Compounds					Qvalue	
13) Acetone	2.117	43	199024	97.525	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034626.D
Acq On : 15 Mar 2024 01:00
Operator : SY/MD
Sample : P1751-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKX7

Quant Time: Mar 15 06:56:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 06:40:01 2024
Response via : Initial Calibration

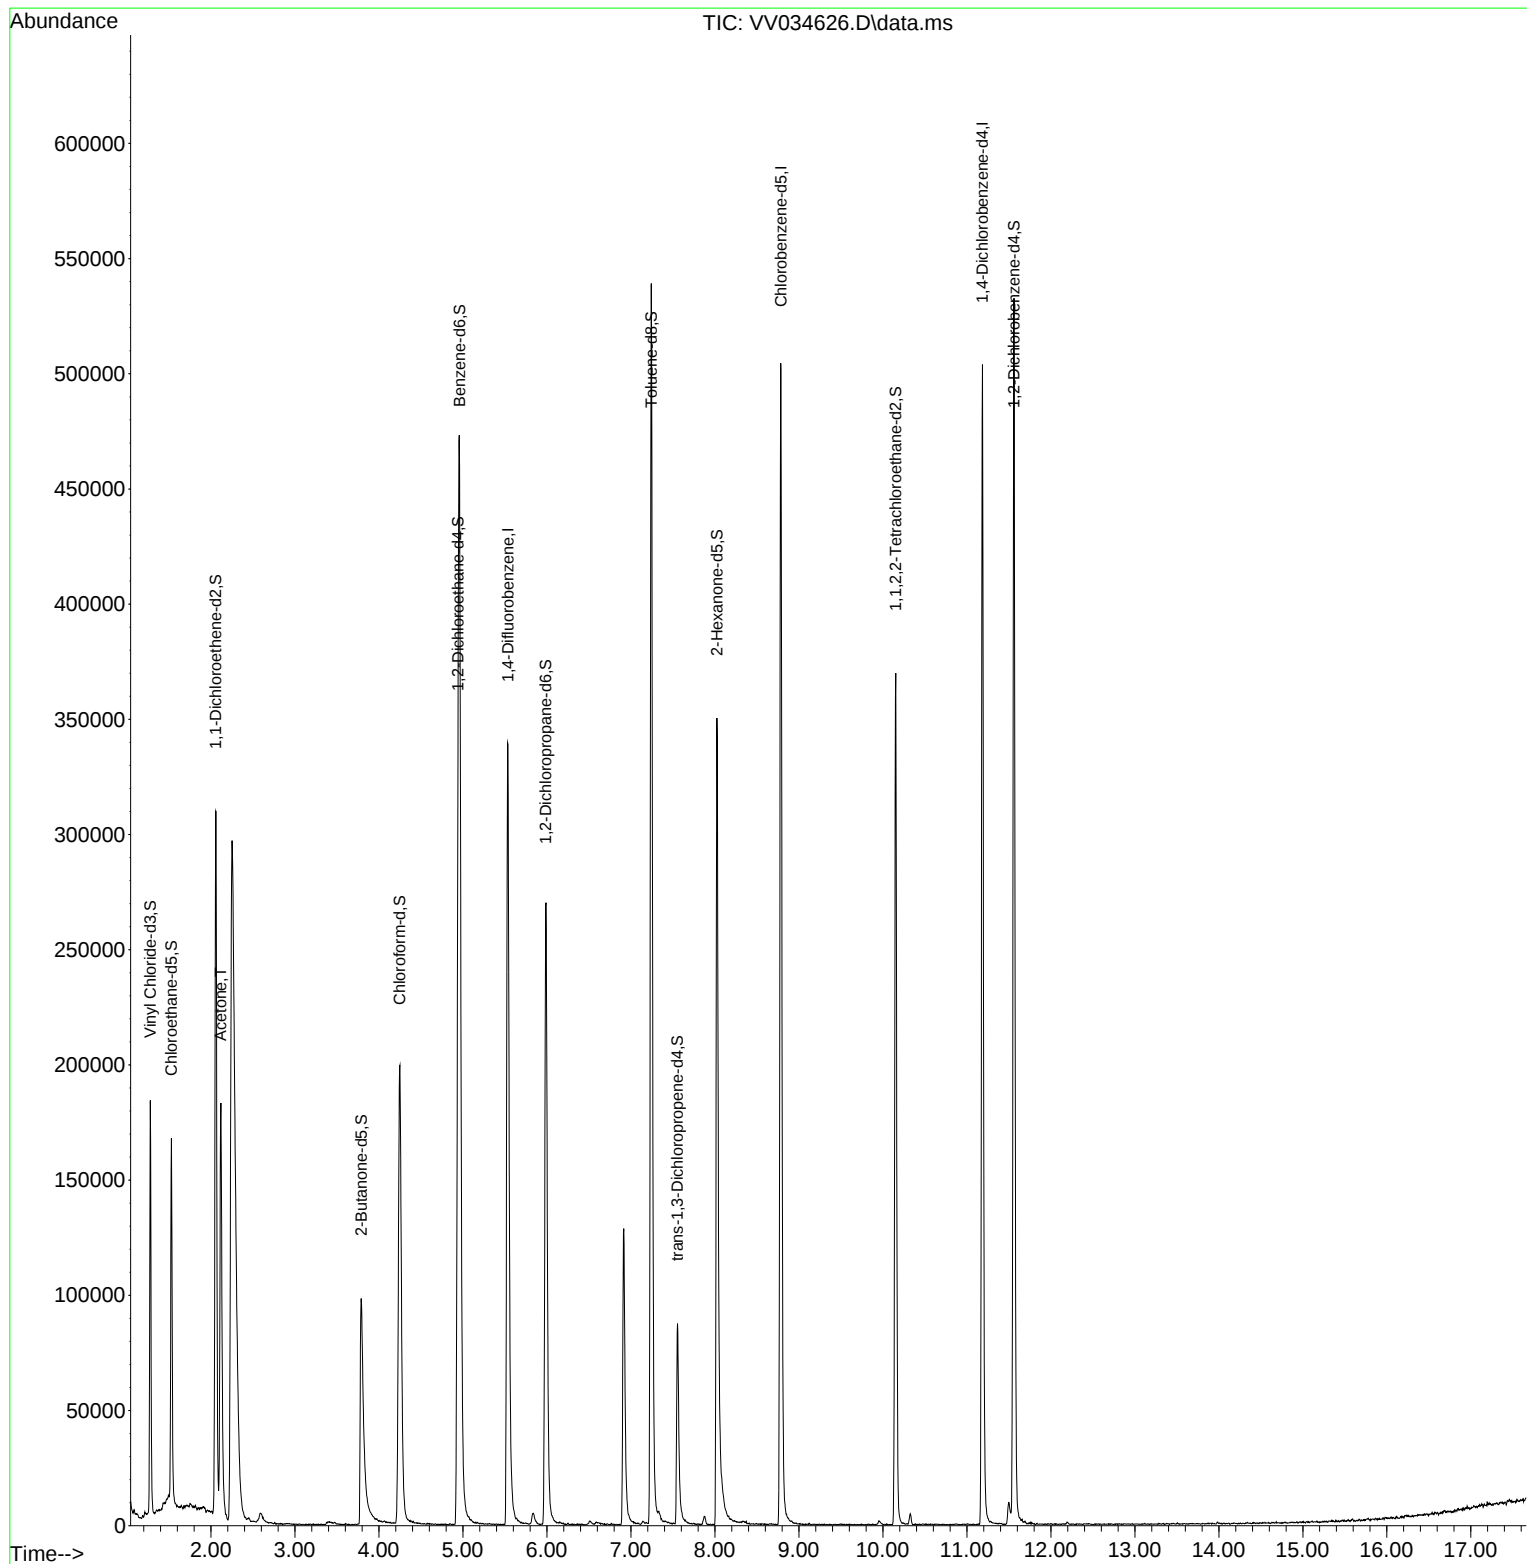

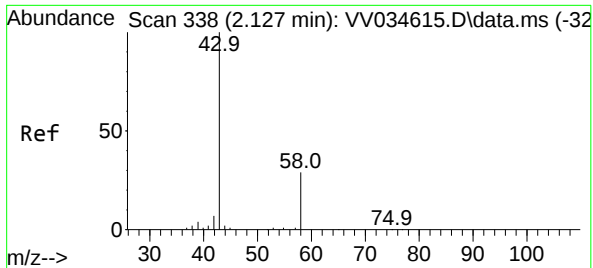

#13
 Acetone
 Concen: 97.525 ug/L
 RT: 2.117 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV034626.D
 Acq: 15 Mar 2024 01:00

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKX7

Tgt Ion: 43 Resp: 199024
 Ion Ratio Lower Upper
 43 100
 58 29.3 0.0 57.2

