

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034627.D
 Acq On : 15 Mar 2024 01:24
 Operator : SY/MD
 Sample : P1751-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKX8

Quant Time: Mar 15 06:57:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 15 06:40:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	295807	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	272551	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	129731	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	116861	45.572	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	91.140%	
7) Chloroethane-d5	1.529	69	97714	48.911	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	97.820%	
11) 1,1-Dichloroethene-d2	2.056	65	52075	44.903	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	89.800%	
21) 2-Butanone-d5	3.789	46	174421	101.711	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	101.710%	
24) Chloroform-d	4.249	84	213379	47.062	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	94.120%	
26) 1,2-Dichloroethane-d4	4.940	65	143096	48.296	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.600%	
32) Benzene-d6	4.960	84	415676	50.534	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.060%	
36) 1,2-Dichloropropane-d6	5.985	67	129613	51.632	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	103.260%	
41) Toluene-d8	7.243	98	360095	48.375	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	96.740%	
43) trans-1,3-Dichloroprop...	7.555	79	53626	42.540	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	85.080%	
47) 2-Hexanone-d5	8.024	63	123506	98.526	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	98.530%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84	173398	52.489	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	104.980%	
66) 1,2-Dichlorobenzene-d4	11.561	152	132598	50.004	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.000%	
Target Compounds						
13) Acetone	2.117	43	78051	37.860	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034627.D
Acq On : 15 Mar 2024 01:24
Operator : SY/MD
Sample : P1751-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKX8

Quant Time: Mar 15 06:57:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 06:40:01 2024
Response via : Initial Calibration

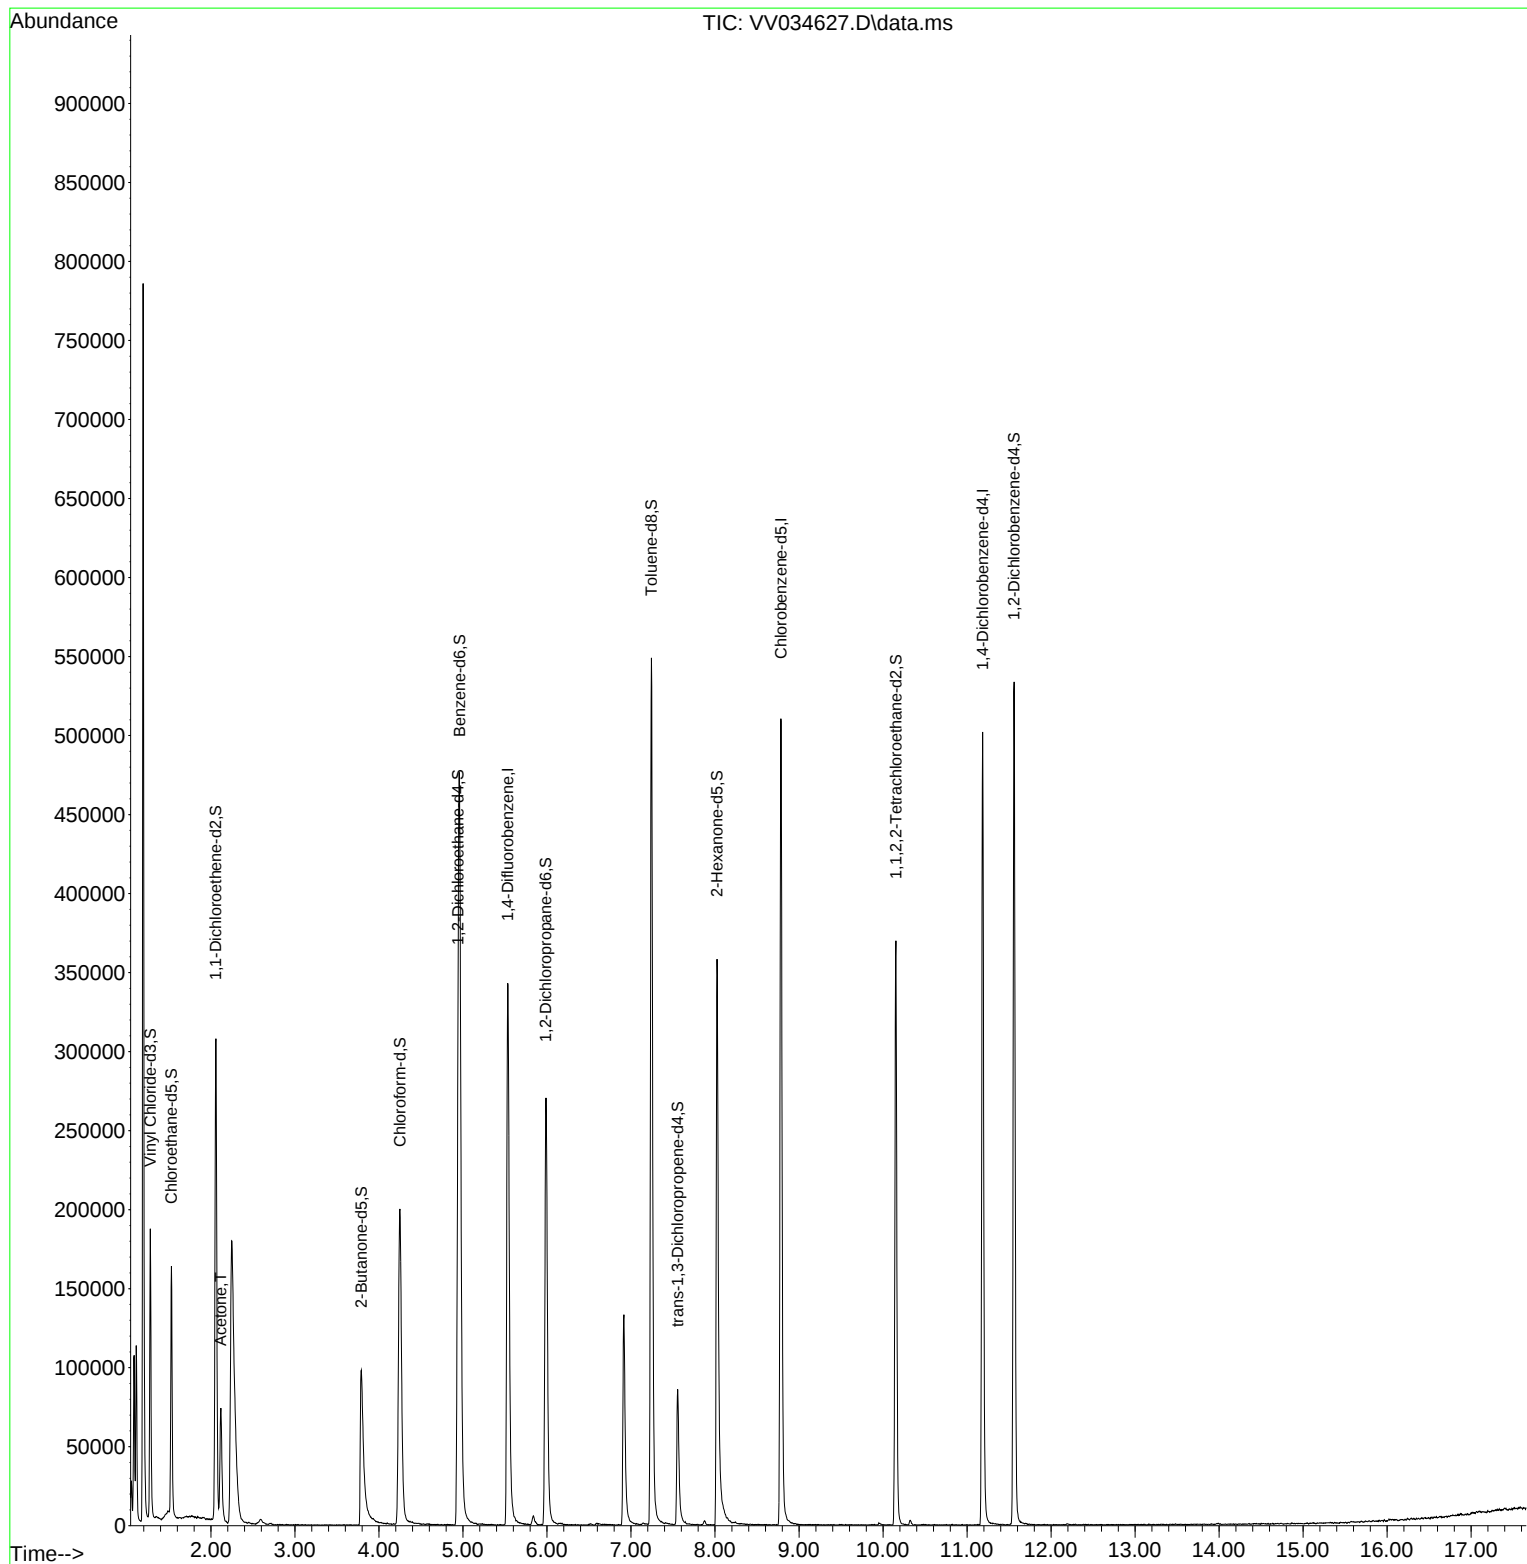

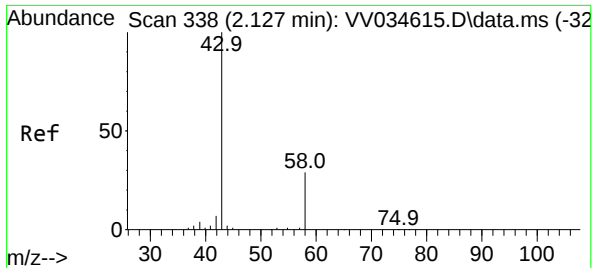

#13
 Acetone
 Concen: 37.860 ug/L
 RT: 2.117 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV034627.D
 Acq: 15 Mar 2024 01:24

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKX8

Tgt Ion: 43 Resp: 78051
 Ion Ratio Lower Upper
 43 100
 58 29.2 0.0 57.2

