

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034628.D
 Acq On : 15 Mar 2024 01:48
 Operator : SY/MD
 Sample : P1751-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKX9

Quant Time: Mar 15 06:57:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 15 06:40:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	295017	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	272572	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	128181	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	114620	44.817	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.640%
7) Chloroethane-d5	1.529	69	98063	49.217	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.440%
11) 1,1-Dichloroethene-d2	2.060	65	52885	45.724	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.440%
21) 2-Butanone-d5	3.786	46	178219	104.204	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.200%
24) Chloroform-d	4.249	84	219478	48.537	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.080%
26) 1,2-Dichloroethane-d4	4.941	65	147840	50.031	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.060%
32) Benzene-d6	4.960	84	421677	51.260	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.520%
36) 1,2-Dichloropropane-d6	5.989	67	130121	51.831	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.660%
41) Toluene-d8	7.243	98	354284	47.591	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.180%
43) trans-1,3-Dichloroprop...	7.555	79	52623	41.741	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.480%
47) 2-Hexanone-d5	8.024	63	123405	98.438	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.440%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	173460	52.503	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	105.000%
66) 1,2-Dichlorobenzene-d4	11.561	152	131003	50.000	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.000%
Target Compounds						
					Qvalue	
13) Acetone	2.117	43	80083	38.950	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034628.D
Acq On : 15 Mar 2024 01:48
Operator : SY/MD
Sample : P1751-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKX9

Quant Time: Mar 15 06:57:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 06:40:01 2024
Response via : Initial Calibration

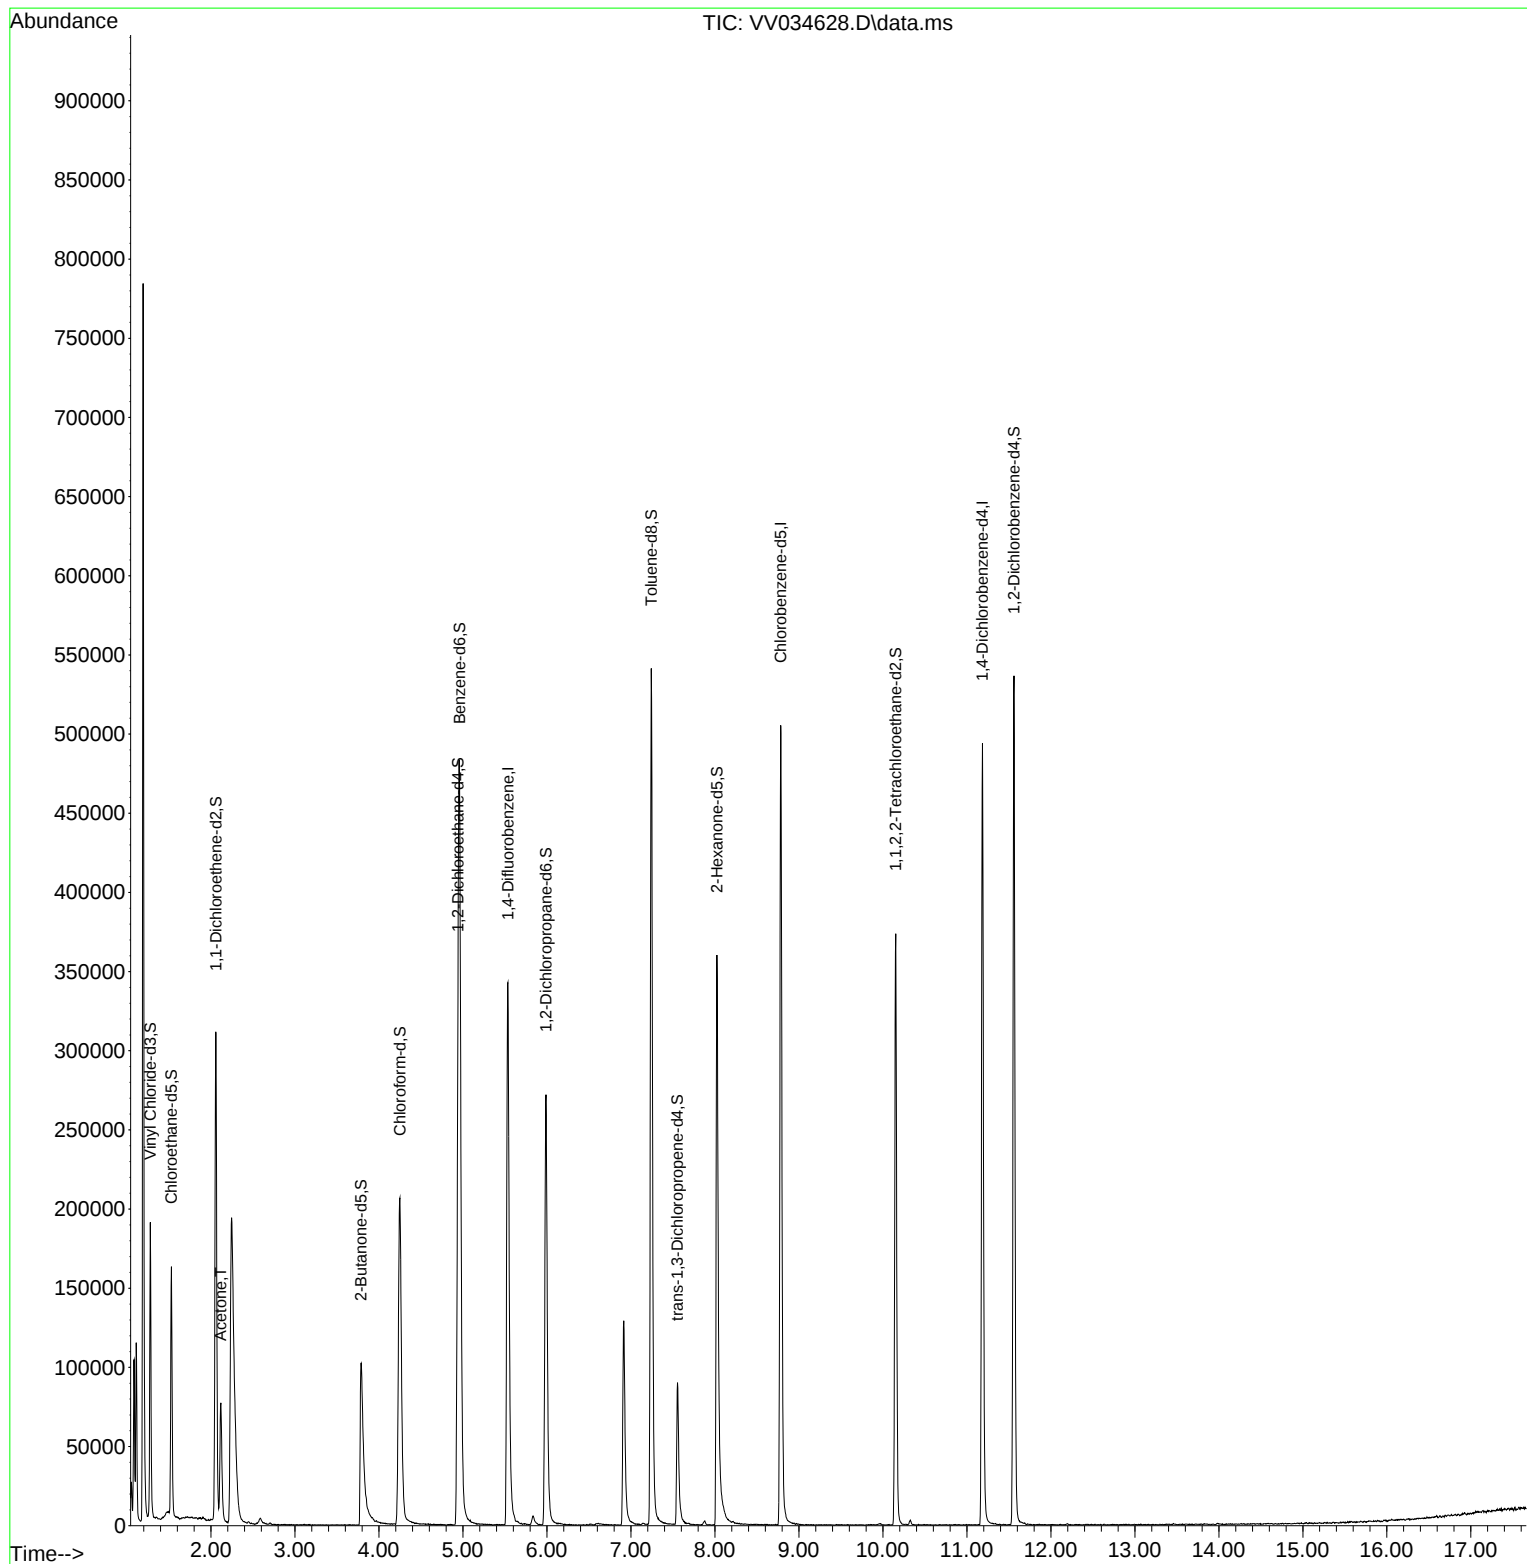

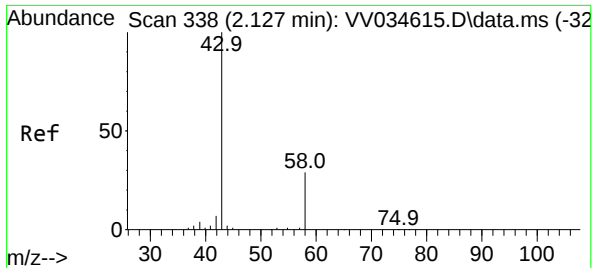

#13
 Acetone
 Concen: 38.950 ug/L
 RT: 2.117 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV034628.D
 Acq: 15 Mar 2024 01:48

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKX9

Tgt Ion: 43 Resp: 80083
 Ion Ratio Lower Upper
 43 100
 58 29.9 0.0 57.2

