

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034590.D
 Acq On : 14 Mar 2024 09:46
 Operator : SY/MD
 Sample : VV0314MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK242

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

Signal : TIC: VV034590.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	229186	239838	16.02%	2.215%
2	1.529	146	152	172	rVB	193719	228294	15.25%	2.108%
3	2.056	307	316	334	rVB	380256	554546	37.04%	5.121%
4	2.243	365	374	385	rBV3	1896	3654	0.24%	0.034%
5	2.384	416	418	422	rBV	606	421	0.03%	0.004%
6	2.423	427	430	431	rBV2	408	255	0.02%	0.002%
7	2.667	500	506	510	rBV2	293	306	0.02%	0.003%
8	2.699	513	516	520	rBV3	526	541	0.04%	0.005%
9	2.744	526	530	533	rBV2	278	284	0.02%	0.003%
10	2.802	541	548	550	rBV2	185	261	0.02%	0.002%
11	2.931	584	588	589	rBV	149	105	0.01%	0.001%
12	2.976	599	602	604	rBV	190	129	0.01%	0.001%
13	3.317	704	708	709	rBV2	237	139	0.01%	0.001%
14	3.343	712	716	720	rVB2	194	161	0.01%	0.001%
15	3.371	720	725	728	rBV2	185	164	0.01%	0.002%
16	3.539	775	777	780	rVV	181	106	0.01%	0.001%
17	3.568	783	786	792	rBV2	161	153	0.01%	0.001%
18	3.680	819	821	826	rVB2	265	144	0.01%	0.001%
19	3.712	826	831	834	rBV2	206	204	0.01%	0.002%
20	3.786	846	854	891	rBV	108653	311996	20.84%	2.881%
21	4.243	982	996	1029	rBV2	231609	594516	39.71%	5.490%
22	4.571	1095	1098	1099	rBV3	344	213	0.01%	0.002%
23	4.629	1113	1116	1119	rVB2	297	178	0.01%	0.002%
24	4.677	1128	1131	1136	rBV2	450	484	0.03%	0.004%
25	4.715	1141	1143	1148	rBV2	292	176	0.01%	0.002%
26	4.876	1190	1193	1194	rBV2	272	115	0.01%	0.001%
27	4.889	1194	1197	1200	rBV3	239	157	0.01%	0.001%
28	4.953	1200	1217	1254	rBV2	569560	1497300	100.00%	13.826%
29	5.285	1315	1320	1327	rBV4	471	531	0.04%	0.005%
30	5.313	1327	1329	1331	rBV2	419	219	0.01%	0.002%
31	5.432	1364	1366	1368	rBV	300	139	0.01%	0.001%
32	5.529	1382	1396	1432	rBV	371892	775171	51.77%	7.158%
33	5.828	1479	1489	1502	rBV3	12823	28130	1.88%	0.260%
34	5.985	1525	1538	1568	rBV	321129	661425	44.17%	6.107%
35	6.240	1614	1617	1621	rVB2	331	230	0.02%	0.002%
36	6.265	1621	1625	1629	rBV	179	185	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034590.D
 Acq On : 14 Mar 2024 09:46
 Operator : SY/MD
 Sample : VV0314MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK242

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.490	1692	1695	1702	rVB2	238	189	0.01%	0.002%
38	6.522	1702	1705	1711	rVB2	186	140	0.01%	0.001%
39	6.584	1718	1724	1729	rBV4	1181	1546	0.10%	0.014%
40	6.719	1764	1766	1771	rVB2	547	284	0.02%	0.003%
41	6.744	1771	1774	1780	rBV	442	419	0.03%	0.004%
42	6.802	1790	1792	1797	rVB	264	179	0.01%	0.002%
43	6.857	1806	1809	1812	rBV2	258	172	0.01%	0.002%
44	6.912	1814	1826	1869	rBV	165032	316548	21.14%	2.923%
45	7.239	1917	1928	1953	rBV	652488	1132693	75.65%	10.459%
46	7.551	2016	2025	2054	rBV	111219	202767	13.54%	1.872%
47	7.847	2113	2117	2118	rBV	301	173	0.01%	0.002%
48	7.918	2136	2139	2142	rVB2	384	220	0.01%	0.002%
49	7.937	2143	2145	2147	rBV	259	104	0.01%	0.001%
50	7.973	2153	2156	2159	rBV2	313	250	0.02%	0.002%
51	8.024	2162	2172	2213	rBV	372693	726292	48.51%	6.706%
52	8.445	2301	2303	2304	rBV	343	124	0.01%	0.001%
53	8.526	2325	2328	2329	rBV	152	101	0.01%	0.001%
54	8.561	2335	2339	2346	rVB3	501	503	0.03%	0.005%
55	8.606	2350	2353	2358	rBV	262	221	0.01%	0.002%
56	8.677	2372	2375	2377	rVB	385	182	0.01%	0.002%
57	8.783	2397	2408	2447	rBV	543923	909744	60.76%	8.400%
58	9.030	2480	2485	2487	rBV2	372	314	0.02%	0.003%
59	9.165	2524	2527	2530	rBV3	309	226	0.02%	0.002%
60	9.217	2539	2543	2546	rBV2	140	136	0.01%	0.001%
61	9.455	2613	2617	2619	rBV2	286	164	0.01%	0.002%
62	9.484	2622	2626	2633	rBV4	708	986	0.07%	0.009%
63	9.571	2650	2653	2655	rBV2	239	120	0.01%	0.001%
64	9.587	2655	2658	2661	rVB2	205	120	0.01%	0.001%
65	9.690	2689	2690	2697	rVV2	185	111	0.01%	0.001%
66	9.715	2697	2698	2704	rVB	229	147	0.01%	0.001%
67	9.960	2771	2774	2778	rVB2	243	159	0.01%	0.001%
68	10.149	2822	2833	2860	rVV	404017	638107	42.62%	5.892%
69	10.329	2880	2889	2894	rBV3	979	1430	0.10%	0.013%
70	10.751	3018	3020	3025	rVB2	251	135	0.01%	0.001%
71	10.773	3025	3027	3030	rVB	212	103	0.01%	0.001%
72	10.808	3035	3038	3042	rBV2	258	190	0.01%	0.002%
73	10.866	3046	3056	3062	rBV2	1398	2205	0.15%	0.020%
74	11.130	3131	3138	3144	rBV4	2435	3387	0.23%	0.031%
75	11.185	3144	3155	3177	rVV	560539	882280	58.92%	8.147%
76	11.500	3248	3253	3256	rBV2	295	248	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034590.D
 Acq On : 14 Mar 2024 09:46
 Operator : SY/MD
 Sample : VV0314MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK242

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	11.558	3258	3271	3297	rBV	640122	1010332	67.48%	9.329%
78	11.718	3319	3321	3325	rBV2	245	152	0.01%	0.001%
79	11.779	3338	3340	3341	rBV	247	108	0.01%	0.001%
80	11.818	3350	3352	3354	rBV	239	122	0.01%	0.001%
81	11.863	3363	3366	3370	rVB2	286	181	0.01%	0.002%
82	11.905	3377	3379	3383	rVB2	232	133	0.01%	0.001%
83	11.937	3383	3389	3390	rBV	224	204	0.01%	0.002%
84	12.194	3460	3469	3482	rBV2	1360	2208	0.15%	0.020%
85	12.368	3520	3523	3524	rBV3	644	377	0.03%	0.003%
86	12.394	3529	3531	3536	rBV2	321	180	0.01%	0.002%
87	12.590	3584	3592	3600	rBV4	3712	5531	0.37%	0.051%
88	12.641	3605	3608	3611	rBV3	296	206	0.01%	0.002%
89	12.670	3615	3617	3619	rBV2	279	132	0.01%	0.001%
90	13.017	3722	3725	3729	rBV2	363	249	0.02%	0.002%
91	13.204	3774	3783	3797	rBV4	8222	13605	0.91%	0.126%
92	13.320	3815	3819	3824	rBV2	362	350	0.02%	0.003%
93	13.342	3824	3826	3828	rVV	243	121	0.01%	0.001%
94	13.377	3834	3837	3839	rBV	351	168	0.01%	0.002%
95	13.442	3849	3857	3880	rVB2	31549	53424	3.57%	0.493%
96	13.567	3894	3896	3899	rBV2	386	231	0.02%	0.002%
97	13.683	3924	3932	3940	rBV3	10356	16200	1.08%	0.150%
98	13.754	3949	3954	3956	rBV3	460	401	0.03%	0.004%
99	14.178	4082	4086	4088	rBV2	427	425	0.03%	0.004%
100	14.435	4164	4166	4169	rBV	557	412	0.03%	0.004%




Sum of corrected areas: 10829741

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034590.D
Acq On : 14 Mar 2024 09:46
Operator : SY/MD
Sample : VV0314MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK242

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

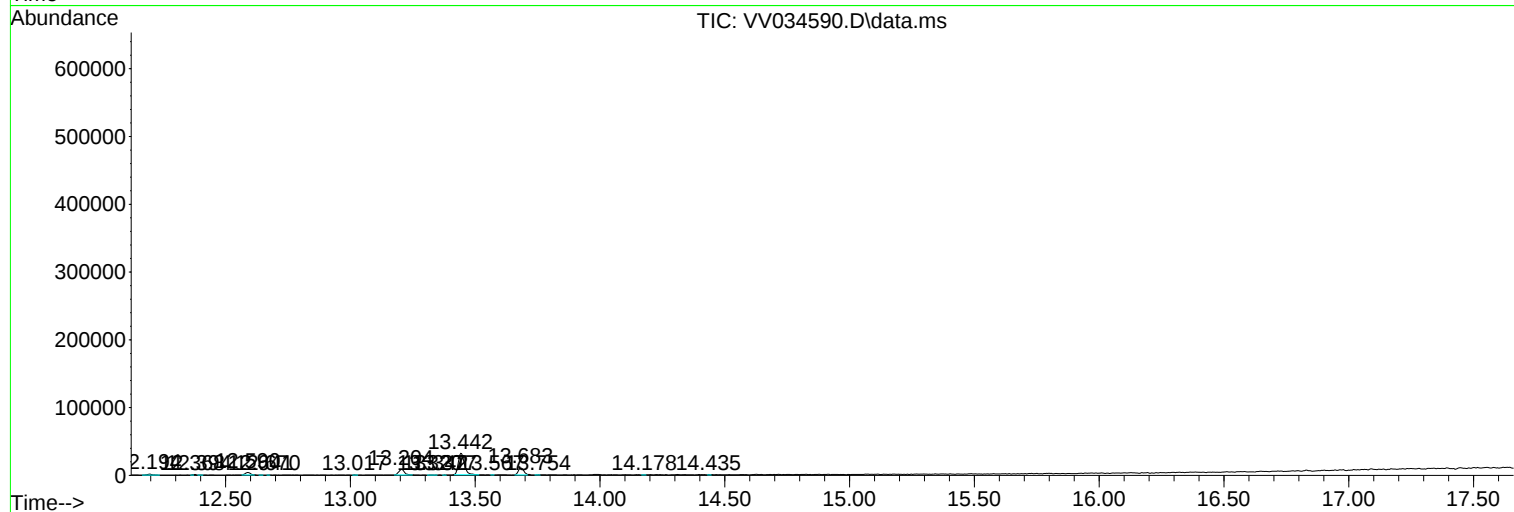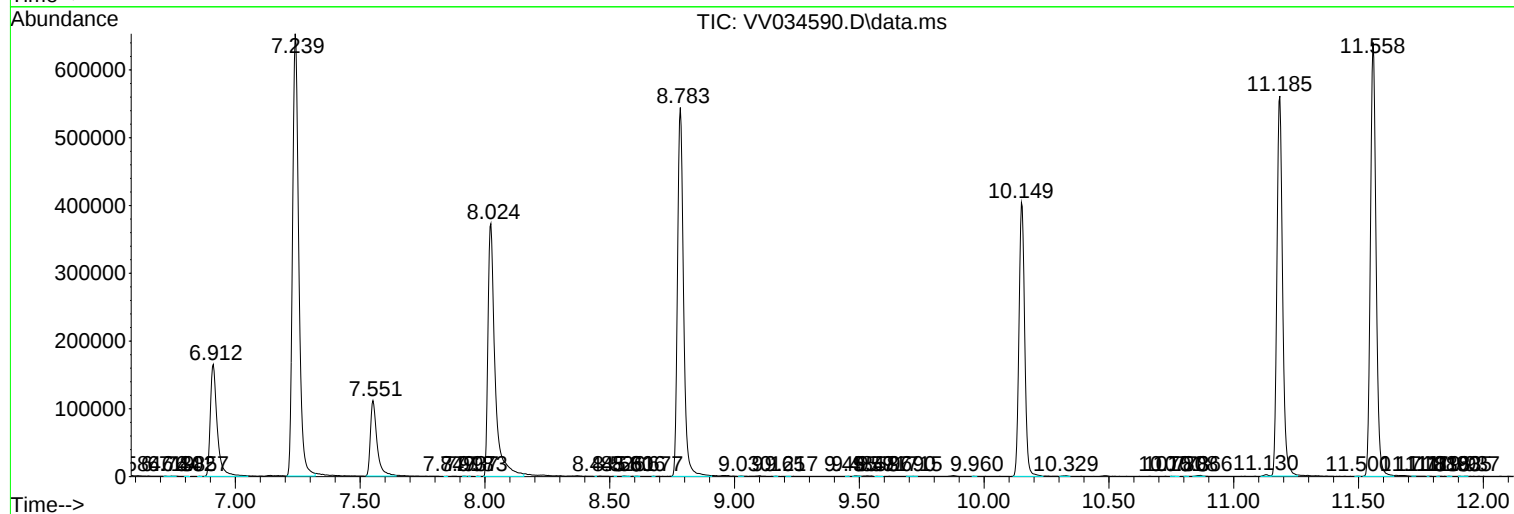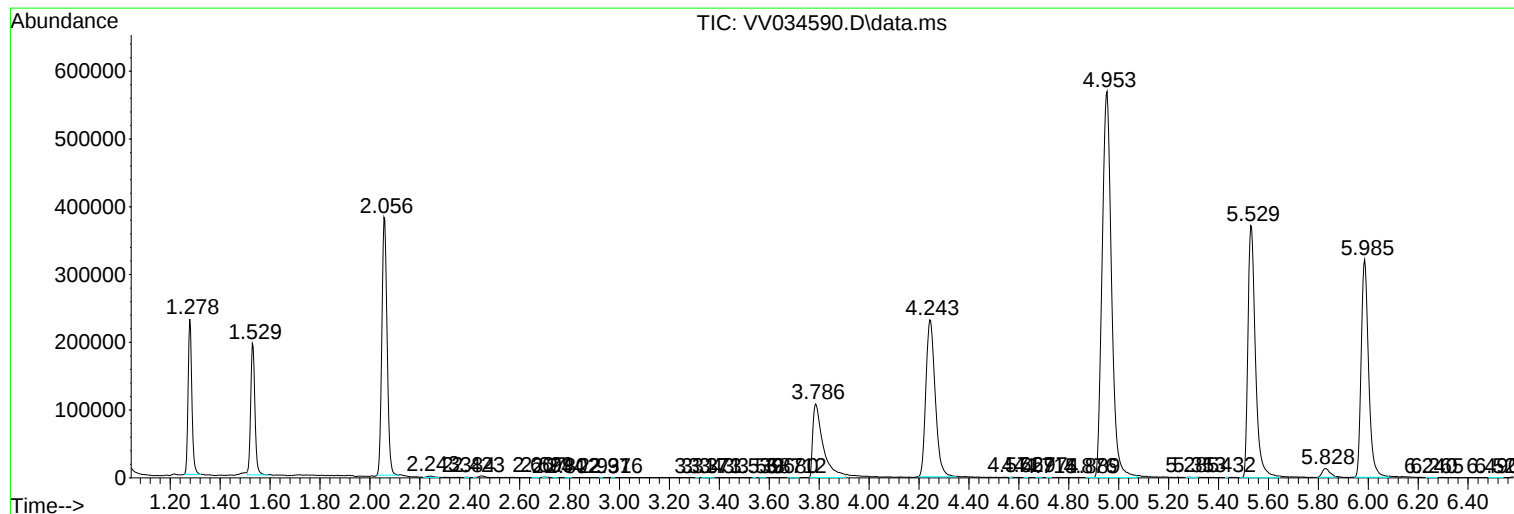

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034590.D
Acq On : 14 Mar 2024 09:46
Operator : SY/MD
Sample : VV0314MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK242

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034590.D
Acq On : 14 Mar 2024 09:46
Operator : SY/MD
Sample : VV0314MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK242

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc