

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034592.D
 Acq On : 14 Mar 2024 10:40
 Operator : SY/MD
 Sample : P1739-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034592.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	211155	222114	15.46%	2.117%
2	1.529	145	152	175	rVB	184275	219669	15.29%	2.093%
3	2.056	306	316	330	rBV	357437	525322	36.55%	5.006%
4	2.548	464	469	470	rBV	708	542	0.04%	0.005%
5	2.632	492	495	498	rBV3	295	221	0.02%	0.002%
6	2.683	509	511	514	rBV2	223	136	0.01%	0.001%
7	2.696	514	515	517	rVB	205	79	0.01%	0.001%
8	2.709	517	519	525	rBV2	280	232	0.02%	0.002%
9	2.789	541	544	546	rBV	252	143	0.01%	0.001%
10	2.908	578	581	587	rVB	295	275	0.02%	0.003%
11	2.950	591	594	596	rVV	358	161	0.01%	0.002%
12	2.966	596	599	604	rVB2	118	95	0.01%	0.001%
13	3.069	628	631	638	rBV2	171	136	0.01%	0.001%
14	3.217	674	677	679	rBV	159	119	0.01%	0.001%
15	3.249	684	687	690	rBV2	135	96	0.01%	0.001%
16	3.458	748	752	755	rVB	240	137	0.01%	0.001%
17	3.478	755	758	760	rBV	147	94	0.01%	0.001%
18	3.529	770	774	778	rBV	245	235	0.02%	0.002%
19	3.555	778	782	784	rVV2	88	76	0.01%	0.001%
20	3.632	803	806	809	rVB	197	121	0.01%	0.001%
21	3.728	832	836	840	rBV	314	383	0.03%	0.004%
22	3.786	845	854	889	rBV	104027	306829	21.35%	2.924%
23	4.243	982	996	1038	rBV2	287309	746216	51.92%	7.111%
24	4.596	1104	1106	1108	rVB	333	159	0.01%	0.002%
25	4.738	1147	1150	1156	rBV3	355	414	0.03%	0.004%
26	4.834	1175	1180	1182	rBV2	382	347	0.02%	0.003%
27	4.879	1188	1194	1195	rBV	285	111	0.01%	0.001%
28	4.953	1201	1217	1250	rBV2	547539	1437136	100.00%	13.695%
29	5.233	1302	1304	1309	rVB3	580	291	0.02%	0.003%
30	5.317	1328	1330	1332	rBV	289	168	0.01%	0.002%
31	5.407	1356	1358	1359	rBV	161	71	0.00%	0.001%
32	5.442	1366	1369	1373	rVB2	332	241	0.02%	0.002%
33	5.468	1373	1377	1378	rBV2	339	194	0.01%	0.002%
34	5.494	1382	1385	1386	rBV2	254	101	0.01%	0.001%
35	5.532	1386	1397	1427	rBV	355491	738230	51.37%	7.035%
36	5.831	1479	1490	1506	rBV5	11056	24137	1.68%	0.230%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034592.D
 Acq On : 14 Mar 2024 10:40
 Operator : SY/MD
 Sample : P1739-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.985	1525	1538	1567	rBV	306950	631882	43.97%	6.021%
38	6.249	1616	1620	1622	rVB2	348	239	0.02%	0.002%
39	6.297	1632	1635	1638	rVV2	369	264	0.02%	0.003%
40	6.355	1649	1653	1657	rBV2	242	216	0.02%	0.002%
41	6.371	1657	1658	1660	rBV2	188	68	0.00%	0.001%
42	6.416	1667	1672	1674	rBV	167	143	0.01%	0.001%
43	6.461	1682	1686	1689	rBV2	255	222	0.02%	0.002%
44	6.584	1716	1724	1726	rBV2	947	947	0.07%	0.009%
45	6.747	1772	1775	1777	rBV2	263	162	0.01%	0.002%
46	6.809	1790	1794	1800	rBV2	185	198	0.01%	0.002%
47	6.876	1812	1815	1816	rBV	277	142	0.01%	0.001%
48	6.911	1816	1826	1850	rBV	161433	305609	21.27%	2.912%
49	7.239	1918	1928	1968	rBV	633093	1118213	77.81%	10.656%
50	7.551	2016	2025	2048	rBV	107020	197313	13.73%	1.880%
51	7.776	2090	2095	2098	rBV4	527	593	0.04%	0.006%
52	7.815	2103	2107	2109	rBV2	265	192	0.01%	0.002%
53	7.873	2117	2125	2138	rVB3	3099	5731	0.40%	0.055%
54	8.024	2162	2172	2216	rBV	363051	701432	48.81%	6.684%
55	8.513	2321	2324	2326	rBV2	389	280	0.02%	0.003%
56	8.706	2380	2384	2387	rBV2	381	267	0.02%	0.003%
57	8.783	2397	2408	2434	rBV	539036	891334	62.02%	8.494%
58	9.014	2479	2480	2481	rBV	312	69	0.00%	0.001%
59	9.075	2497	2499	2501	rVB2	300	146	0.01%	0.001%
60	9.101	2501	2507	2508	rBV2	122	98	0.01%	0.001%
61	9.117	2509	2512	2514	rVB2	326	143	0.01%	0.001%
62	9.156	2521	2524	2528	rVB3	330	188	0.01%	0.002%
63	9.181	2530	2532	2536	rVB2	245	124	0.01%	0.001%
64	9.201	2536	2538	2540	rBV	134	65	0.00%	0.001%
65	9.271	2558	2560	2561	rBV	191	70	0.00%	0.001%
66	9.281	2561	2563	2571	rVB2	298	304	0.02%	0.003%
67	9.484	2623	2626	2627	rBV	147	79	0.01%	0.001%
68	9.490	2627	2628	2635	rVB2	294	201	0.01%	0.002%
69	9.526	2636	2639	2643	rVB	194	135	0.01%	0.001%
70	9.548	2643	2646	2648	rBV2	171	109	0.01%	0.001%
71	9.731	2699	2703	2707	rBV2	273	272	0.02%	0.003%
72	9.963	2768	2775	2788	rBV5	2984	6544	0.46%	0.062%
73	10.075	2808	2810	2815	rBV	228	166	0.01%	0.002%
74	10.149	2822	2833	2857	rBV	385129	605555	42.14%	5.770%
75	10.329	2878	2889	2896	rBV3	3370	4963	0.35%	0.047%
76	10.384	2903	2906	2911	rBV2	153	147	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034592.D
 Acq On : 14 Mar 2024 10:40
 Operator : SY/MD
 Sample : P1739-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.426	2916	2919	2922	rBV2	147	141	0.01%	0.001%
78	10.439	2922	2923	2926	rBV	174	94	0.01%	0.001%
79	10.480	2934	2936	2937	rBV	329	122	0.01%	0.001%
80	10.651	2986	2989	2993	rBV2	119	136	0.01%	0.001%
81	10.796	3030	3034	3037	rBV	278	184	0.01%	0.002%
82	10.860	3050	3054	3057	rBV2	314	267	0.02%	0.003%
83	11.005	3097	3099	3101	rBV2	182	94	0.01%	0.001%
84	11.091	3123	3126	3127	rBV2	230	136	0.01%	0.001%
85	11.130	3134	3138	3141	rBV2	493	398	0.03%	0.004%
86	11.185	3144	3155	3181	rBV	530738	834694	58.08%	7.954%
87	11.493	3248	3251	3253	rBV	224	161	0.01%	0.002%
88	11.558	3259	3271	3293	rBV	597945	951293	66.19%	9.065%
89	11.763	3331	3335	3342	rBV3	344	491	0.03%	0.005%
90	11.853	3361	3363	3366	rVB	397	144	0.01%	0.001%
91	11.869	3366	3368	3369	rBV	197	89	0.01%	0.001%
92	12.406	3533	3535	3537	rBV	235	112	0.01%	0.001%
93	12.625	3601	3603	3606	rVB	368	159	0.01%	0.002%
94	12.805	3656	3659	3661	rBV2	415	254	0.02%	0.002%
95	12.931	3697	3698	3702	rVB	234	88	0.01%	0.001%
96	12.953	3702	3705	3708	rBV2	378	287	0.02%	0.003%
97	13.451	3853	3860	3871	rBV2	2968	4474	0.31%	0.043%
98	13.551	3889	3891	3895	rBV	337	126	0.01%	0.001%
99	13.567	3895	3896	3899	rBV	280	103	0.01%	0.001%
100	13.911	4002	4003	4006	rBV	298	213	0.01%	0.002%




Sum of corrected areas: 10494116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034592.D
Acq On : 14 Mar 2024 10:40
Operator : SY/MD
Sample : P1739-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

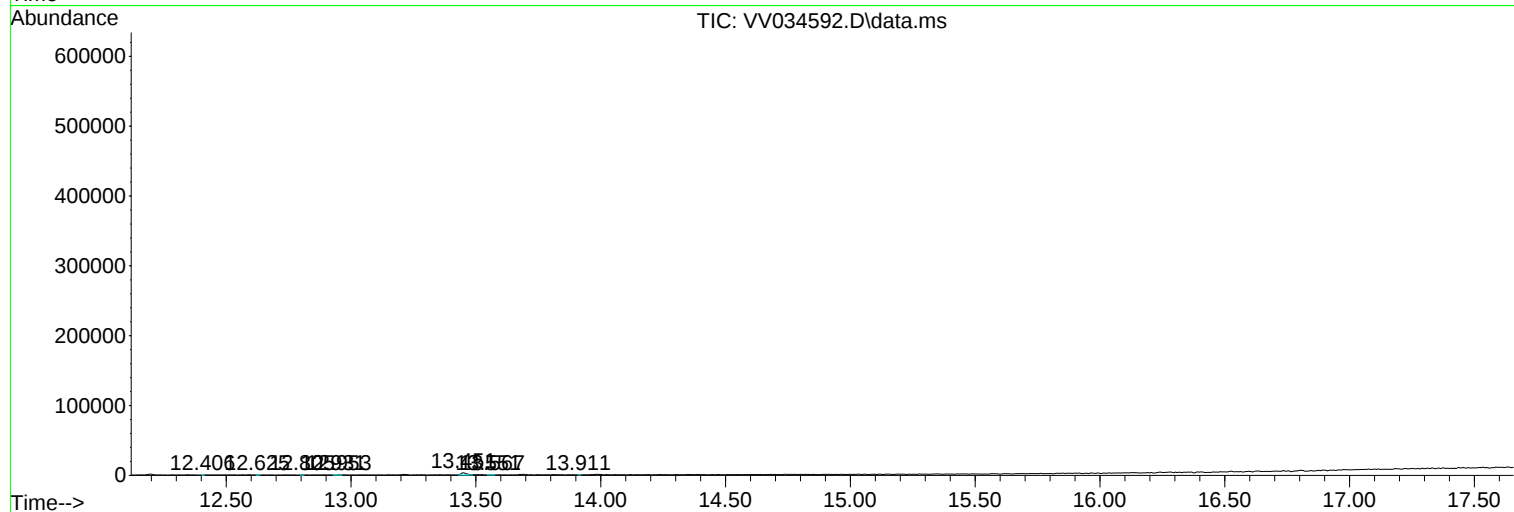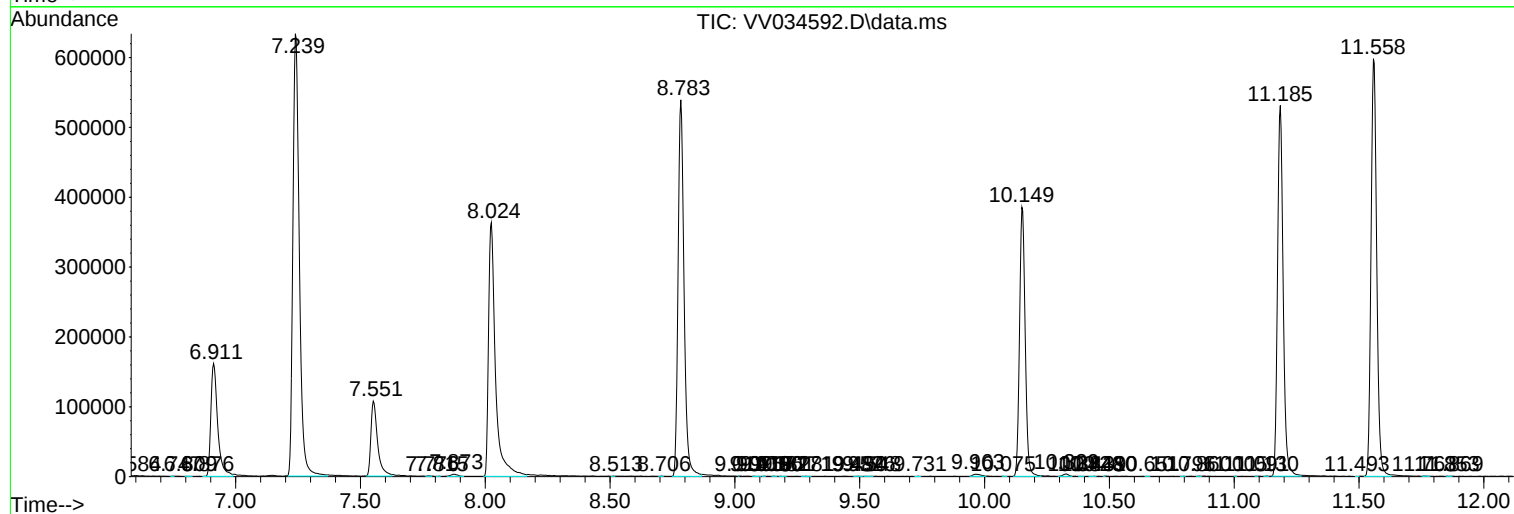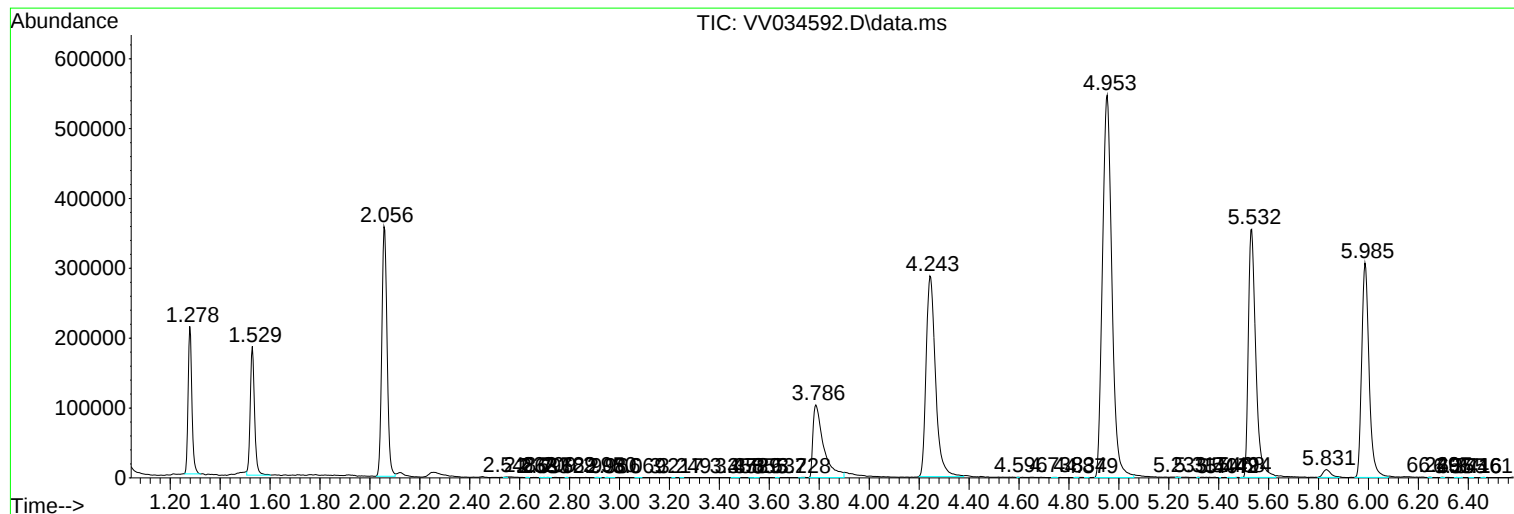

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034592.D
Acq On : 14 Mar 2024 10:40
Operator : SY/MD
Sample : P1739-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034592.D
Acq On : 14 Mar 2024 10:40
Operator : SY/MD
Sample : P1739-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc