

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034593.D
 Acq On : 14 Mar 2024 11:04
 Operator : SY/MD
 Sample : P1739-04DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	205687	214969	15.85%	2.050%
2	1.529	145	152	168	rVB	174639	204880	15.11%	1.954%
3	2.059	306	317	333	rBV2	362195	540703	39.87%	5.156%
4	2.449	431	438	449	rVB4	2246	3328	0.25%	0.032%
5	2.587	477	481	484	rVB2	264	185	0.01%	0.002%
6	2.606	484	487	490	rVB3	250	140	0.01%	0.001%
7	2.767	534	537	544	rVB2	431	381	0.03%	0.004%
8	2.802	544	548	550	rBV	253	230	0.02%	0.002%
9	2.844	557	561	564	rBV	206	179	0.01%	0.002%
10	2.889	571	575	577	rBV	214	200	0.01%	0.002%
11	3.011	608	613	615	rBV2	147	124	0.01%	0.001%
12	3.027	615	618	621	rVB2	167	100	0.01%	0.001%
13	3.088	630	637	639	rBV2	166	210	0.02%	0.002%
14	3.285	694	698	704	rBV2	182	202	0.01%	0.002%
15	3.317	704	708	711	rVB2	231	181	0.01%	0.002%
16	3.481	754	759	762	rBV2	158	139	0.01%	0.001%
17	3.593	791	794	798	rBV	120	103	0.01%	0.001%
18	3.703	824	828	834	rBV2	218	272	0.02%	0.003%
19	3.786	846	854	895	rBV	105060	336303	24.80%	3.207%
20	4.246	981	997	1026	rBV	213333	547613	40.38%	5.221%
21	4.513	1066	1080	1095	rBV3	8569	22497	1.66%	0.215%
22	4.702	1136	1139	1141	rBV2	307	168	0.01%	0.002%
23	4.738	1146	1150	1153	rBV2	167	188	0.01%	0.002%
24	4.786	1162	1165	1169	rBV2	314	271	0.02%	0.003%
25	4.838	1176	1181	1184	rVB2	316	291	0.02%	0.003%
26	4.873	1186	1192	1195	rVV3	527	397	0.03%	0.004%
27	4.953	1201	1217	1259	rBV2	510969	1356179	100.00%	12.931%
28	5.339	1335	1337	1344	rVB4	511	585	0.04%	0.006%
29	5.381	1344	1350	1352	rVB3	382	320	0.02%	0.003%
30	5.400	1352	1356	1362	rBV2	193	322	0.02%	0.003%
31	5.448	1368	1371	1373	rBV2	182	122	0.01%	0.001%
32	5.487	1380	1383	1386	rBV	217	198	0.01%	0.002%
33	5.532	1387	1397	1432	rBV	339085	703270	51.86%	6.706%
34	5.831	1478	1490	1521	rBV2	269082	559951	41.29%	5.339%
35	5.985	1527	1538	1567	rBV2	288467	597250	44.04%	5.695%
36	6.149	1585	1589	1590	rBV3	557	386	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034593.D
 Acq On : 14 Mar 2024 11:04
 Operator : SY/MD
 Sample : P1739-04DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.284	1629	1631	1635	rVB2	331	149	0.01%	0.001%
38	6.304	1635	1637	1639	rVV	287	132	0.01%	0.001%
39	6.381	1656	1661	1663	rBV2	152	128	0.01%	0.001%
40	6.391	1663	1664	1670	rVB	250	121	0.01%	0.001%
41	6.426	1673	1675	1676	rBV2	281	108	0.01%	0.001%
42	6.571	1716	1720	1722	rBV2	282	262	0.02%	0.002%
43	6.587	1723	1725	1727	rBV2	570	328	0.02%	0.003%
44	6.686	1752	1756	1757	rBV	313	216	0.02%	0.002%
45	6.715	1763	1765	1768	rBV	301	215	0.02%	0.002%
46	6.751	1773	1776	1778	rBV2	330	273	0.02%	0.003%
47	6.911	1815	1826	1856	rBV2	149022	286357	21.11%	2.730%
48	7.243	1918	1929	1960	rBV	595885	1055779	77.85%	10.067%
49	7.554	2016	2026	2060	rBV	101127	190312	14.03%	1.815%
50	7.789	2095	2099	2101	rBV	398	257	0.02%	0.002%
51	7.821	2106	2109	2112	rBV3	275	188	0.01%	0.002%
52	7.866	2119	2123	2128	rBV4	560	713	0.05%	0.007%
53	8.024	2163	2172	2211	rBV	365064	694700	51.22%	6.624%
54	8.471	2309	2311	2313	rBV2	390	208	0.02%	0.002%
55	8.583	2343	2346	2347	rBV	248	163	0.01%	0.002%
56	8.664	2369	2371	2372	rVB	328	102	0.01%	0.001%
57	8.744	2393	2396	2398	rBV	469	304	0.02%	0.003%
58	8.783	2398	2408	2436	rVV	514225	845974	62.38%	8.066%
59	9.095	2500	2505	2509	rBV4	240	292	0.02%	0.003%
60	9.188	2531	2534	2537	rBV2	167	113	0.01%	0.001%
61	9.352	2582	2585	2590	rBV2	222	165	0.01%	0.002%
62	9.445	2611	2614	2615	rVV2	231	121	0.01%	0.001%
63	9.529	2637	2640	2642	rBV2	218	106	0.01%	0.001%
64	9.609	2662	2665	2667	rBV2	311	178	0.01%	0.002%
65	9.734	2701	2704	2711	rVB2	164	183	0.01%	0.002%
66	9.873	2745	2747	2749	rBV2	283	122	0.01%	0.001%
67	10.043	2797	2800	2803	rBV2	188	134	0.01%	0.001%
68	10.152	2822	2834	2857	rBV	374727	593868	43.79%	5.662%
69	10.320	2881	2886	2888	rBV2	814	619	0.05%	0.006%
70	10.378	2900	2904	2905	rBV	262	194	0.01%	0.002%
71	10.413	2912	2915	2918	rBV2	171	134	0.01%	0.001%
72	10.439	2920	2923	2928	rBV2	222	222	0.02%	0.002%
73	10.471	2930	2933	2935	rBV	191	134	0.01%	0.001%
74	10.529	2949	2951	2955	rVB2	231	104	0.01%	0.001%
75	10.551	2955	2958	2961	rBV2	205	144	0.01%	0.001%
76	10.670	2993	2995	2996	rBV	281	103	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034593.D
 Acq On : 14 Mar 2024 11:04
 Operator : SY/MD
 Sample : P1739-04DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.789	3027	3032	3034	rBV2	154	158	0.01%	0.002%
78	10.824	3040	3043	3045	rBV	154	106	0.01%	0.001%
79	10.853	3049	3052	3055	rBV2	372	226	0.02%	0.002%
80	10.873	3055	3058	3062	rBV3	396	350	0.03%	0.003%
81	10.895	3062	3065	3068	rVB2	353	184	0.01%	0.002%
82	11.133	3136	3139	3141	rBV3	244	146	0.01%	0.001%
83	11.185	3144	3155	3179	rVV	504085	799232	58.93%	7.621%
84	11.496	3249	3252	3254	rBV	396	219	0.02%	0.002%
85	11.558	3259	3271	3302	rVV	581786	916447	67.58%	8.738%
86	11.779	3338	3340	3345	rVB2	359	204	0.02%	0.002%
87	11.802	3345	3347	3352	rVB3	643	515	0.04%	0.005%
88	11.837	3352	3358	3361	rBV2	256	284	0.02%	0.003%
89	11.979	3399	3402	3404	rBV2	195	116	0.01%	0.001%
90	12.561	3580	3583	3584	rBV	208	116	0.01%	0.001%
91	12.593	3591	3593	3597	rBV2	277	214	0.02%	0.002%
92	12.622	3600	3602	3607	rVB3	373	155	0.01%	0.001%
93	12.676	3616	3619	3624	rBV3	324	281	0.02%	0.003%
94	12.995	3715	3718	3721	rVB	375	200	0.01%	0.002%
95	13.294	3808	3811	3814	rBV2	436	267	0.02%	0.003%
96	13.737	3946	3949	3953	rBV3	399	290	0.02%	0.003%
97	13.956	4015	4017	4019	rBV2	275	157	0.01%	0.001%
98	14.017	4033	4036	4038	rBV2	371	231	0.02%	0.002%
99	14.172	4081	4084	4087	rBV2	536	367	0.03%	0.003%
100	14.329	4129	4133	4136	rBV3	562	523	0.04%	0.005%




Sum of corrected areas: 10487750

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034593.D
Acq On : 14 Mar 2024 11:04
Operator : SY/MD
Sample : P1739-04DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

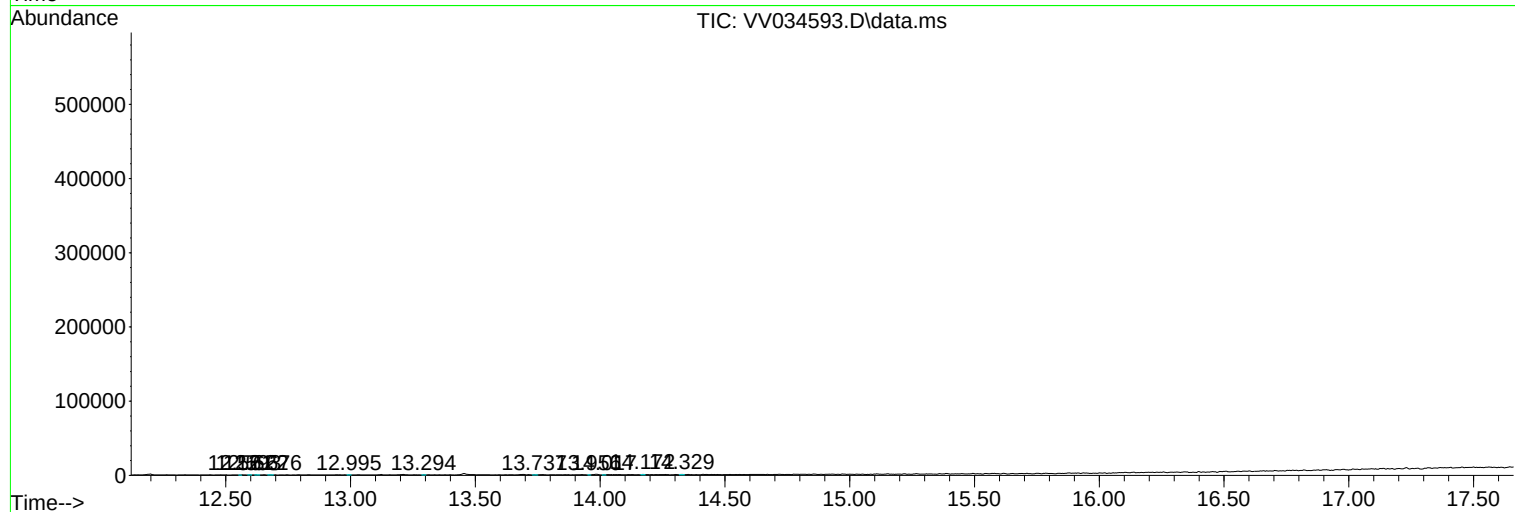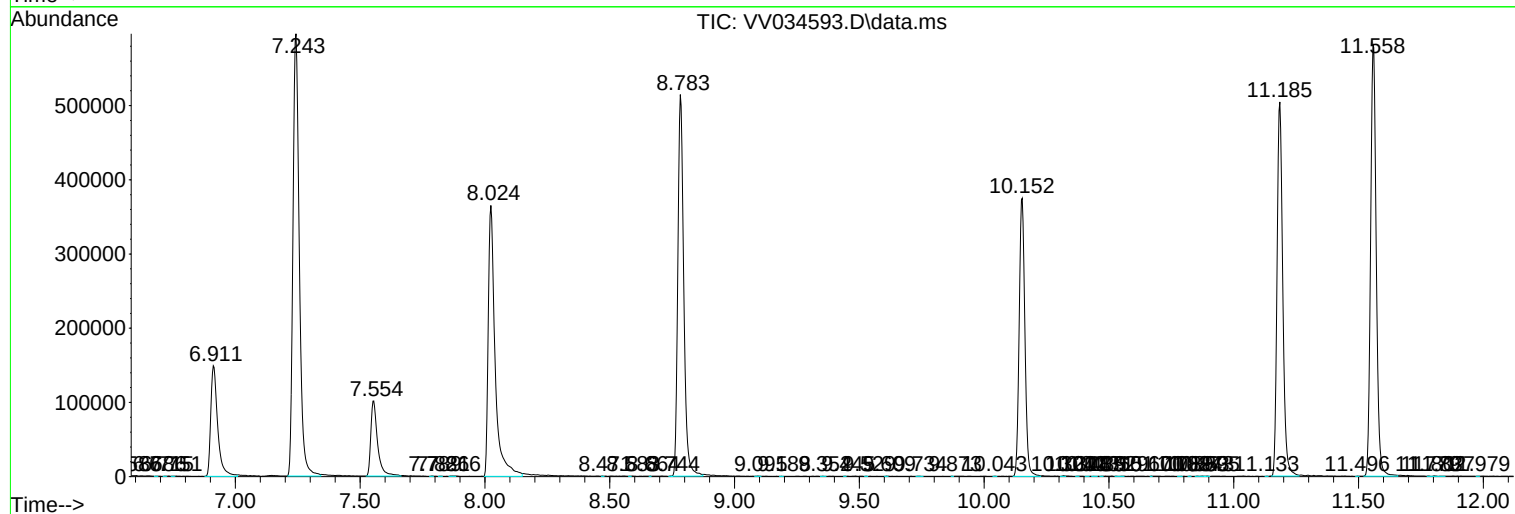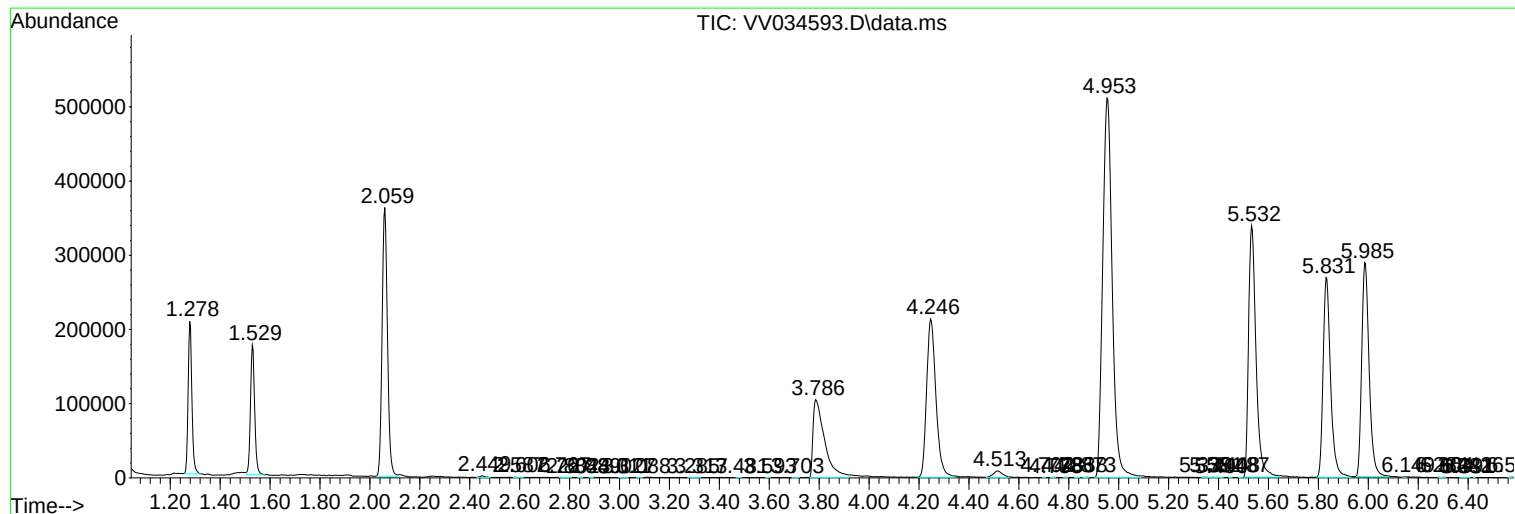

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034593.D
Acq On : 14 Mar 2024 11:04
Operator : SY/MD
Sample : P1739-04DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034593.D
Acq On : 14 Mar 2024 11:04
Operator : SY/MD
Sample : P1739-04DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------