

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034595.D
 Acq On : 14 Mar 2024 11:52
 Operator : SY/MD
 Sample : P1739-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034595.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	209149	222152	16.36%	2.220%
2	1.529	146	152	172	rVB	181010	212118	15.62%	2.120%
3	2.060	306	317	331	rBV	349048	509419	37.50%	5.092%
4	2.262	365	380	382	rBV4	6791	12943	0.95%	0.129%
5	2.497	450	453	455	rBV2	222	124	0.01%	0.001%
6	2.700	513	516	519	rBV3	273	174	0.01%	0.002%
7	2.844	559	561	562	rBV	275	69	0.01%	0.001%
8	2.925	585	586	590	rVB	197	72	0.01%	0.001%
9	2.950	590	594	598	rBV2	273	284	0.02%	0.003%
10	3.121	645	647	649	rBV	172	80	0.01%	0.001%
11	3.188	665	668	670	rBV2	152	83	0.01%	0.001%
12	3.388	728	730	733	rBV2	317	119	0.01%	0.001%
13	3.584	790	791	793	rVB	248	62	0.00%	0.001%
14	3.603	793	797	801	rBV	183	172	0.01%	0.002%
15	3.632	804	806	807	rBV	193	92	0.01%	0.001%
16	3.712	828	831	834	rBV	224	143	0.01%	0.001%
17	3.732	834	837	842	rBV2	172	151	0.01%	0.002%
18	3.786	846	854	892	rBV	101358	286773	21.11%	2.866%
19	4.246	981	997	1023	rBV2	211112	541175	39.84%	5.409%
20	4.654	1120	1124	1128	rVB3	357	311	0.02%	0.003%
21	4.677	1129	1131	1135	rVB2	166	105	0.01%	0.001%
22	4.699	1135	1138	1140	rBV2	180	100	0.01%	0.001%
23	4.725	1140	1146	1148	rBV2	247	229	0.02%	0.002%
24	4.761	1155	1157	1159	rBV	199	122	0.01%	0.001%
25	4.825	1174	1177	1180	rBV3	286	207	0.02%	0.002%
26	4.844	1180	1183	1187	rBV3	189	131	0.01%	0.001%
27	4.860	1187	1188	1189	rBV	192	40	0.00%	0.000%
28	4.892	1196	1198	1201	rVB2	206	70	0.01%	0.001%
29	4.953	1201	1217	1255	rBV2	512720	1358276	100.00%	13.576%
30	5.333	1334	1335	1336	rBV	248	56	0.00%	0.001%
31	5.365	1343	1345	1348	rBV2	257	164	0.01%	0.002%
32	5.429	1363	1365	1367	rBV	288	139	0.01%	0.001%
33	5.471	1375	1378	1379	rBV2	264	145	0.01%	0.001%
34	5.532	1386	1397	1435	rBV	353285	743562	54.74%	7.432%
35	5.834	1481	1491	1516	rVB8	21288	52244	3.85%	0.522%
36	5.989	1526	1539	1565	rBV	288680	599842	44.16%	5.996%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034595.D
 Acq On : 14 Mar 2024 11:52
 Operator : SY/MD
 Sample : P1739-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.304	1636	1637	1639	rVB	356	84	0.01%	0.001%
38	6.355	1651	1653	1657	rVB2	199	81	0.01%	0.001%
39	6.375	1657	1659	1663	rVB2	217	122	0.01%	0.001%
40	6.407	1666	1669	1670	rBV	165	99	0.01%	0.001%
41	6.436	1675	1678	1680	rBV2	158	110	0.01%	0.001%
42	6.548	1710	1713	1717	rBV	171	133	0.01%	0.001%
43	6.596	1720	1728	1731	rBV4	1152	1597	0.12%	0.016%
44	6.825	1798	1799	1800	rBV	85	20	0.00%	0.000%
45	6.857	1807	1809	1810	rBV	273	115	0.01%	0.001%
46	6.912	1815	1826	1861	rBV	149264	287585	21.17%	2.875%
47	7.137	1892	1896	1898	rBV3	1038	880	0.06%	0.009%
48	7.243	1918	1929	1958	rBV	594483	1050810	77.36%	10.503%
49	7.555	2016	2026	2054	rBV	100583	187085	13.77%	1.870%
50	7.748	2084	2086	2088	rVB2	624	300	0.02%	0.003%
51	7.828	2107	2111	2115	rBV3	282	280	0.02%	0.003%
52	7.973	2153	2156	2158	rBV2	204	133	0.01%	0.001%
53	7.982	2158	2159	2160	rVB	207	40	0.00%	0.000%
54	8.024	2163	2172	2212	rBV	363203	694478	51.13%	6.942%
55	8.571	2340	2342	2344	rBV	128	56	0.00%	0.001%
56	8.619	2353	2357	2358	rBV	260	178	0.01%	0.002%
57	8.638	2361	2363	2368	rVV2	458	247	0.02%	0.002%
58	8.677	2372	2375	2380	rVV2	645	481	0.04%	0.005%
59	8.696	2380	2381	2385	rVB3	360	184	0.01%	0.002%
60	8.783	2397	2408	2435	rBV	535645	883743	65.06%	8.833%
61	9.030	2481	2485	2487	rBV3	311	248	0.02%	0.002%
62	9.143	2517	2520	2526	rVB3	344	272	0.02%	0.003%
63	9.172	2528	2529	2531	rBV	250	90	0.01%	0.001%
64	9.230	2543	2547	2550	rVB3	232	190	0.01%	0.002%
65	9.310	2570	2572	2573	rBV	220	104	0.01%	0.001%
66	9.423	2605	2607	2610	rVB	307	144	0.01%	0.001%
67	9.439	2610	2612	2614	rBV	127	76	0.01%	0.001%
68	9.510	2631	2634	2637	rVB2	473	274	0.02%	0.003%
69	9.526	2637	2639	2641	rBV2	86	51	0.00%	0.001%
70	9.561	2647	2650	2654	rBV	160	125	0.01%	0.001%
71	9.715	2697	2698	2700	rVB	258	69	0.01%	0.001%
72	9.786	2713	2720	2724	rBV2	287	369	0.03%	0.004%
73	9.805	2725	2726	2728	rVV2	143	61	0.00%	0.001%
74	9.870	2744	2746	2749	rVB	247	118	0.01%	0.001%
75	9.895	2752	2754	2760	rBV3	536	286	0.02%	0.003%
76	10.153	2815	2834	2850	rBV	370222	595640	43.85%	5.954%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034595.D
 Acq On : 14 Mar 2024 11:52
 Operator : SY/MD
 Sample : P1739-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.326	2882	2888	2898	rVB6	2177	2824	0.21%	0.028%
78	10.368	2898	2901	2902	rBV	209	105	0.01%	0.001%
79	10.561	2959	2961	2964	rVB2	225	117	0.01%	0.001%
80	10.583	2964	2968	2973	rBV2	190	248	0.02%	0.002%
81	10.603	2973	2974	2981	rVB3	388	226	0.02%	0.002%
82	10.635	2982	2984	2988	rBV	244	169	0.01%	0.002%
83	10.802	3033	3036	3038	rBV	469	284	0.02%	0.003%
84	10.889	3059	3063	3069	rBV2	271	305	0.02%	0.003%
85	10.937	3075	3078	3081	rBV	289	194	0.01%	0.002%
86	10.979	3089	3091	3096	rVB3	331	207	0.02%	0.002%
87	11.133	3136	3139	3142	rBV3	365	261	0.02%	0.003%
88	11.185	3145	3155	3177	rBV	534195	829773	61.09%	8.294%
89	11.403	3220	3223	3226	rBV2	400	242	0.02%	0.002%
90	11.419	3226	3228	3233	rVV3	430	380	0.03%	0.004%
91	11.558	3258	3271	3306	rBV	575047	918961	67.66%	9.185%
92	11.976	3399	3401	3407	rBV2	228	102	0.01%	0.001%
93	12.059	3423	3427	3429	rBV	303	220	0.02%	0.002%
94	12.297	3499	3501	3503	rBV	291	139	0.01%	0.001%
95	12.988	3714	3716	3723	rBV2	338	323	0.02%	0.003%
96	13.599	3902	3906	3908	rBV3	415	314	0.02%	0.003%
97	14.152	4076	4078	4084	rVB4	530	324	0.02%	0.003%




Sum of corrected areas: 10004624

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034595.D
Acq On : 14 Mar 2024 11:52
Operator : SY/MD
Sample : P1739-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

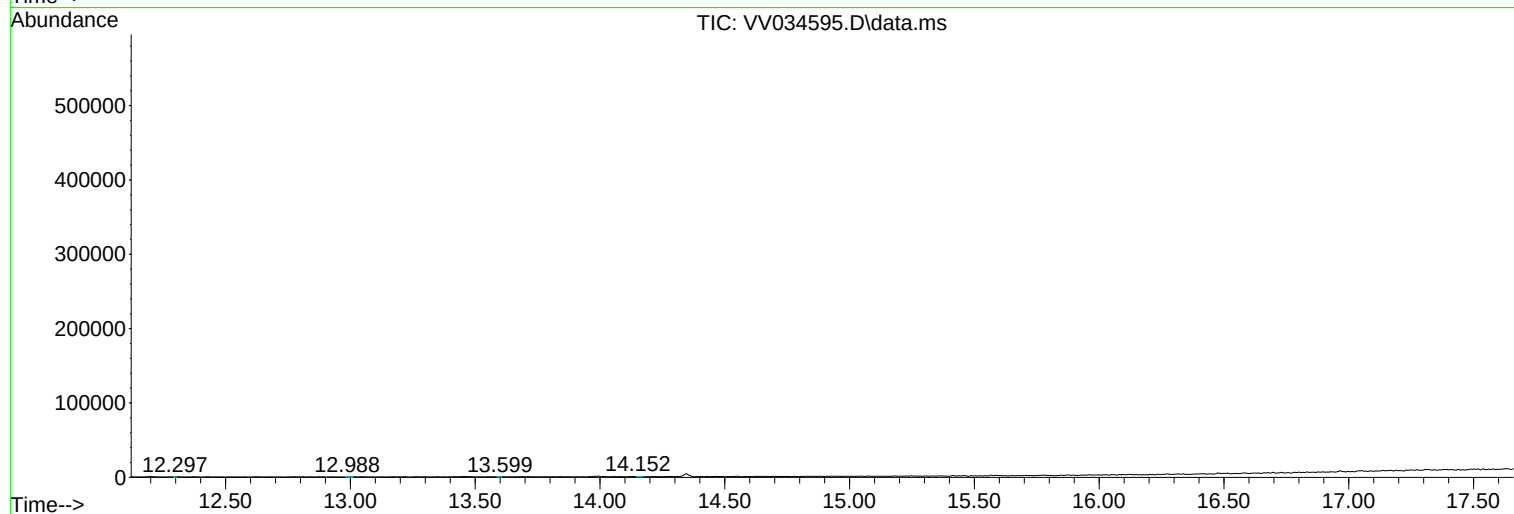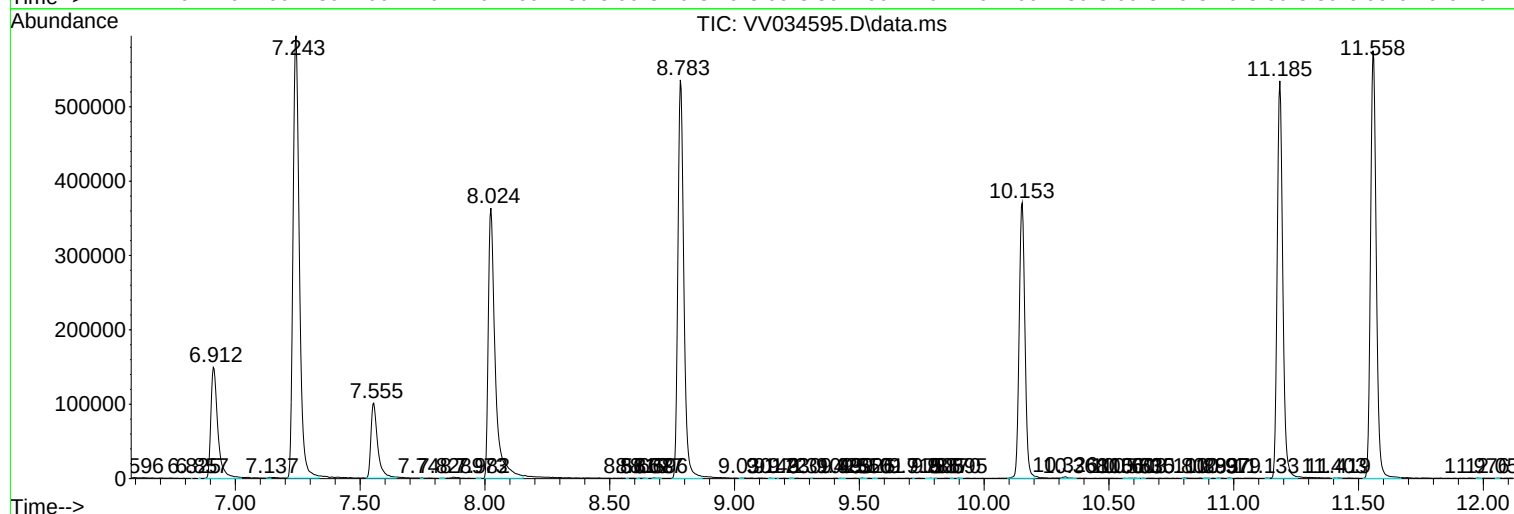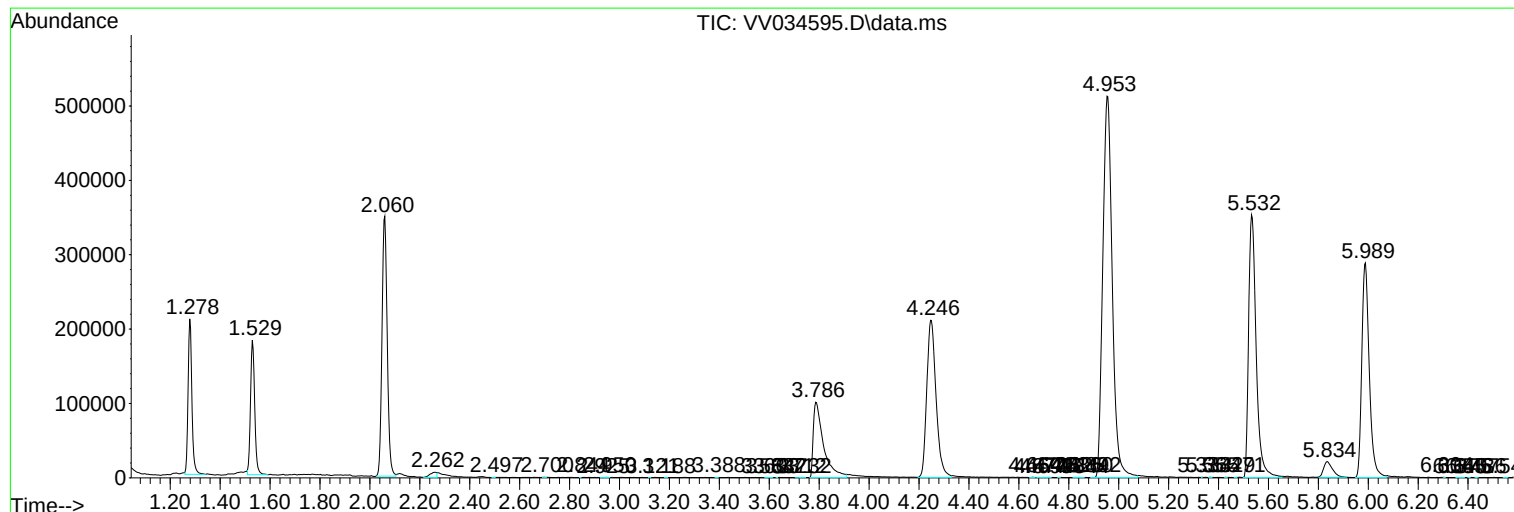

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034595.D
Acq On : 14 Mar 2024 11:52
Operator : SY/MD
Sample : P1739-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034595.D
Acq On : 14 Mar 2024 11:52
Operator : SY/MD
Sample : P1739-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------