

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034600.D
 Acq On : 14 Mar 2024 13:51
 Operator : SY/MD
 Sample : P1739-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034600.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	204438	212644	15.73%	2.149%
2	1.529	145	152	166	rVB	169821	199056	14.72%	2.011%
3	2.060	307	317	333	rBV	344107	500302	37.00%	5.055%
4	2.246	367	375	385	rBV	8012	17364	1.28%	0.175%
5	2.442	433	436	437	rBV	1223	709	0.05%	0.007%
6	2.828	550	556	559	rBV2	220	262	0.02%	0.003%
7	2.925	584	586	587	rBV	208	91	0.01%	0.001%
8	3.027	616	618	623	rBV2	261	217	0.02%	0.002%
9	3.085	635	636	637	rVB2	105	20	0.00%	0.000%
10	3.146	653	655	656	rVB	148	43	0.00%	0.000%
11	3.172	656	663	666	rBV2	215	232	0.02%	0.002%
12	3.220	674	678	681	rBV	192	133	0.01%	0.001%
13	3.310	705	706	708	rVB	140	36	0.00%	0.000%
14	3.339	712	715	717	rBB	112	56	0.00%	0.001%
15	3.362	718	722	725	rBV2	186	143	0.01%	0.001%
16	3.407	730	736	742	rBV2	250	280	0.02%	0.003%
17	3.526	771	773	775	rBV	95	52	0.00%	0.001%
18	3.600	793	796	800	rBV2	216	135	0.01%	0.001%
19	3.638	807	808	810	rVB	128	47	0.00%	0.000%
20	3.674	817	819	822	rBV	149	105	0.01%	0.001%
21	3.786	846	854	893	rBV	100765	280915	20.77%	2.838%
22	4.249	981	998	1028	rBV	209995	547696	40.50%	5.534%
23	4.580	1097	1101	1102	rBV2	366	244	0.02%	0.002%
24	4.616	1108	1112	1117	rBV3	388	430	0.03%	0.004%
25	4.706	1137	1140	1143	rBV2	121	91	0.01%	0.001%
26	4.722	1143	1145	1146	rBV2	167	80	0.01%	0.001%
27	4.761	1154	1157	1161	rVB2	368	212	0.02%	0.002%
28	4.953	1200	1217	1247	rBV2	510738	1352199	100.00%	13.663%
29	5.442	1368	1369	1371	rVB2	169	56	0.00%	0.001%
30	5.458	1373	1374	1375	rVV	116	26	0.00%	0.000%
31	5.474	1377	1379	1381	rBV	99	57	0.00%	0.001%
32	5.532	1386	1397	1431	rBV	339431	713140	52.74%	7.206%
33	5.838	1479	1492	1520	rVB8	25547	65596	4.85%	0.663%
34	5.989	1526	1539	1578	rBV	294018	611483	45.22%	6.179%
35	6.262	1622	1624	1625	rBV	520	176	0.01%	0.002%
36	6.336	1642	1647	1649	rBV2	294	210	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034600.D
 Acq On : 14 Mar 2024 13:51
 Operator : SY/MD
 Sample : P1739-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.355	1651	1653	1660	rVB	355	260	0.02%	0.003%
38	6.465	1682	1687	1690	rBV	138	168	0.01%	0.002%
39	6.481	1690	1692	1693	rVV	157	54	0.00%	0.001%
40	6.494	1694	1696	1699	rVB	217	115	0.01%	0.001%
41	6.596	1719	1728	1730	rBV3	989	1537	0.11%	0.016%
42	6.844	1802	1805	1808	rVB2	386	195	0.01%	0.002%
43	6.915	1816	1827	1850	rBV	148218	280547	20.75%	2.835%
44	7.098	1881	1884	1886	rBV	291	202	0.01%	0.002%
45	7.243	1918	1929	1957	rBV	597072	1050989	77.72%	10.619%
46	7.555	2016	2026	2056	rBV	100230	186082	13.76%	1.880%
47	7.815	2106	2107	2108	rBV	150	45	0.00%	0.000%
48	7.831	2108	2112	2116	rVB2	342	259	0.02%	0.003%
49	7.860	2118	2121	2122	rBV	219	129	0.01%	0.001%
50	7.940	2143	2146	2148	rBV	145	99	0.01%	0.001%
51	7.969	2153	2155	2157	rBV3	212	127	0.01%	0.001%
52	8.024	2163	2172	2209	rBV	362174	679317	50.24%	6.864%
53	8.522	2324	2327	2329	rBV	324	184	0.01%	0.002%
54	8.590	2346	2348	2353	rVB2	332	256	0.02%	0.003%
55	8.619	2355	2357	2360	rBV	170	82	0.01%	0.001%
56	8.648	2360	2366	2370	rBV2	394	400	0.03%	0.004%
57	8.690	2374	2379	2381	rBV2	267	280	0.02%	0.003%
58	8.783	2393	2408	2432	rBV	515695	850471	62.90%	8.593%
59	9.072	2496	2498	2504	rVB3	288	253	0.02%	0.003%
60	9.098	2504	2506	2508	rBV	167	67	0.00%	0.001%
61	9.149	2520	2522	2526	rVB2	243	116	0.01%	0.001%
62	9.191	2530	2535	2536	rBV2	336	266	0.02%	0.003%
63	9.355	2581	2586	2590	rBV2	249	231	0.02%	0.002%
64	9.371	2590	2591	2592	rBV2	174	63	0.00%	0.001%
65	9.477	2622	2624	2627	rVB	209	70	0.01%	0.001%
66	9.493	2627	2629	2632	rBV2	348	145	0.01%	0.001%
67	9.754	2708	2710	2712	rBV	179	65	0.00%	0.001%
68	9.899	2753	2755	2756	rVB	174	48	0.00%	0.000%
69	10.153	2822	2834	2856	rBV	383085	597520	44.19%	6.038%
70	10.326	2884	2888	2894	rVB2	386	464	0.03%	0.005%
71	10.362	2896	2899	2904	rBV	290	172	0.01%	0.002%
72	10.452	2924	2927	2929	rBV2	146	79	0.01%	0.001%
73	10.509	2944	2945	2946	rBV	309	71	0.01%	0.001%
74	10.558	2957	2960	2962	rBV	253	162	0.01%	0.002%
75	10.632	2981	2983	2985	rBV	172	105	0.01%	0.001%
76	10.731	3012	3014	3016	rVB2	309	75	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034600.D
 Acq On : 14 Mar 2024 13:51
 Operator : SY/MD
 Sample : P1739-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	11.014	3100	3102	3103	rBV	243	80	0.01%	0.001%
78	11.101	3127	3129	3133	rBV2	196	169	0.01%	0.002%
79	11.185	3144	3155	3180	rBV	517261	810811	59.96%	8.193%
80	11.432	3227	3232	3234	rBV3	452	311	0.02%	0.003%
81	11.464	3239	3242	3244	rBV	308	207	0.02%	0.002%
82	11.561	3260	3272	3297	rBV	594116	927599	68.60%	9.373%
83	11.927	3384	3386	3389	rBV2	326	192	0.01%	0.002%
84	11.947	3389	3392	3396	rVB2	245	127	0.01%	0.001%
85	12.181	3463	3465	3466	rBV	357	160	0.01%	0.002%
86	13.307	3813	3815	3816	rBV	312	139	0.01%	0.001%
87	13.506	3875	3877	3882	rBV3	343	177	0.01%	0.002%
88	13.750	3950	3953	3956	rBV2	350	296	0.02%	0.003%
89	13.876	3988	3992	3993	rBV2	326	231	0.02%	0.002%



Sum of corrected areas: 9896807

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034600.D
Acq On : 14 Mar 2024 13:51
Operator : SY/MD
Sample : P1739-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

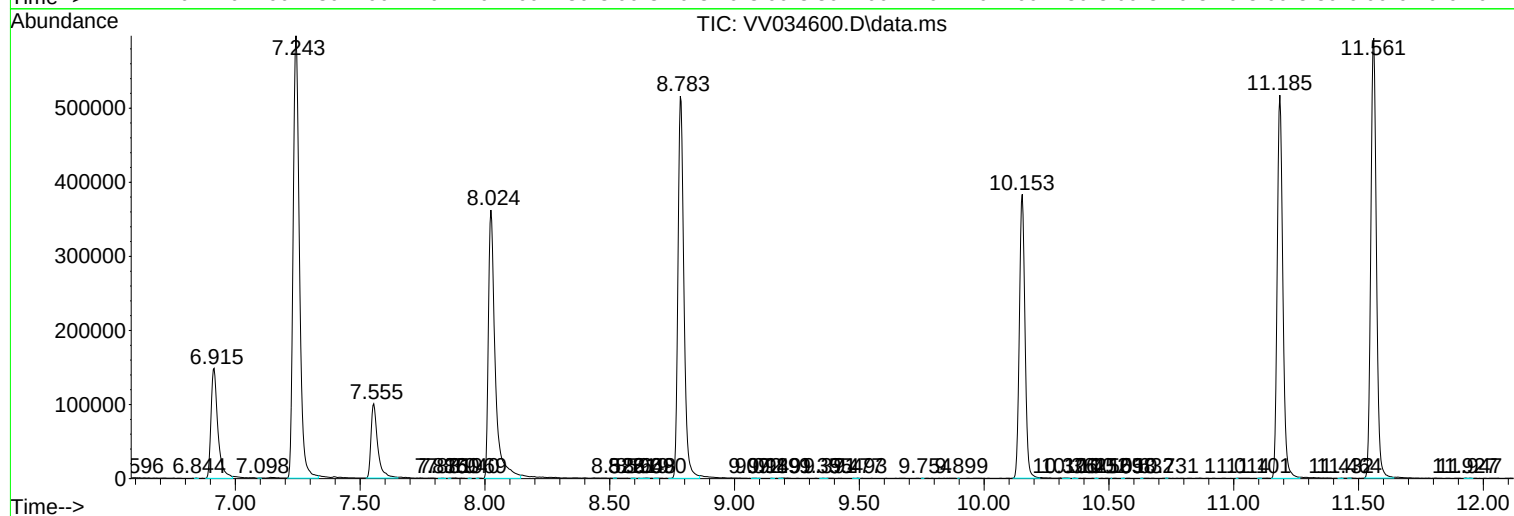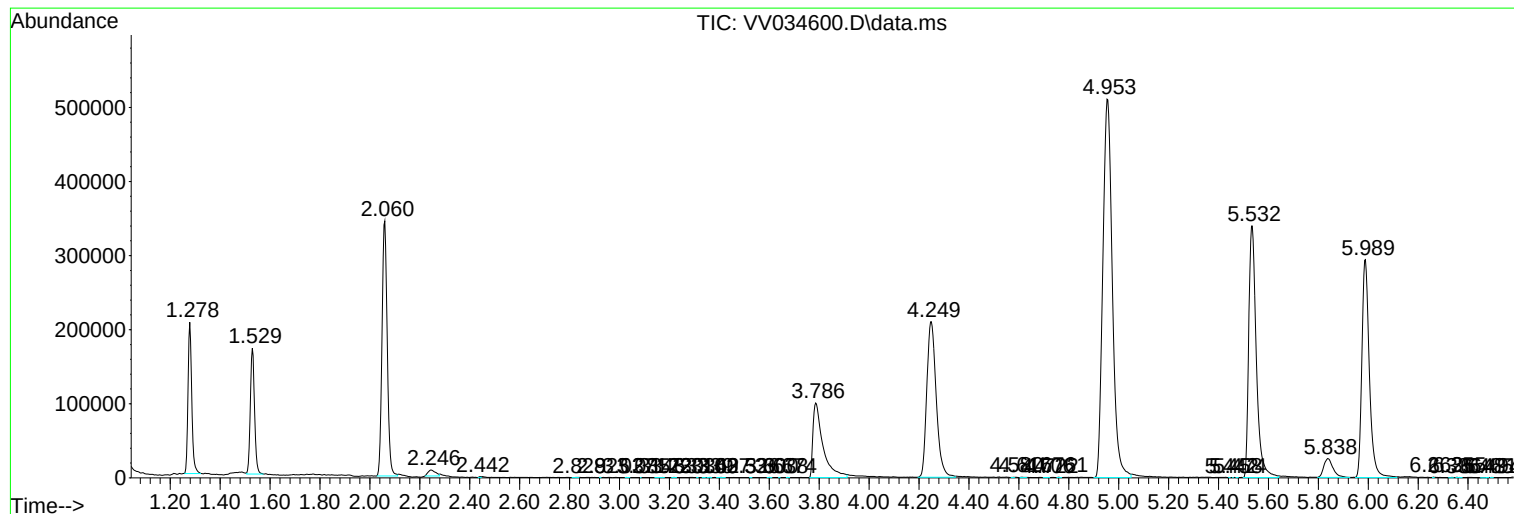

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034600.D
Acq On : 14 Mar 2024 13:51
Operator : SY/MD
Sample : P1739-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034600.D
Acq On : 14 Mar 2024 13:51
Operator : SY/MD
Sample : P1739-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------