

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034602.D
 Acq On : 14 Mar 2024 14:39
 Operator : SY/MD
 Sample : P1740-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034602.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	197199	211581	15.90%	2.165%
2	1.532	146	153	173	rVB	171867	197939	14.88%	2.026%
3	2.059	307	317	333	rBV	336540	489009	36.76%	5.004%
4	2.571	474	476	479	rBV	355	155	0.01%	0.002%
5	2.584	479	480	482	rVB	273	91	0.01%	0.001%
6	2.600	482	485	486	rBV	198	98	0.01%	0.001%
7	2.667	502	506	508	rBV3	333	214	0.02%	0.002%
8	2.703	512	517	519	rBV2	471	392	0.03%	0.004%
9	2.873	567	570	572	rBV2	160	109	0.01%	0.001%
10	2.992	604	607	615	rBV2	250	371	0.03%	0.004%
11	3.220	676	678	680	rVB	180	58	0.00%	0.001%
12	3.236	680	683	685	rBV	260	169	0.01%	0.002%
13	3.265	690	692	696	rBV2	278	142	0.01%	0.001%
14	3.416	735	739	742	rBV2	149	131	0.01%	0.001%
15	3.574	786	788	792	rBV2	123	90	0.01%	0.001%
16	3.593	792	794	796	rVB	139	62	0.00%	0.001%
17	3.609	797	799	801	rBV2	138	71	0.01%	0.001%
18	3.635	803	807	810	rBV2	150	152	0.01%	0.002%
19	3.744	838	841	843	rBV	210	126	0.01%	0.001%
20	3.760	843	846	848	rBV2	198	153	0.01%	0.002%
21	3.796	848	857	896	rBV	92043	278395	20.93%	2.849%
22	4.249	982	998	1029	rBV	207482	534557	40.18%	5.470%
23	4.731	1145	1148	1149	rBV2	254	146	0.01%	0.001%
24	4.773	1158	1161	1162	rBV2	222	139	0.01%	0.001%
25	4.805	1168	1171	1173	rBV	191	144	0.01%	0.001%
26	4.956	1199	1218	1255	rBV2	502367	1330334	100.00%	13.614%
27	5.265	1312	1314	1317	rBV	419	186	0.01%	0.002%
28	5.333	1331	1335	1341	rBV3	335	395	0.03%	0.004%
29	5.403	1355	1357	1361	rBV	238	148	0.01%	0.002%
30	5.532	1383	1397	1428	rBV	351320	730402	54.90%	7.475%
31	5.831	1480	1490	1516	rVB3	10229	24680	1.86%	0.253%
32	5.989	1526	1539	1569	rBV	287150	594854	44.71%	6.087%
33	6.201	1603	1605	1607	rBV3	340	184	0.01%	0.002%
34	6.329	1642	1645	1648	rBV	107	96	0.01%	0.001%
35	6.452	1681	1683	1686	rVB	209	69	0.01%	0.001%
36	6.554	1710	1715	1717	rBV2	172	172	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034602.D
 Acq On : 14 Mar 2024 14:39
 Operator : SY/MD
 Sample : P1740-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.606	1719	1731	1733	rBV5	892	1815	0.14%	0.019%
38	6.757	1775	1778	1779	rBV	165	110	0.01%	0.001%
39	6.860	1805	1810	1812	rBV2	177	170	0.01%	0.002%
40	6.915	1815	1827	1849	rBV	143912	276593	20.79%	2.831%
41	7.146	1891	1899	1908	rBV4	1085	1927	0.14%	0.020%
42	7.243	1918	1929	1965	rBV	580281	1030866	77.49%	10.549%
43	7.554	2017	2026	2051	rBV	97355	177177	13.32%	1.813%
44	7.844	2114	2116	2117	rBV	238	129	0.01%	0.001%
45	7.921	2138	2140	2143	rVB2	251	96	0.01%	0.001%
46	7.982	2157	2159	2161	rVB	167	46	0.00%	0.000%
47	8.024	2163	2172	2219	rBV	347076	674202	50.68%	6.899%
48	8.538	2330	2332	2334	rBV2	161	90	0.01%	0.001%
49	8.554	2334	2337	2339	rBV2	330	179	0.01%	0.002%
50	8.567	2339	2341	2345	rVB2	280	244	0.02%	0.002%
51	8.689	2376	2379	2380	rBV2	429	221	0.02%	0.002%
52	8.783	2397	2408	2443	rBV	516088	875133	65.78%	8.956%
53	9.085	2500	2502	2504	rVB	269	71	0.01%	0.001%
54	9.098	2504	2506	2508	rBV	235	112	0.01%	0.001%
55	9.291	2562	2566	2570	rBV2	222	203	0.02%	0.002%
56	9.374	2586	2592	2594	rBV2	226	206	0.02%	0.002%
57	9.503	2630	2632	2636	rBV2	155	106	0.01%	0.001%
58	9.625	2666	2670	2674	rBV2	187	181	0.01%	0.002%
59	9.693	2689	2691	2695	rBV2	454	211	0.02%	0.002%
60	9.799	2719	2724	2729	rBV2	228	299	0.02%	0.003%
61	10.111	2817	2821	2822	rBV2	711	400	0.03%	0.004%
62	10.152	2822	2834	2852	rVV	367503	584946	43.97%	5.986%
63	10.326	2882	2888	2894	rBV4	1134	1742	0.13%	0.018%
64	10.448	2924	2926	2931	rVB2	168	82	0.01%	0.001%
65	10.513	2944	2946	2950	rVB2	271	141	0.01%	0.001%
66	10.551	2956	2958	2961	rBV2	242	172	0.01%	0.002%
67	10.638	2983	2985	2988	rBV2	218	82	0.01%	0.001%
68	10.779	3026	3029	3036	rVB2	294	258	0.02%	0.003%
69	10.808	3036	3038	3039	rBV2	166	51	0.00%	0.001%
70	11.146	3142	3143	3144	rBV	170	49	0.00%	0.001%
71	11.185	3144	3155	3181	rBV	533003	833127	62.63%	8.526%
72	11.484	3245	3248	3249	rBV	283	133	0.01%	0.001%
73	11.557	3260	3271	3299	rBV	571592	911644	68.53%	9.329%
74	12.027	3416	3417	3418	rBV	310	65	0.00%	0.001%
75	12.162	3455	3459	3463	rBV2	323	314	0.02%	0.003%
76	12.246	3482	3485	3488	rBV2	353	193	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034602.D
Acq On : 14 Mar 2024 14:39
Operator : SY/MD
Sample : P1740-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

77	12.390	3527	3530	3533	rVB	305	163	0.01%	0.002%
78	12.580	3588	3589	3592	rBV2	243	161	0.01%	0.002%
79	12.799	3655	3657	3658	rBV	283	79	0.01%	0.001%
80	12.895	3685	3687	3689	rBV	303	135	0.01%	0.001%
81	13.255	3798	3799	3802	rVB	210	98	0.01%	0.001%
82	14.342	4133	4137	4143	rBV8	1282	1375	0.10%	0.014%




Sum of corrected areas: 9771811

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034602.D
Acq On : 14 Mar 2024 14:39
Operator : SY/MD
Sample : P1740-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

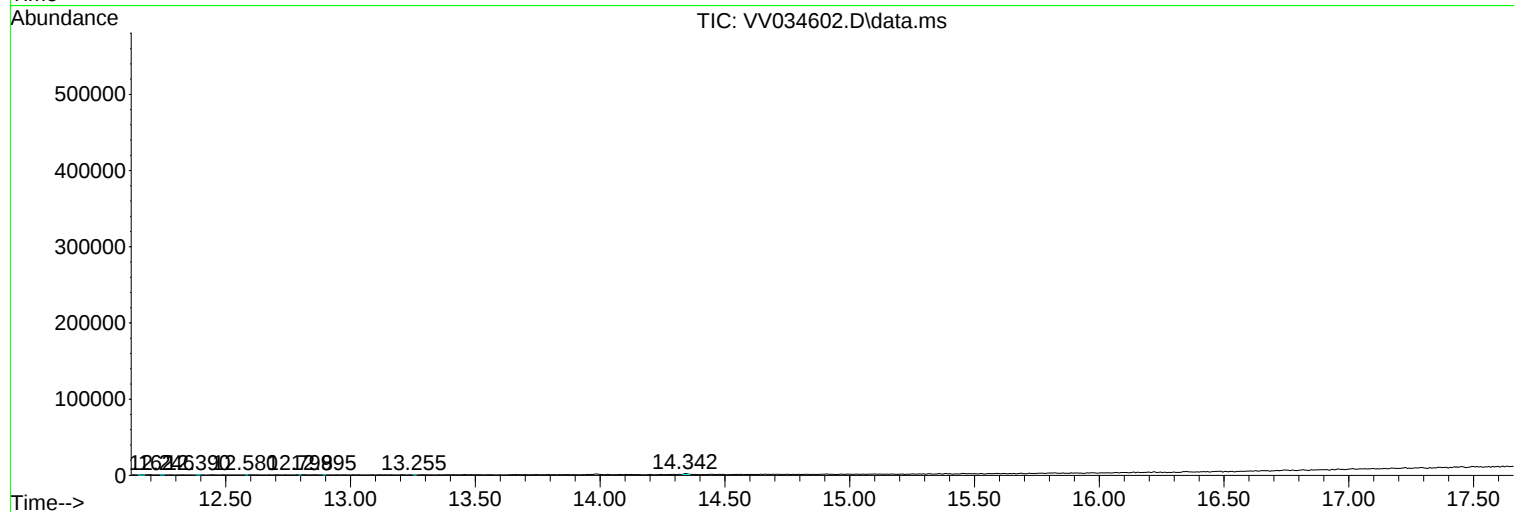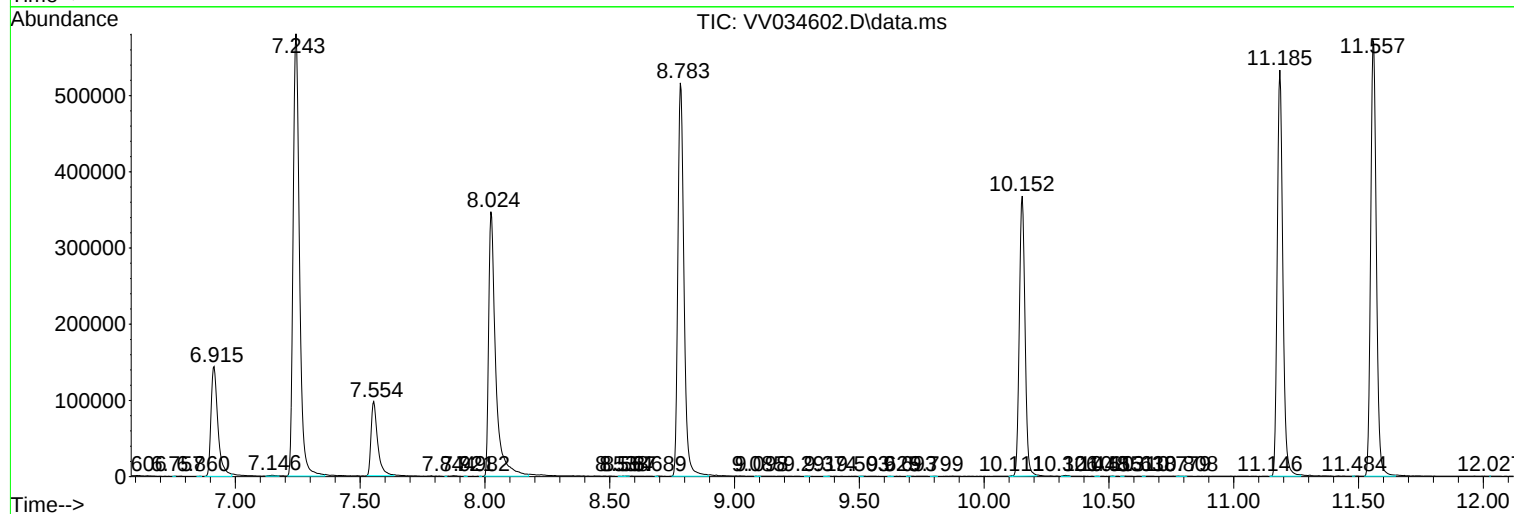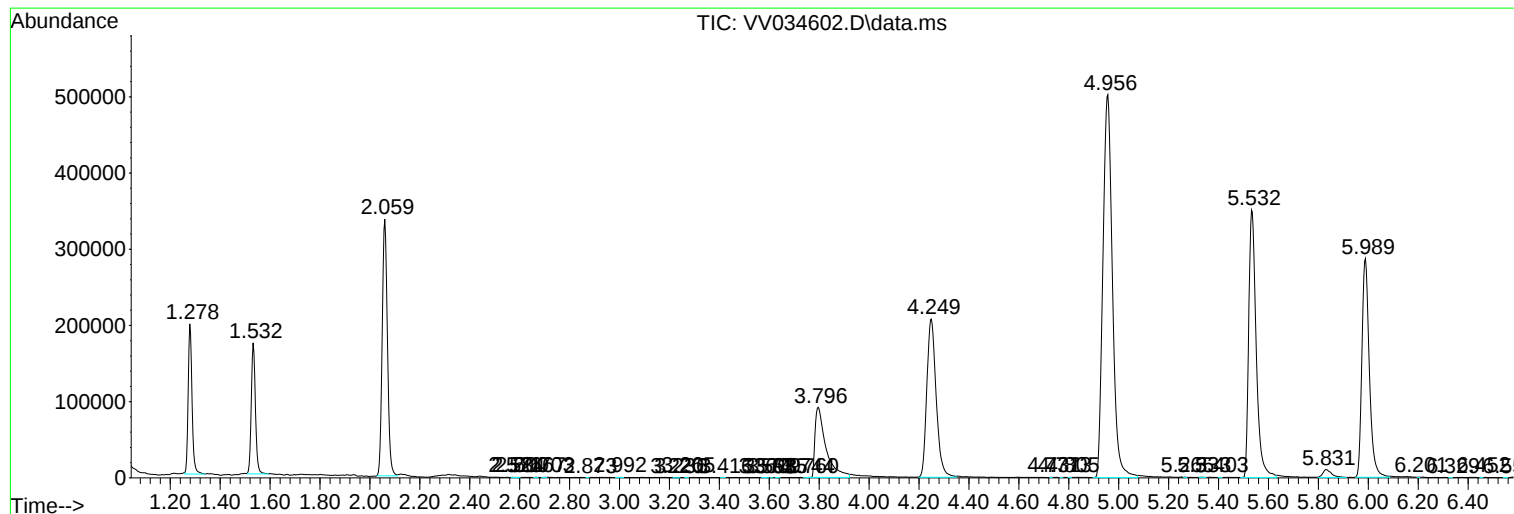

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034602.D
Acq On : 14 Mar 2024 14:39
Operator : SY/MD
Sample : P1740-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034602.D
Acq On : 14 Mar 2024 14:39
Operator : SY/MD
Sample : P1740-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------