

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034606.D
 Acq On : 14 Mar 2024 16:15
 Operator : SY/MD
 Sample : P1728-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B75DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	204584	213380	14.63%	2.015%
2	1.532	146	153	166	rVB	174221	198894	13.64%	1.878%
3	2.060	306	317	333	rBV	344653	508355	34.86%	4.801%
4	2.227	367	369	370	rBV	622	245	0.02%	0.002%
5	2.320	392	398	400	rBV3	365	344	0.02%	0.003%
6	2.416	426	428	430	rBV	235	123	0.01%	0.001%
7	2.449	430	438	448	rVB6	2827	4504	0.31%	0.043%
8	2.497	448	453	456	rBV2	323	370	0.03%	0.003%
9	2.523	459	461	465	rBV2	306	176	0.01%	0.002%
10	2.712	518	520	522	rBV2	283	168	0.01%	0.002%
11	2.767	532	537	538	rBV	170	139	0.01%	0.001%
12	2.876	567	571	574	rBV2	303	185	0.01%	0.002%
13	3.124	644	648	651	rBV2	187	152	0.01%	0.001%
14	3.156	655	658	662	rVV2	382	239	0.02%	0.002%
15	3.240	682	684	686	rBV	277	135	0.01%	0.001%
16	3.375	723	726	728	rBV	203	116	0.01%	0.001%
17	3.404	734	735	738	rVB	250	122	0.01%	0.001%
18	3.452	747	750	753	rBV	226	191	0.01%	0.002%
19	3.532	772	775	779	rVB	187	122	0.01%	0.001%
20	3.584	789	791	798	rVB2	252	176	0.01%	0.002%
21	3.796	848	857	894	rBV	98034	298286	20.45%	2.817%
22	4.246	982	997	1034	rBV	219834	565148	38.75%	5.337%
23	4.461	1061	1064	1066	rBV2	589	326	0.02%	0.003%
24	4.590	1102	1104	1108	rBV3	279	208	0.01%	0.002%
25	4.706	1136	1140	1141	rBV	260	186	0.01%	0.002%
26	4.773	1156	1161	1164	rVB2	234	242	0.02%	0.002%
27	4.796	1164	1168	1169	rBV2	171	119	0.01%	0.001%
28	4.821	1174	1176	1178	rBV2	312	120	0.01%	0.001%
29	4.883	1192	1195	1197	rBV	197	125	0.01%	0.001%
30	4.953	1201	1217	1259	rBV2	533478	1458467	100.00%	13.774%
31	5.413	1357	1360	1362	rBV2	450	306	0.02%	0.003%
32	5.461	1371	1375	1378	rBV2	319	334	0.02%	0.003%
33	5.532	1386	1397	1423	rBV	363738	746949	51.21%	7.054%
34	5.834	1480	1491	1515	rVB3	11878	27711	1.90%	0.262%
35	5.985	1526	1538	1575	rBV	300333	641298	43.97%	6.056%
36	6.265	1623	1625	1627	rBV2	361	146	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034606.D
 Acq On : 14 Mar 2024 16:15
 Operator : SY/MD
 Sample : P1728-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B75DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.323	1640	1643	1644	rBV2	252	129	0.01%	0.001%
38	6.355	1650	1653	1658	rVB2	162	127	0.01%	0.001%
39	6.400	1664	1667	1673	rBV2	210	224	0.02%	0.002%
40	6.532	1703	1708	1712	rBV2	147	185	0.01%	0.002%
41	6.593	1718	1727	1729	rBV4	1078	1464	0.10%	0.014%
42	6.757	1776	1778	1781	rBV3	279	132	0.01%	0.001%
43	6.847	1802	1806	1808	rVB2	194	124	0.01%	0.001%
44	6.915	1816	1827	1855	rBV	155538	297218	20.38%	2.807%
45	7.243	1918	1929	1963	rBV	611296	1078604	73.95%	10.186%
46	7.513	2011	2013	2014	rBV	348	163	0.01%	0.002%
47	7.554	2016	2026	2055	rVV	102828	189320	12.98%	1.788%
48	7.966	2151	2154	2158	rBV	128	118	0.01%	0.001%
49	8.024	2163	2172	2206	rBV	359115	688404	47.20%	6.501%
50	8.542	2330	2333	2336	rBV2	332	307	0.02%	0.003%
51	8.564	2338	2340	2343	rVV2	744	283	0.02%	0.003%
52	8.587	2345	2347	2348	rVV	324	143	0.01%	0.001%
53	8.609	2352	2354	2356	rVV	229	124	0.01%	0.001%
54	8.632	2359	2361	2366	rVB3	185	122	0.01%	0.001%
55	8.689	2374	2379	2381	rBV3	318	241	0.02%	0.002%
56	8.783	2398	2408	2414	rBV	561100	924979	63.42%	8.736%
57	9.066	2494	2496	2501	rVB	250	142	0.01%	0.001%
58	9.095	2501	2505	2508	rBV	369	304	0.02%	0.003%
59	9.194	2533	2536	2541	rBV	171	179	0.01%	0.002%
60	9.223	2541	2545	2547	rBV2	181	144	0.01%	0.001%
61	9.288	2562	2565	2567	rVB3	255	130	0.01%	0.001%
62	9.336	2572	2580	2592	rBV3	7684	15546	1.07%	0.147%
63	9.487	2626	2627	2631	rBV2	267	198	0.01%	0.002%
64	9.525	2636	2639	2642	rVB2	309	180	0.01%	0.002%
65	9.554	2642	2648	2649	rBV2	360	257	0.02%	0.002%
66	9.632	2668	2672	2677	rBV2	235	239	0.02%	0.002%
67	9.686	2687	2689	2692	rVB	248	128	0.01%	0.001%
68	9.805	2724	2726	2729	rBV	218	137	0.01%	0.001%
69	9.844	2735	2738	2741	rBV2	179	140	0.01%	0.001%
70	10.085	2809	2813	2819	rBV2	262	236	0.02%	0.002%
71	10.152	2821	2834	2859	rBV	382521	602416	41.30%	5.689%
72	10.313	2881	2884	2886	rBV2	606	447	0.03%	0.004%
73	10.480	2933	2936	2940	rBV3	339	354	0.02%	0.003%
74	10.570	2960	2964	2969	rBV2	203	272	0.02%	0.003%
75	10.596	2970	2972	2976	rVB	446	263	0.02%	0.002%
76	10.622	2976	2980	2981	rBV2	166	135	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034606.D
 Acq On : 14 Mar 2024 16:15
 Operator : SY/MD
 Sample : P1728-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B75DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.651	2988	2989	2991	rBV	456	142	0.01%	0.001%
78	10.722	3008	3011	3013	rBV2	474	334	0.02%	0.003%
79	10.802	3034	3036	3041	rBV2	173	139	0.01%	0.001%
80	10.914	3068	3071	3073	rBV2	175	120	0.01%	0.001%
81	11.123	3127	3136	3145	rBV	27151	42617	2.92%	0.402%
82	11.188	3145	3156	3158	rBV	617194	830149	56.92%	7.840%
83	11.496	3243	3252	3260	rBV5	9625	19612	1.34%	0.185%
84	11.561	3262	3272	3303	rVB2	619266	1086244	74.48%	10.259%
85	11.840	3354	3359	3361	rBV2	357	284	0.02%	0.003%
86	11.876	3367	3370	3375	rVB3	241	217	0.01%	0.002%
87	11.947	3389	3392	3393	rBV	252	131	0.01%	0.001%
88	12.069	3426	3430	3433	rBV2	382	342	0.02%	0.003%
89	12.316	3504	3507	3509	rBV2	388	240	0.02%	0.002%
90	12.464	3550	3553	3555	rVB2	229	117	0.01%	0.001%
91	13.004	3718	3721	3724	rBV3	337	248	0.02%	0.002%
92	13.201	3772	3782	3796	rBV3	48453	77246	5.30%	0.730%
93	13.278	3804	3806	3810	rBV2	247	161	0.01%	0.002%
94	13.455	3857	3861	3863	rBV2	478	397	0.03%	0.004%
95	13.509	3876	3878	3880	rBV	272	157	0.01%	0.001%
96	13.602	3904	3907	3908	rBV	263	126	0.01%	0.001%
97	13.638	3914	3918	3919	rBV	362	261	0.02%	0.002%
98	13.683	3923	3932	3945	rVB	36224	56295	3.86%	0.532%
99	13.808	3966	3971	3973	rBV3	428	438	0.03%	0.004%
100	14.162	4078	4081	4085	rBV2	355	318	0.02%	0.003%




Sum of corrected areas: 10588700

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034606.D
Acq On : 14 Mar 2024 16:15
Operator : SY/MD
Sample : P1728-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

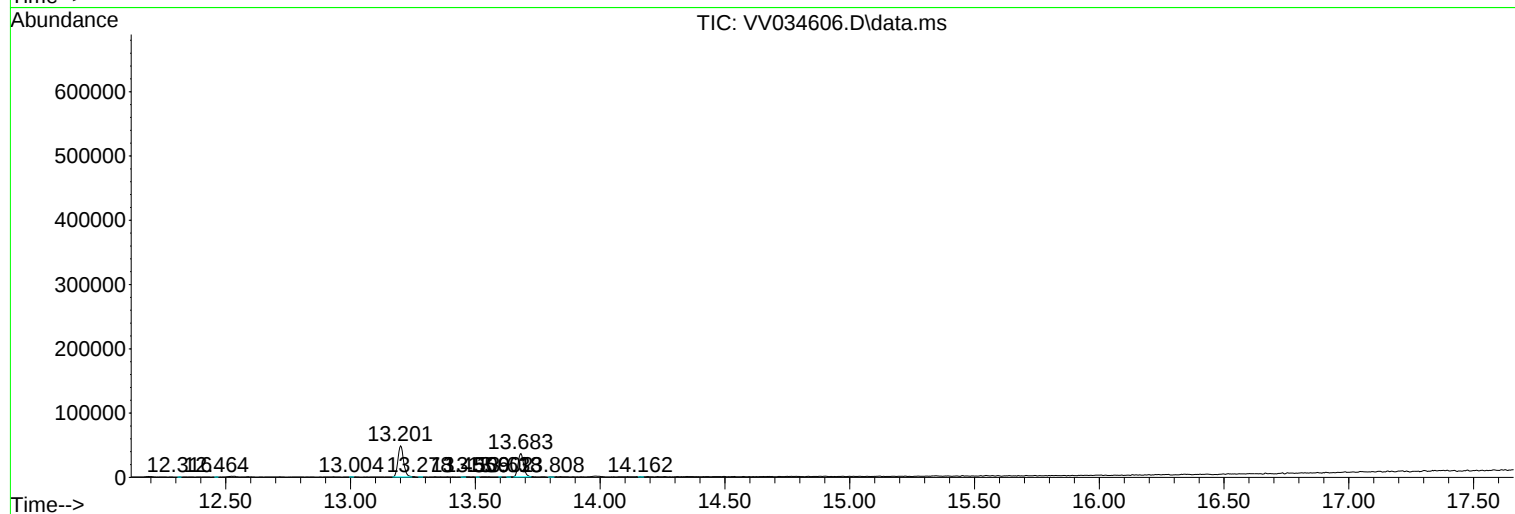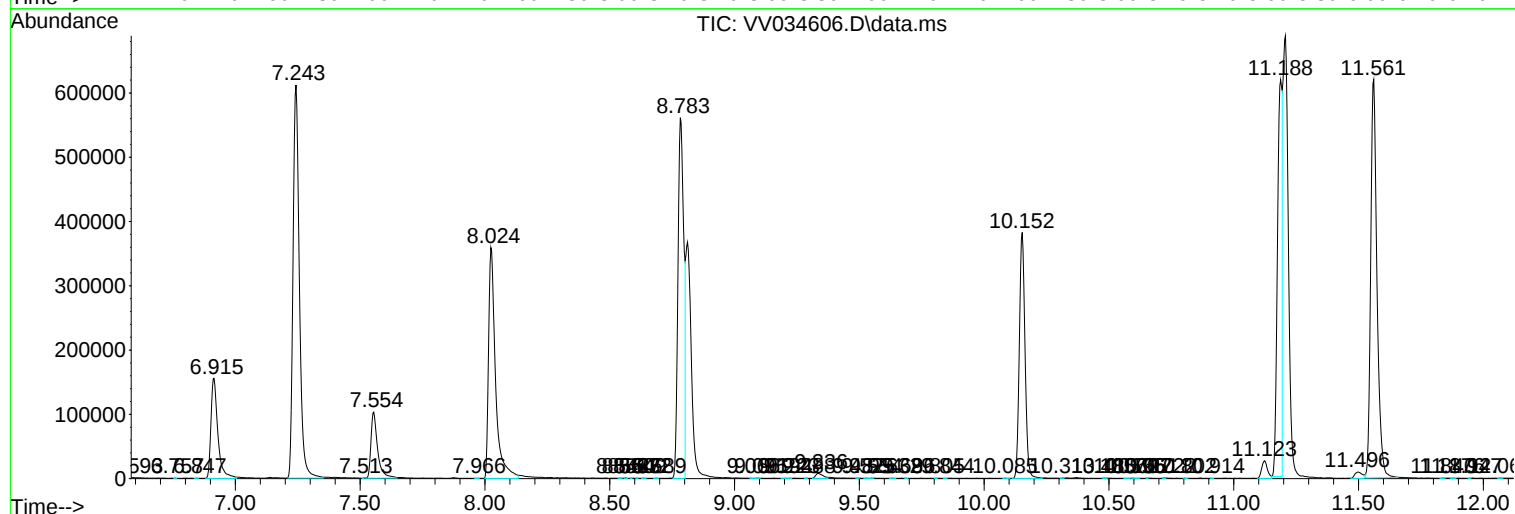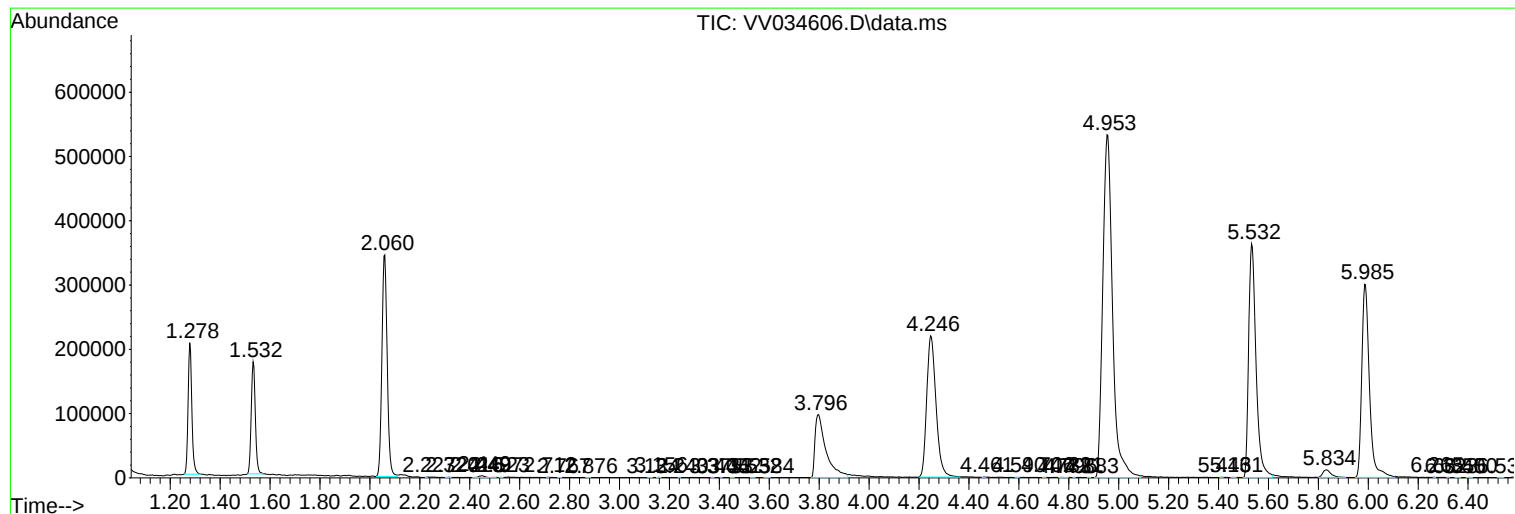

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034606.D
Acq On : 14 Mar 2024 16:15
Operator : SY/MD
Sample : P1728-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034606.D
Acq On : 14 Mar 2024 16:15
Operator : SY/MD
Sample : P1728-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc