

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034607.D
 Acq On : 14 Mar 2024 16:39
 Operator : SY/MD
 Sample : P1742-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0761

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.192	43	47	52	rBV	10308	8693	0.63%	0.085%
2	1.278	67	74	90	rVB	195205	213213	15.54%	2.095%
3	1.532	146	153	165	rBV	168743	190063	13.85%	1.867%
4	2.060	306	317	330	rBV	328592	480370	35.01%	4.720%
5	2.610	486	488	493	rVB3	615	425	0.03%	0.004%
6	2.809	548	550	554	rVB	158	89	0.01%	0.001%
7	2.973	598	601	603	rBV	166	106	0.01%	0.001%
8	3.005	608	611	615	rBV2	189	129	0.01%	0.001%
9	3.092	632	638	641	rBV2	121	137	0.01%	0.001%
10	3.159	654	659	662	rBV2	182	199	0.01%	0.002%
11	3.211	672	675	679	rBV	188	124	0.01%	0.001%
12	3.230	679	681	683	rBV	188	89	0.01%	0.001%
13	3.304	698	704	706	rBV2	145	149	0.01%	0.001%
14	3.336	712	714	721	rVB2	212	118	0.01%	0.001%
15	3.388	725	730	733	rBV2	223	203	0.01%	0.002%
16	3.413	735	738	741	rVB	151	86	0.01%	0.001%
17	3.564	779	785	787	rBV2	165	169	0.01%	0.002%
18	3.638	806	808	814	rBV	232	122	0.01%	0.001%
19	3.693	821	825	826	rBV	152	94	0.01%	0.001%
20	3.719	831	833	837	rVB	239	109	0.01%	0.001%
21	3.754	841	844	846	rBV	166	114	0.01%	0.001%
22	3.793	847	856	898	rBV	98476	297020	21.65%	2.918%
23	4.249	982	998	1036	rBV3	223039	643038	46.87%	6.318%
24	4.458	1061	1063	1066	rVB2	588	260	0.02%	0.003%
25	4.638	1116	1119	1122	rBV2	418	249	0.02%	0.002%
26	4.751	1150	1154	1159	rVB2	399	360	0.03%	0.004%
27	4.841	1180	1182	1185	rVB2	333	122	0.01%	0.001%
28	4.886	1194	1196	1197	rBV	294	123	0.01%	0.001%
29	4.953	1200	1217	1264	rBV3	516667	1372095	100.00%	13.481%
30	5.352	1338	1341	1342	rBV	326	187	0.01%	0.002%
31	5.378	1347	1349	1357	rVB2	487	476	0.03%	0.005%
32	5.410	1357	1359	1360	rBV2	196	88	0.01%	0.001%
33	5.429	1360	1365	1369	rBV4	363	379	0.03%	0.004%
34	5.461	1373	1375	1379	rVB3	383	192	0.01%	0.002%
35	5.484	1379	1382	1384	rVB	258	153	0.01%	0.002%
36	5.532	1384	1397	1424	rBV	352861	735322	53.59%	7.225%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034607.D
 Acq On : 14 Mar 2024 16:39
 Operator : SY/MD
 Sample : P1742-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0761

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	5.828	1478	1489	1506	rBV2	18722	41519	3.03%	0.408%
38	5.986	1526	1538	1570	rBV	290211	615609	44.87%	6.048%
39	6.207	1605	1607	1610	rBV2	481	305	0.02%	0.003%
40	6.304	1635	1637	1643	rBV3	247	208	0.02%	0.002%
41	6.368	1653	1657	1659	rVV	194	128	0.01%	0.001%
42	6.442	1669	1680	1698	rBV2	6647	14261	1.04%	0.140%
43	6.593	1717	1727	1730	rBV4	1192	1771	0.13%	0.017%
44	6.693	1756	1758	1761	rBV3	269	134	0.01%	0.001%
45	6.786	1785	1787	1790	rVB2	324	142	0.01%	0.001%
46	6.876	1812	1815	1816	rBV	158	96	0.01%	0.001%
47	6.912	1816	1826	1854	rBV	150082	288272	21.01%	2.832%
48	7.143	1889	1898	1901	rBV3	1094	1798	0.13%	0.018%
49	7.243	1916	1929	1969	rBV	596053	1056368	76.99%	10.379%
50	7.555	2016	2026	2056	rBV	101549	191624	13.97%	1.883%
51	7.879	2113	2127	2138	rBV3	3766	7079	0.52%	0.070%
52	7.921	2138	2140	2143	rVB	247	109	0.01%	0.001%
53	7.947	2143	2148	2153	rBV2	302	226	0.02%	0.002%
54	8.024	2163	2172	2213	rBV	364128	706586	51.50%	6.942%
55	8.657	2367	2369	2372	rBV	180	122	0.01%	0.001%
56	8.709	2382	2385	2389	rBV2	281	193	0.01%	0.002%
57	8.783	2397	2408	2435	rBV	537421	893753	65.14%	8.781%
58	9.040	2487	2488	2491	rBV2	317	152	0.01%	0.001%
59	9.120	2510	2513	2516	rVB2	149	94	0.01%	0.001%
60	9.140	2516	2519	2520	rBV	196	118	0.01%	0.001%
61	9.191	2533	2535	2540	rVB	244	167	0.01%	0.002%
62	9.265	2554	2558	2559	rBV	249	166	0.01%	0.002%
63	9.375	2586	2592	2596	rBV	246	274	0.02%	0.003%
64	9.407	2599	2602	2605	rVV2	247	157	0.01%	0.002%
65	9.432	2607	2610	2613	rVB2	332	155	0.01%	0.002%
66	9.481	2621	2625	2627	rBV	122	95	0.01%	0.001%
67	9.497	2627	2630	2637	rBV2	496	394	0.03%	0.004%
68	9.683	2677	2688	2692	rVV2	316	547	0.04%	0.005%
69	9.722	2698	2700	2703	rBV	197	108	0.01%	0.001%
70	9.950	2765	2771	2773	rBV	221	197	0.01%	0.002%
71	10.011	2784	2790	2794	rBV2	301	349	0.03%	0.003%
72	10.082	2810	2812	2815	rVB2	188	86	0.01%	0.001%
73	10.153	2821	2834	2862	rBV	371036	590624	43.05%	5.803%
74	10.326	2879	2888	2901	rVB2	5380	8515	0.62%	0.084%
75	10.481	2934	2936	2940	rVB2	302	182	0.01%	0.002%
76	10.503	2940	2943	2947	rBV2	169	123	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034607.D
 Acq On : 14 Mar 2024 16:39
 Operator : SY/MD
 Sample : P1742-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0761

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.609	2970	2976	2983	rVB2	290	407	0.03%	0.004%
78	10.645	2983	2987	2991	rVB2	264	227	0.02%	0.002%
79	10.706	3004	3006	3007	rBV	227	93	0.01%	0.001%
80	10.776	3024	3028	3030	rBV2	169	120	0.01%	0.001%
81	10.870	3053	3057	3059	rBV3	205	136	0.01%	0.001%
82	11.014	3099	3102	3106	rBV2	164	128	0.01%	0.001%
83	11.185	3143	3155	3182	rBV	546824	865270	63.06%	8.501%
84	11.426	3227	3230	3234	rVB2	465	331	0.02%	0.003%
85	11.458	3236	3240	3245	rVB2	385	328	0.02%	0.003%
86	11.493	3247	3251	3253	rBV3	289	211	0.02%	0.002%
87	11.558	3255	3271	3295	rBV	587607	938229	68.38%	9.218%
88	11.799	3343	3346	3348	rBV2	400	263	0.02%	0.003%
89	11.831	3353	3356	3358	rBV2	294	184	0.01%	0.002%
90	11.899	3372	3377	3378	rBV	638	472	0.03%	0.005%
91	11.934	3385	3388	3393	rBV2	341	285	0.02%	0.003%
92	11.956	3393	3395	3396	rBV	377	134	0.01%	0.001%
93	12.291	3496	3499	3501	rBV	254	121	0.01%	0.001%
94	12.310	3502	3505	3509	rVV3	498	370	0.03%	0.004%
95	12.387	3525	3529	3533	rBV2	362	226	0.02%	0.002%
96	12.538	3573	3576	3578	rBV2	338	148	0.01%	0.001%
97	12.583	3588	3590	3593	rBV	273	101	0.01%	0.001%
98	13.204	3779	3783	3785	rBV2	1505	1043	0.08%	0.010%
99	13.641	3916	3919	3924	rBV2	605	543	0.04%	0.005%
100	13.828	3975	3977	3989	rVB4	649	891	0.06%	0.009%




Sum of corrected areas: 10177932

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034607.D
Acq On : 14 Mar 2024 16:39
Operator : SY/MD
Sample : P1742-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0761

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

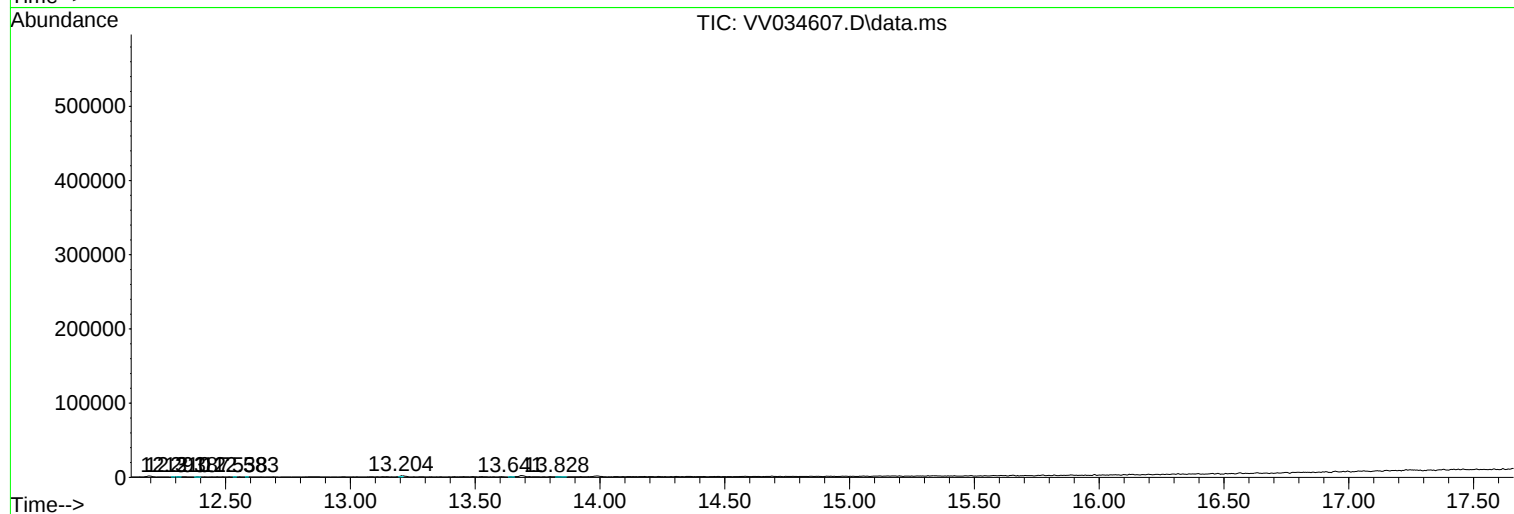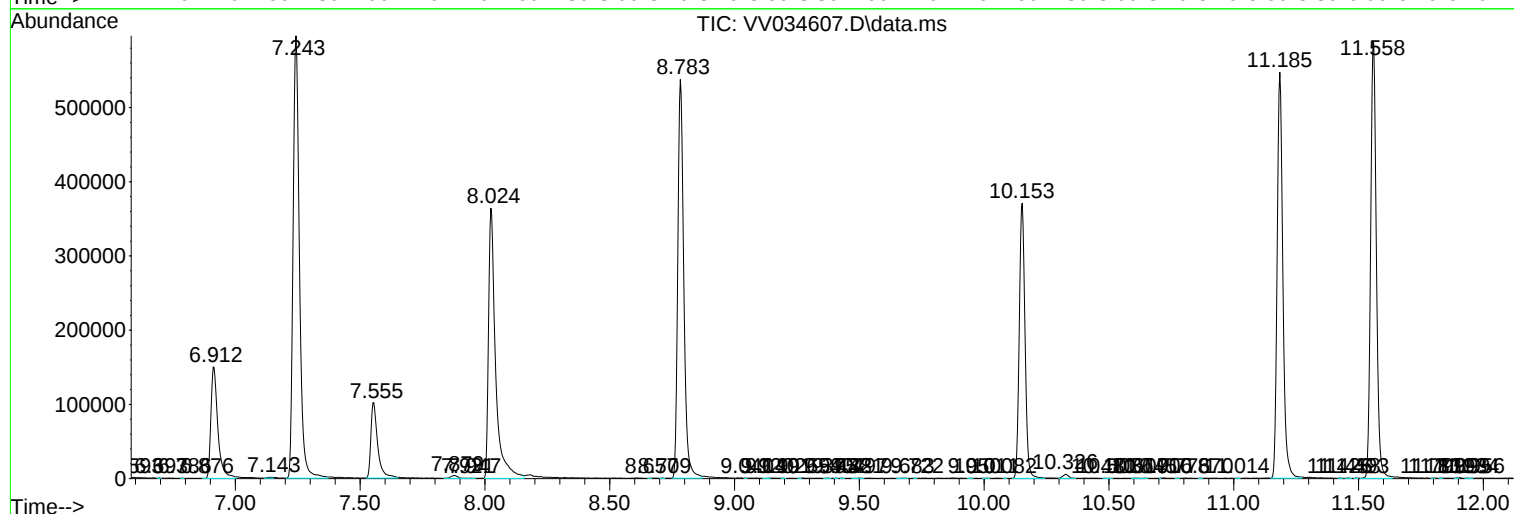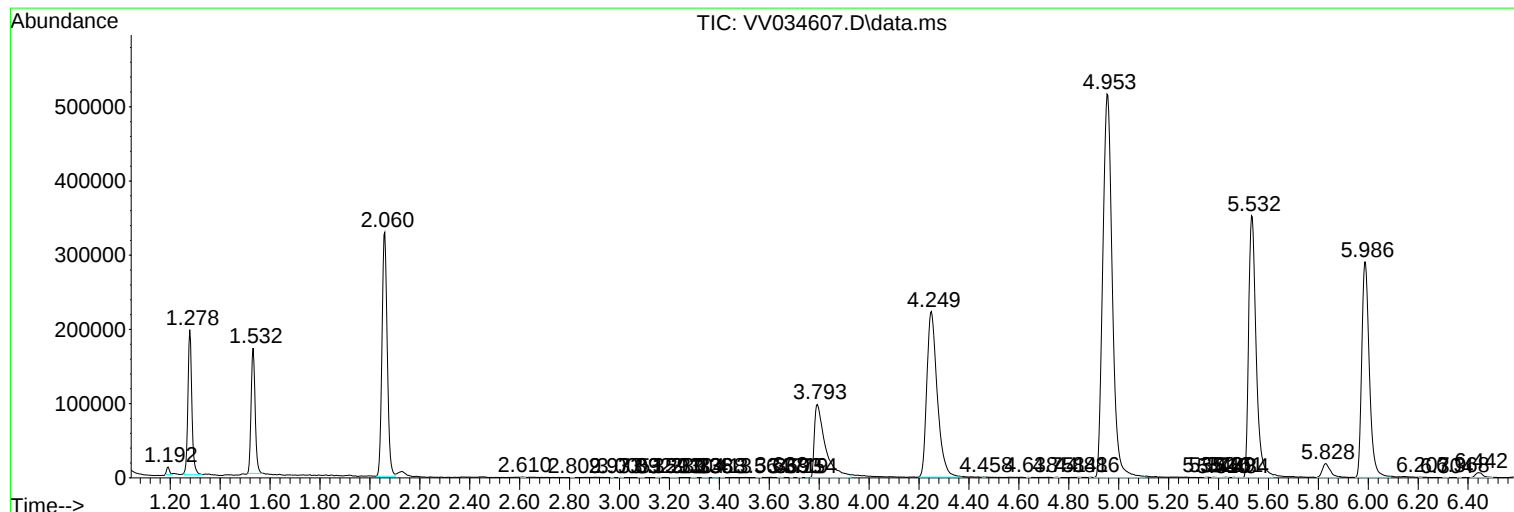

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034607.D
Acq On : 14 Mar 2024 16:39
Operator : SY/MD
Sample : P1742-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0761

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034607.D
Acq On : 14 Mar 2024 16:39
Operator : SY/MD
Sample : P1742-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0761

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------