

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034609.D
 Acq On : 14 Mar 2024 17:27
 Operator : SY/MD
 Sample : P1742-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	189446	197790	14.82%	2.048%
2	1.535	146	154	168	rBV	164741	191013	14.32%	1.977%
3	2.060	307	317	335	rBV	328989	475290	35.62%	4.920%
4	2.355	407	409	411	rBV2	290	138	0.01%	0.001%
5	2.423	426	430	432	rBV2	706	625	0.05%	0.006%
6	2.715	518	521	530	rVB2	255	235	0.02%	0.002%
7	2.802	544	548	550	rBV	186	135	0.01%	0.001%
8	2.825	552	555	556	rBV	249	135	0.01%	0.001%
9	2.886	571	574	579	rVB2	188	132	0.01%	0.001%
10	2.950	591	594	596	rBV	195	139	0.01%	0.001%
11	2.989	603	606	609	rBV	128	105	0.01%	0.001%
12	3.092	635	638	640	rBV	179	128	0.01%	0.001%
13	3.185	663	667	670	rBV2	173	166	0.01%	0.002%
14	3.256	686	689	692	rBV2	229	174	0.01%	0.002%
15	3.297	699	702	708	rVB2	231	210	0.02%	0.002%
16	3.330	708	712	715	rBV2	242	224	0.02%	0.002%
17	3.465	751	754	756	rBV	198	130	0.01%	0.001%
18	3.535	772	776	781	rVB	366	207	0.02%	0.002%
19	3.799	849	858	904	rVV	89051	292055	21.89%	3.023%
20	4.249	982	998	1026	rBV	206533	532732	39.93%	5.515%
21	4.776	1158	1162	1165	rBV2	276	230	0.02%	0.002%
22	4.802	1168	1170	1172	rVB	258	113	0.01%	0.001%
23	4.818	1172	1175	1176	rBV	244	140	0.01%	0.001%
24	4.953	1201	1217	1250	rBV2	504360	1334260	100.00%	13.812%
25	5.326	1331	1333	1336	rBV3	206	136	0.01%	0.001%
26	5.381	1348	1350	1352	rBV2	199	105	0.01%	0.001%
27	5.532	1386	1397	1437	rBV	349049	729412	54.67%	7.551%
28	5.831	1479	1490	1514	rVB	12693	30416	2.28%	0.315%
29	5.989	1526	1539	1564	rBV	285613	597261	44.76%	6.183%
30	6.243	1616	1618	1622	rBV3	366	231	0.02%	0.002%
31	6.426	1673	1675	1679	rVB	215	123	0.01%	0.001%
32	6.452	1679	1683	1685	rBV2	181	108	0.01%	0.001%
33	6.519	1702	1704	1708	rBV2	326	180	0.01%	0.002%
34	6.596	1719	1728	1729	rBV3	836	1198	0.09%	0.012%
35	6.747	1770	1775	1780	rVB2	425	466	0.03%	0.005%
36	6.770	1780	1782	1788	rVB3	396	329	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034609.D
 Acq On : 14 Mar 2024 17:27
 Operator : SY/MD
 Sample : P1742-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.796	1788	1790	1794	rVB2	264	146	0.01%	0.002%
38	6.825	1794	1799	1802	rBV2	172	138	0.01%	0.001%
39	6.915	1816	1827	1864	rBV	141366	272515	20.42%	2.821%
40	7.243	1918	1929	1959	rBV	571627	1002000	75.10%	10.373%
41	7.554	2017	2026	2058	rBV	96909	178051	13.34%	1.843%
42	7.879	2119	2127	2136	rBV4	558	1027	0.08%	0.011%
43	8.024	2163	2172	2211	rBV	338670	676240	50.68%	7.001%
44	8.455	2303	2306	2309	rBV	417	213	0.02%	0.002%
45	8.564	2338	2340	2343	rBV3	183	145	0.01%	0.002%
46	8.616	2354	2356	2359	rBV2	281	182	0.01%	0.002%
47	8.638	2361	2363	2368	rVB3	558	332	0.02%	0.003%
48	8.706	2380	2384	2386	rBV2	338	266	0.02%	0.003%
49	8.783	2398	2408	2443	rBV	513487	845758	63.39%	8.755%
50	9.149	2517	2522	2524	rBV2	292	221	0.02%	0.002%
51	9.175	2527	2530	2531	rBV	272	147	0.01%	0.002%
52	9.439	2609	2612	2616	rVB2	267	202	0.02%	0.002%
53	9.468	2616	2621	2625	rBV2	180	224	0.02%	0.002%
54	9.493	2625	2629	2632	rVB	364	280	0.02%	0.003%
55	9.516	2632	2636	2640	rBV	216	202	0.02%	0.002%
56	9.558	2646	2649	2652	rVB2	177	112	0.01%	0.001%
57	9.583	2655	2657	2659	rBV	186	105	0.01%	0.001%
58	9.603	2659	2663	2669	rVB2	289	259	0.02%	0.003%
59	9.632	2669	2672	2677	rBV2	138	162	0.01%	0.002%
60	9.667	2681	2683	2686	rVB2	200	118	0.01%	0.001%
61	9.689	2686	2690	2695	rBV2	174	174	0.01%	0.002%
62	9.722	2695	2700	2705	rBV2	250	281	0.02%	0.003%
63	9.850	2736	2740	2742	rBV	258	214	0.02%	0.002%
64	9.882	2747	2750	2754	rVV	187	129	0.01%	0.001%
65	9.972	2776	2778	2784	rVB2	232	181	0.01%	0.002%
66	10.014	2788	2791	2799	rVB2	249	278	0.02%	0.003%
67	10.053	2799	2803	2805	rBV2	180	153	0.01%	0.002%
68	10.078	2809	2811	2814	rBV	247	104	0.01%	0.001%
69	10.152	2822	2834	2859	rBV	366807	580102	43.48%	6.005%
70	10.413	2909	2915	2917	rBV	272	264	0.02%	0.003%
71	10.660	2991	2992	2997	rVB	336	142	0.01%	0.001%
72	10.686	2997	3000	3003	rBV2	135	115	0.01%	0.001%
73	10.805	3033	3037	3039	rBV2	134	117	0.01%	0.001%
74	10.873	3054	3058	3061	rBV3	261	241	0.02%	0.002%
75	10.918	3070	3072	3076	rBV	250	171	0.01%	0.002%
76	10.940	3077	3079	3082	rBV	168	116	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034609.D
 Acq On : 14 Mar 2024 17:27
 Operator : SY/MD
 Sample : P1742-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	11.040	3104	3110	3115	rBV3	361	450	0.03%	0.005%
78	11.066	3115	3118	3121	rBV2	160	126	0.01%	0.001%
79	11.185	3144	3155	3182	rBV	516418	810952	60.78%	8.395%
80	11.361	3209	3210	3214	rBV3	349	189	0.01%	0.002%
81	11.458	3238	3240	3243	rVB	391	177	0.01%	0.002%
82	11.477	3243	3246	3252	rBV2	261	287	0.02%	0.003%
83	11.561	3258	3272	3298	rBV	561437	893519	66.97%	9.250%
84	11.747	3326	3330	3331	rBV2	300	212	0.02%	0.002%
85	11.815	3347	3351	3353	rBV	437	259	0.02%	0.003%
86	11.905	3376	3379	3382	rBV	208	167	0.01%	0.002%
87	12.004	3407	3410	3416	rBV2	406	395	0.03%	0.004%
88	12.194	3462	3469	3478	rVB2	1730	2438	0.18%	0.025%
89	12.239	3478	3483	3486	rBV2	278	306	0.02%	0.003%
90	12.345	3514	3516	3521	rVB	232	133	0.01%	0.001%
91	12.435	3541	3544	3545	rBV	497	188	0.01%	0.002%
92	12.554	3578	3581	3582	rBV	179	113	0.01%	0.001%
93	12.654	3610	3612	3617	rBV	200	144	0.01%	0.001%
94	12.757	3641	3644	3645	rBV	207	115	0.01%	0.001%
95	12.860	3673	3676	3678	rBV	171	106	0.01%	0.001%
96	13.107	3749	3753	3755	rBV3	473	334	0.03%	0.003%
97	13.162	3767	3770	3773	rBV2	283	192	0.01%	0.002%
98	13.316	3815	3818	3820	rBV	213	149	0.01%	0.002%
99	13.647	3918	3921	3922	rBV	247	150	0.01%	0.002%
100	14.873	4299	4302	4306	rBV2	487	436	0.03%	0.005%




Sum of corrected areas: 9659835

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034609.D
Acq On : 14 Mar 2024 17:27
Operator : SY/MD
Sample : P1742-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

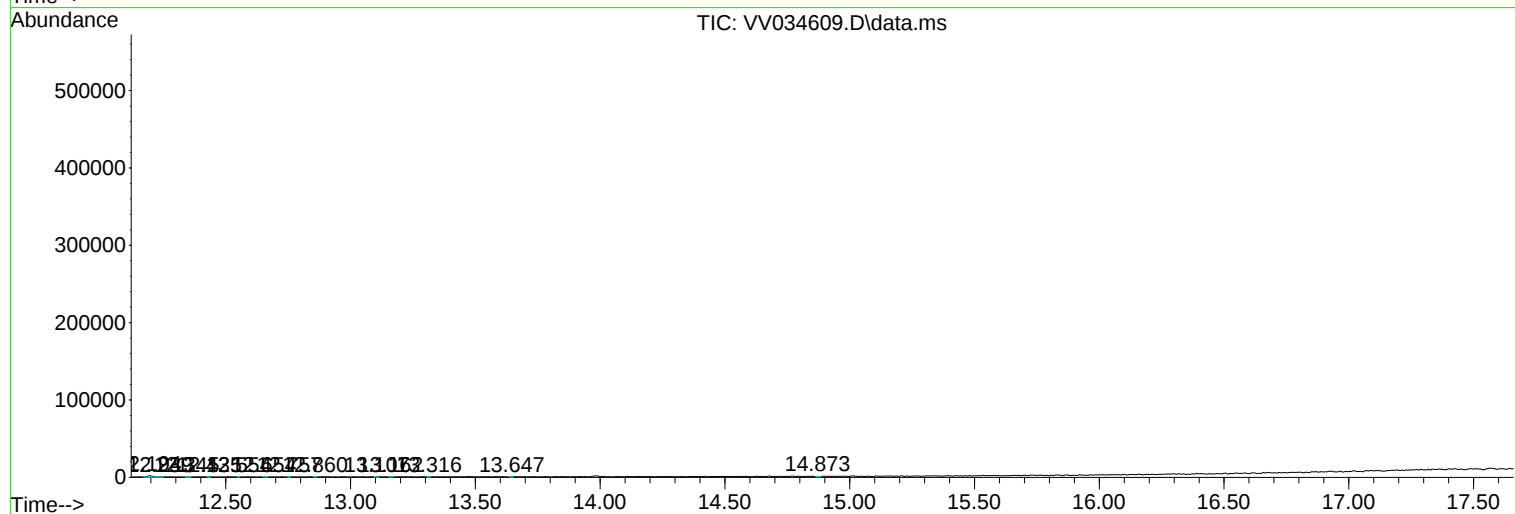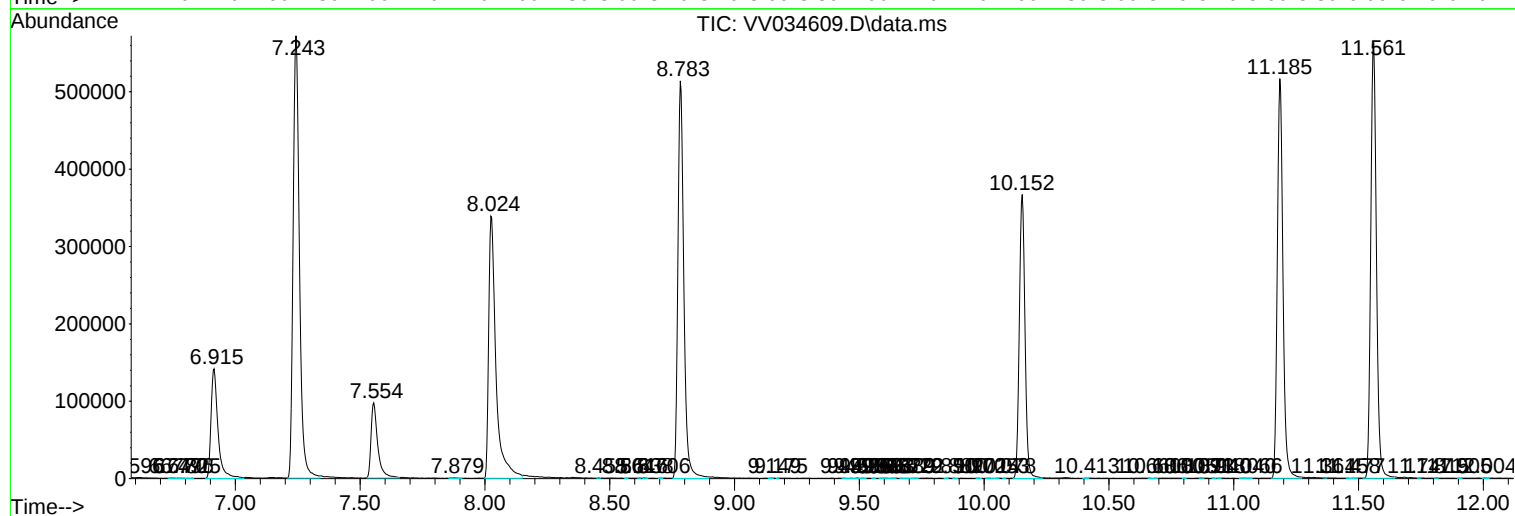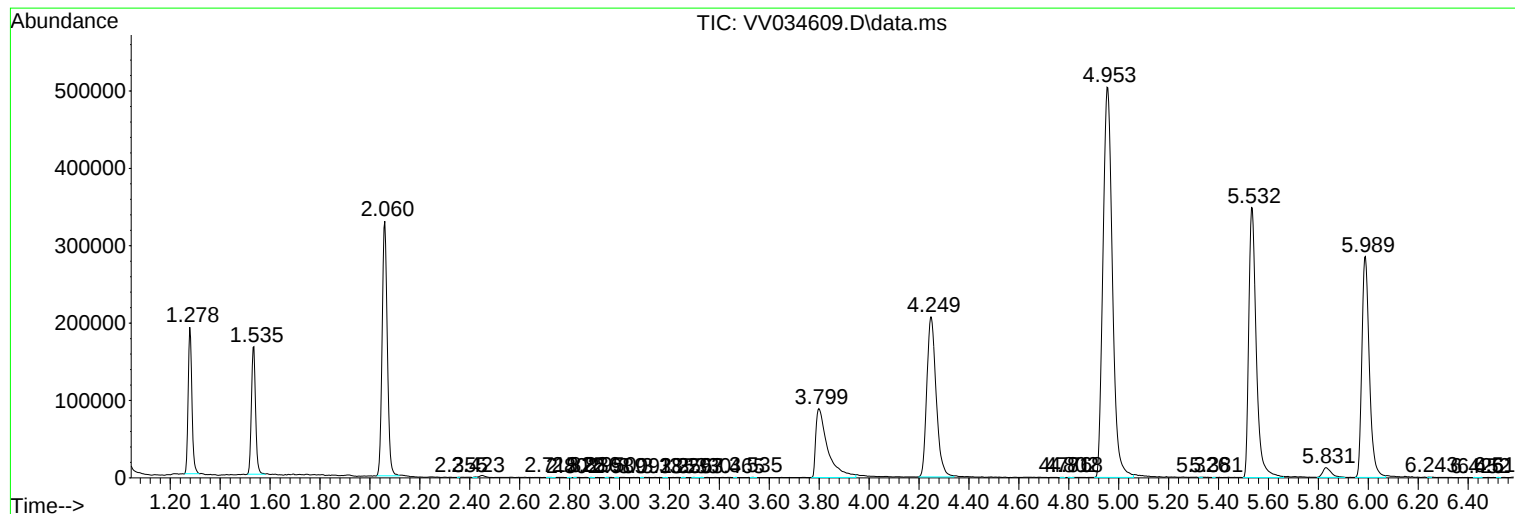

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034609.D
Acq On : 14 Mar 2024 17:27
Operator : SY/MD
Sample : P1742-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034609.D
Acq On : 14 Mar 2024 17:27
Operator : SY/MD
Sample : P1742-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc