

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034611.D
 Acq On : 14 Mar 2024 18:14
 Operator : SY/MD
 Sample : P1752-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034611.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	93	rVB2	355734	417789	31.14%	3.369%
2	1.532	146	153	168	rVB	156313	182396	13.60%	1.471%
3	2.063	307	318	331	rBV3	554913	939950	70.07%	7.579%
4	2.696	508	515	530	rVB2	21090	38953	2.90%	0.314%
5	2.928	586	587	589	rBV	282	111	0.01%	0.001%
6	3.111	631	644	667	rBV	99762	211334	15.75%	1.704%
7	3.291	698	700	702	rBV	361	151	0.01%	0.001%
8	3.362	718	722	724	rBV	178	149	0.01%	0.001%
9	3.391	727	731	732	rBV2	269	128	0.01%	0.001%
10	3.465	747	754	755	rBV	206	147	0.01%	0.001%
11	3.503	763	766	768	rBV	131	83	0.01%	0.001%
12	3.516	768	770	772	rVV	239	96	0.01%	0.001%
13	3.529	772	774	778	rVB2	241	123	0.01%	0.001%
14	3.574	782	788	791	rBV2	94	113	0.01%	0.001%
15	3.593	791	794	795	rBV2	111	69	0.01%	0.001%
16	3.722	831	834	838	rVB2	130	81	0.01%	0.001%
17	3.748	838	842	844	rBV	124	104	0.01%	0.001%
18	3.812	848	862	898	rBV2	497575	1341435	100.00%	10.817%
19	4.249	982	998	1026	rBV	196617	514220	38.33%	4.146%
20	4.629	1113	1116	1120	rBV3	470	357	0.03%	0.003%
21	4.802	1165	1170	1172	rBV	339	248	0.02%	0.002%
22	4.815	1172	1174	1178	rVV	364	198	0.01%	0.002%
23	4.831	1178	1179	1184	rVB3	363	198	0.01%	0.002%
24	4.953	1201	1217	1246	rBV2	471670	1274616	95.02%	10.278%
25	5.230	1301	1303	1309	rVB3	402	308	0.02%	0.002%
26	5.304	1325	1326	1327	rBV	275	87	0.01%	0.001%
27	5.394	1350	1354	1356	rBV2	275	153	0.01%	0.001%
28	5.407	1356	1358	1361	rBV2	196	127	0.01%	0.001%
29	5.423	1361	1363	1365	rBV2	229	128	0.01%	0.001%
30	5.458	1372	1374	1377	rVB	248	106	0.01%	0.001%
31	5.471	1377	1378	1385	rVB	218	215	0.02%	0.002%
32	5.532	1385	1397	1428	rBV	321080	668100	49.80%	5.387%
33	5.831	1477	1490	1525	rBV	556302	1126668	83.99%	9.085%
34	5.989	1527	1539	1564	rBV2	269539	556348	41.47%	4.486%
35	6.201	1603	1605	1606	rBV	294	100	0.01%	0.001%
36	6.323	1642	1643	1644	rBV	240	77	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034611.D
 Acq On : 14 Mar 2024 18:14
 Operator : SY/MD
 Sample : P1752-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.352	1650	1652	1655	rVB	189	88	0.01%	0.001%
38	6.477	1689	1691	1693	rBV	373	184	0.01%	0.001%
39	6.503	1693	1699	1700	rBV2	565	500	0.04%	0.004%
40	6.580	1719	1723	1724	rBV	525	329	0.02%	0.003%
41	6.696	1757	1759	1762	rVB3	312	158	0.01%	0.001%
42	6.754	1774	1777	1779	rBV	186	122	0.01%	0.001%
43	6.812	1792	1795	1799	rVB2	207	121	0.01%	0.001%
44	6.844	1803	1805	1809	rVB	239	110	0.01%	0.001%
45	6.915	1812	1827	1853	rBV	139510	265780	19.81%	2.143%
46	7.191	1911	1913	1917	rVB3	690	390	0.03%	0.003%
47	7.243	1917	1929	1964	rBV	540512	960111	71.57%	7.742%
48	7.554	2016	2026	2056	rBV	91802	171956	12.82%	1.387%
49	7.789	2097	2099	2103	rVB2	395	233	0.02%	0.002%
50	7.834	2109	2113	2115	rBV3	218	189	0.01%	0.002%
51	7.870	2118	2124	2128	rBV4	3355	4358	0.32%	0.035%
52	7.979	2156	2158	2159	rBV2	242	106	0.01%	0.001%
53	8.027	2163	2173	2215	rBV	334679	672474	50.13%	5.422%
54	8.323	2263	2265	2266	rBV	567	238	0.02%	0.002%
55	8.448	2302	2304	2307	rVB	367	162	0.01%	0.001%
56	8.506	2320	2322	2326	rVB2	323	213	0.02%	0.002%
57	8.554	2335	2337	2338	rBV	194	73	0.01%	0.001%
58	8.738	2391	2394	2397	rVB2	305	186	0.01%	0.001%
59	8.783	2397	2408	2440	rBV	481036	812759	60.59%	6.554%
60	9.056	2489	2493	2496	rBV2	307	279	0.02%	0.002%
61	9.088	2496	2503	2507	rVB4	648	544	0.04%	0.004%
62	9.117	2511	2512	2518	rBV2	411	308	0.02%	0.002%
63	9.201	2535	2538	2539	rBV	128	70	0.01%	0.001%
64	9.223	2543	2545	2548	rVV	215	119	0.01%	0.001%
65	9.300	2568	2569	2571	rBV	173	70	0.01%	0.001%
66	9.313	2571	2573	2578	rVB2	230	148	0.01%	0.001%
67	9.468	2619	2621	2623	rBV	253	122	0.01%	0.001%
68	9.545	2638	2645	2648	rBV2	239	298	0.02%	0.002%
69	9.657	2676	2680	2683	rVB2	320	222	0.02%	0.002%
70	9.673	2683	2685	2688	rBV2	164	94	0.01%	0.001%
71	9.879	2745	2749	2753	rBV3	301	337	0.03%	0.003%
72	9.921	2759	2762	2763	rBV2	221	117	0.01%	0.001%
73	9.963	2768	2775	2785	rVB4	876	1160	0.09%	0.009%
74	10.001	2785	2787	2789	rBV	232	93	0.01%	0.001%
75	10.152	2822	2834	2853	rBV	365120	580938	43.31%	4.684%
76	10.326	2879	2888	2900	rVB2	5363	8202	0.61%	0.066%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034611.D
 Acq On : 14 Mar 2024 18:14
 Operator : SY/MD
 Sample : P1752-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.400	2907	2911	2913	rBV	302	189	0.01%	0.002%
78	10.477	2932	2935	2938	rVB3	314	212	0.02%	0.002%
79	10.496	2940	2941	2943	rVV	275	100	0.01%	0.001%
80	10.554	2957	2959	2962	rBV2	202	100	0.01%	0.001%
81	10.599	2966	2973	2978	rBV2	340	492	0.04%	0.004%
82	10.660	2987	2992	2994	rBV	310	238	0.02%	0.002%
83	10.763	3021	3024	3028	rBV2	175	162	0.01%	0.001%
84	10.799	3032	3035	3037	rBV	218	140	0.01%	0.001%
85	11.140	3139	3141	3144	rVB2	172	95	0.01%	0.001%
86	11.185	3144	3155	3181	rBV	497444	775740	57.83%	6.255%
87	11.461	3240	3241	3243	rBV	282	78	0.01%	0.001%
88	11.561	3260	3272	3298	rBV	551829	862740	64.31%	6.957%
89	11.828	3352	3355	3357	rBV2	399	227	0.02%	0.002%
90	12.001	3407	3409	3411	rBV	361	152	0.01%	0.001%
91	12.120	3443	3446	3448	rBV	178	132	0.01%	0.001%
92	12.316	3505	3507	3514	rBV2	325	241	0.02%	0.002%
93	12.455	3548	3550	3552	rVB	317	102	0.01%	0.001%
94	12.648	3608	3610	3612	rBV2	235	114	0.01%	0.001%
95	12.776	3647	3650	3652	rBV2	244	171	0.01%	0.001%
96	13.046	3730	3734	3737	rBV2	393	299	0.02%	0.002%
97	13.236	3790	3793	3795	rBV2	335	189	0.01%	0.002%
98	13.281	3805	3807	3809	rBV	208	73	0.01%	0.001%
99	13.490	3870	3872	3873	rBV	212	97	0.01%	0.001%
100	13.532	3882	3885	3886	rBV	368	154	0.01%	0.001%




Sum of corrected areas: 12401664

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034611.D
Acq On : 14 Mar 2024 18:14
Operator : SY/MD
Sample : P1752-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

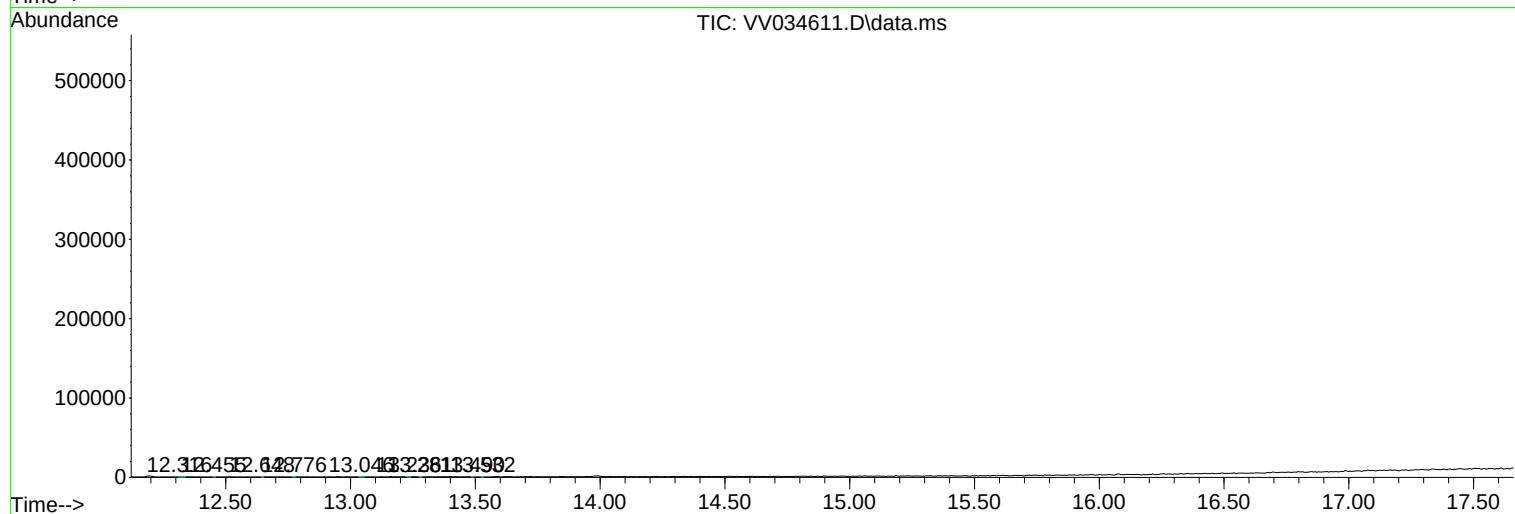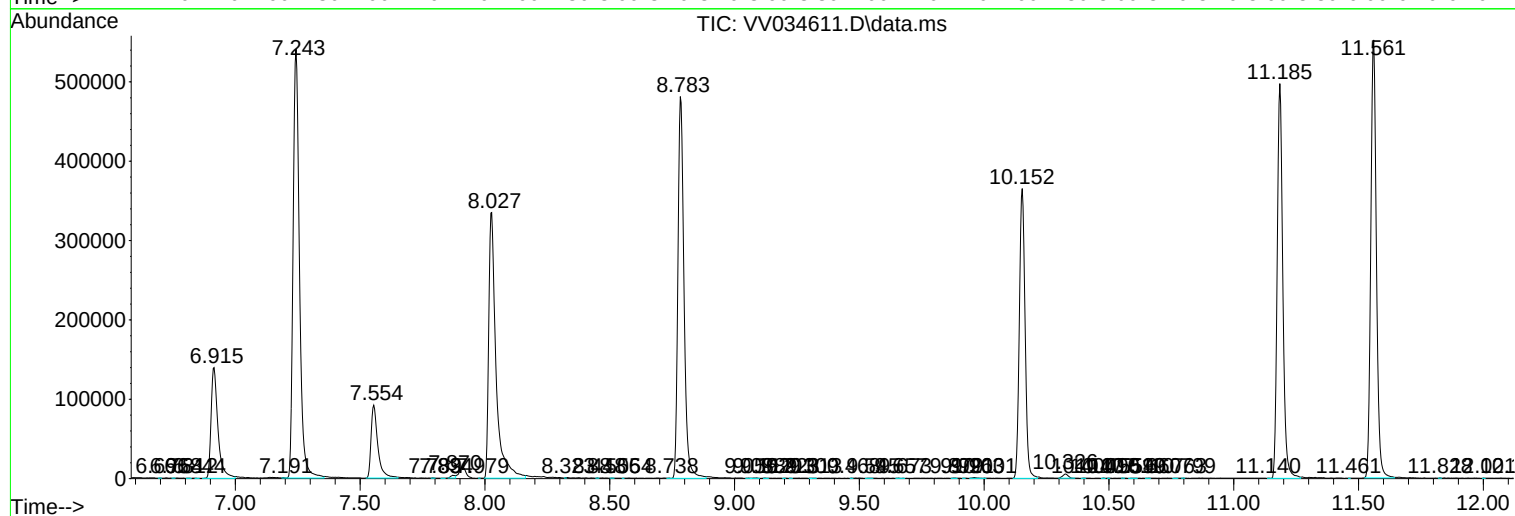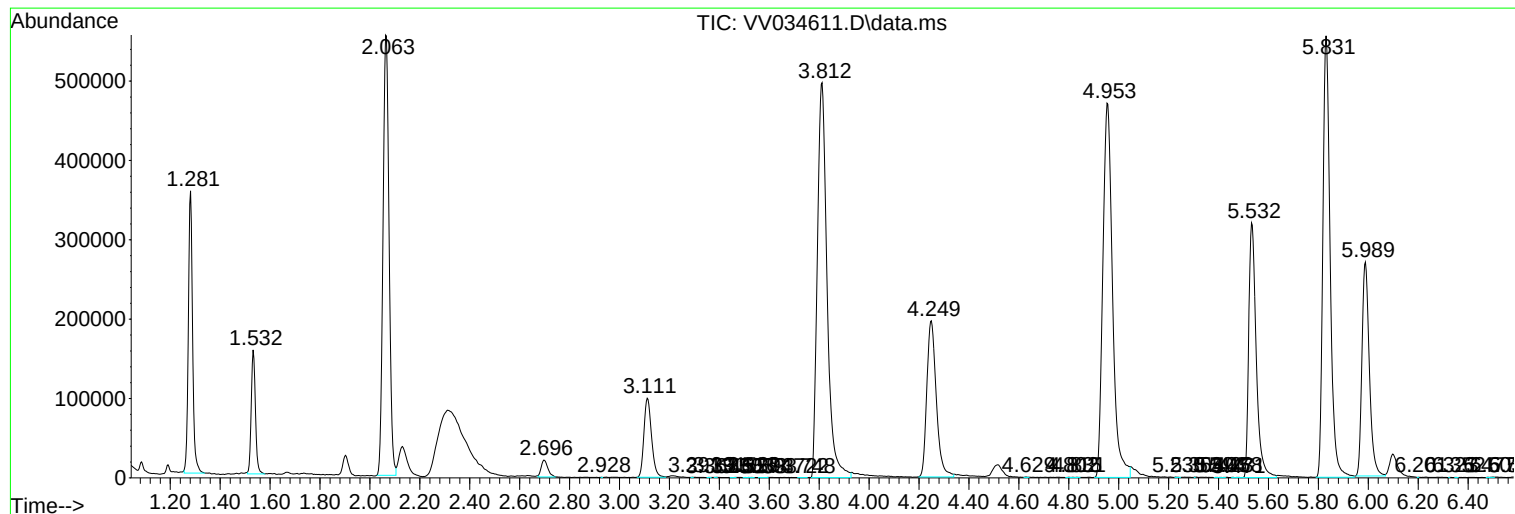

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034611.D
Acq On : 14 Mar 2024 18:14
Operator : SY/MD
Sample : P1752-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034611.D
Acq On : 14 Mar 2024 18:14
Operator : SY/MD
Sample : P1752-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------