

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034614.D
 Acq On : 14 Mar 2024 19:26
 Operator : SY/MD
 Sample : P1751-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	175253	175266	14.49%	1.885%
2	1.532	146	153	166	rBV	147015	168871	13.96%	1.817%
3	2.056	307	316	329	rBV	282503	408123	33.74%	4.390%
4	2.558	461	472	488	rBV	15905	32441	2.68%	0.349%
5	2.789	542	544	545	rBV	181	94	0.01%	0.001%
6	2.876	566	571	572	rBV	273	185	0.02%	0.002%
7	2.963	596	598	602	rBV2	169	96	0.01%	0.001%
8	3.079	630	634	636	rBV2	241	131	0.01%	0.001%
9	3.172	660	663	668	rVB2	130	127	0.01%	0.001%
10	3.240	680	684	688	rBV	199	231	0.02%	0.002%
11	3.304	701	704	705	rBV	185	88	0.01%	0.001%
12	3.326	707	711	714	rBV2	119	131	0.01%	0.001%
13	3.346	714	717	718	rBV	194	107	0.01%	0.001%
14	3.461	750	753	756	rBV2	144	102	0.01%	0.001%
15	3.548	777	780	783	rBV	160	141	0.01%	0.002%
16	3.699	824	827	832	rVB2	141	125	0.01%	0.001%
17	3.722	832	834	839	rVB2	128	92	0.01%	0.001%
18	3.802	843	859	907	rBV3	148854	547664	45.28%	5.891%
19	4.246	983	997	1027	rBV	189054	495103	40.93%	5.326%
20	4.558	1090	1094	1095	rBV2	623	371	0.03%	0.004%
21	4.635	1114	1118	1124	rBV3	701	687	0.06%	0.007%
22	4.664	1124	1127	1132	rBV2	274	259	0.02%	0.003%
23	4.693	1132	1136	1139	rBV2	448	360	0.03%	0.004%
24	4.732	1146	1148	1154	rVB2	303	186	0.02%	0.002%
25	4.793	1165	1167	1169	rBV2	384	158	0.01%	0.002%
26	4.834	1177	1180	1182	rBV	222	137	0.01%	0.001%
27	4.886	1194	1196	1200	rVB2	452	278	0.02%	0.003%
28	4.953	1201	1217	1244	rBV2	461442	1209548	100.00%	13.011%
29	5.291	1318	1322	1324	rBV2	716	516	0.04%	0.006%
30	5.378	1344	1349	1354	rBV2	371	418	0.03%	0.004%
31	5.410	1357	1359	1361	rVV	282	105	0.01%	0.001%
32	5.439	1361	1368	1369	rVB2	251	252	0.02%	0.003%
33	5.471	1375	1378	1381	rBV	239	159	0.01%	0.002%
34	5.532	1386	1397	1421	rBV	328933	676030	55.89%	7.272%
35	5.828	1480	1489	1510	rBV4	15044	34420	2.85%	0.370%
36	5.989	1525	1539	1566	rBV	261303	546265	45.16%	5.876%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034614.D
 Acq On : 14 Mar 2024 19:26
 Operator : SY/MD
 Sample : P1751-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.201	1603	1605	1606	rBV	292	100	0.01%	0.001%
38	6.243	1614	1618	1621	rBV3	263	271	0.02%	0.003%
39	6.285	1625	1631	1634	rBV3	328	353	0.03%	0.004%
40	6.349	1649	1651	1659	rVB3	408	308	0.03%	0.003%
41	6.426	1672	1675	1677	rBV2	193	126	0.01%	0.001%
42	6.452	1681	1683	1684	rBV	291	102	0.01%	0.001%
43	6.484	1691	1693	1696	rBV2	150	78	0.01%	0.001%
44	6.500	1696	1698	1699	rBV2	222	86	0.01%	0.001%
45	6.574	1717	1721	1722	rBV2	696	496	0.04%	0.005%
46	6.735	1768	1771	1773	rBV2	217	138	0.01%	0.001%
47	6.776	1782	1784	1787	rBV2	254	107	0.01%	0.001%
48	6.915	1816	1827	1857	rBV	132689	257220	21.27%	2.767%
49	7.243	1918	1929	1953	rBV	515430	914540	75.61%	9.838%
50	7.555	2016	2026	2047	rBV2	90612	167707	13.87%	1.804%
51	7.792	2096	2100	2107	rVB	6001	4941	0.41%	0.053%
52	7.838	2112	2114	2116	rBV	133	79	0.01%	0.001%
53	7.873	2116	2125	2136	rVV2	2786	4954	0.41%	0.053%
54	7.928	2140	2142	2145	rVB	217	118	0.01%	0.001%
55	7.944	2145	2147	2148	rBV	308	75	0.01%	0.001%
56	7.982	2157	2159	2162	rBV2	435	301	0.02%	0.003%
57	8.027	2163	2173	2216	rVV	332907	668263	55.25%	7.189%
58	8.538	2330	2332	2337	rVB2	326	241	0.02%	0.003%
59	8.616	2351	2356	2361	rBV3	265	375	0.03%	0.004%
60	8.725	2387	2390	2393	rVB2	208	157	0.01%	0.002%
61	8.741	2393	2395	2397	rBV	207	115	0.01%	0.001%
62	8.783	2397	2408	2439	rBV	492135	823516	68.08%	8.859%
63	9.079	2497	2500	2502	rVB	351	203	0.02%	0.002%
64	9.124	2512	2514	2521	rVB4	271	202	0.02%	0.002%
65	9.272	2557	2560	2567	rVB3	410	437	0.04%	0.005%
66	9.307	2567	2571	2572	rBV	203	134	0.01%	0.001%
67	9.516	2631	2636	2640	rBV3	374	431	0.04%	0.005%
68	9.580	2653	2656	2658	rVV2	232	109	0.01%	0.001%
69	9.612	2662	2666	2671	rVB2	314	280	0.02%	0.003%
70	9.638	2671	2674	2675	rBV2	281	141	0.01%	0.002%
71	9.715	2695	2698	2700	rBV	144	96	0.01%	0.001%
72	9.744	2704	2707	2710	rVB2	192	115	0.01%	0.001%
73	9.805	2723	2726	2728	rBV	178	124	0.01%	0.001%
74	9.850	2738	2740	2744	rVB	223	152	0.01%	0.002%
75	9.873	2744	2747	2751	rBV2	221	190	0.02%	0.002%
76	9.937	2762	2767	2771	rVB2	288	236	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034614.D
 Acq On : 14 Mar 2024 19:26
 Operator : SY/MD
 Sample : P1751-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.027	2793	2795	2800	rVB2	236	143	0.01%	0.002%
78	10.059	2800	2805	2807	rBV2	254	211	0.02%	0.002%
79	10.153	2822	2834	2861	rBV	350955	550682	45.53%	5.924%
80	10.323	2883	2887	2900	rVB4	3602	5048	0.42%	0.054%
81	10.394	2906	2909	2912	rBV	197	151	0.01%	0.002%
82	10.448	2924	2926	2928	rBV	161	80	0.01%	0.001%
83	10.728	3009	3013	3016	rBV2	142	135	0.01%	0.001%
84	11.043	3107	3111	3114	rBV	252	215	0.02%	0.002%
85	11.185	3144	3155	3181	rBV	493853	776365	64.19%	8.351%
86	11.558	3261	3271	3292	rVB	510540	813045	67.22%	8.746%
87	11.770	3335	3337	3340	rVB	465	217	0.02%	0.002%
88	11.812	3348	3350	3353	rVB2	522	285	0.02%	0.003%
89	11.834	3353	3357	3359	rBV2	314	248	0.02%	0.003%
90	11.895	3374	3376	3378	rBV2	204	106	0.01%	0.001%
91	12.181	3461	3465	3466	rBV	553	372	0.03%	0.004%
92	12.313	3503	3506	3509	rBV	263	232	0.02%	0.002%
93	12.432	3541	3543	3545	rVB	286	76	0.01%	0.001%
94	12.609	3595	3598	3600	rBV	264	148	0.01%	0.002%
95	12.689	3620	3623	3627	rBV	384	334	0.03%	0.004%
96	13.156	3765	3768	3769	rBV	352	159	0.01%	0.002%
97	13.580	3899	3900	3902	rBV	225	82	0.01%	0.001%
98	13.689	3930	3934	3938	rBV2	354	374	0.03%	0.004%
99	13.722	3941	3944	3946	rBV2	367	206	0.02%	0.002%
100	13.734	3946	3948	3954	rBV2	424	403	0.03%	0.004%




Sum of corrected areas: 9296201

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034614.D
Acq On : 14 Mar 2024 19:26
Operator : SY/MD
Sample : P1751-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

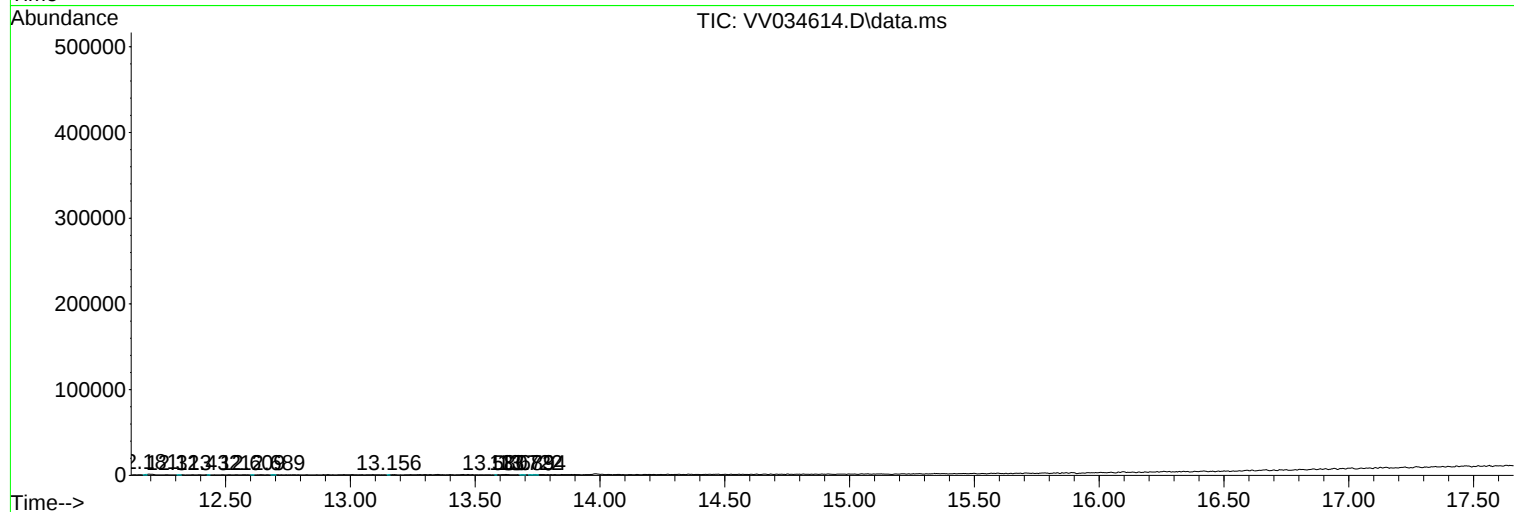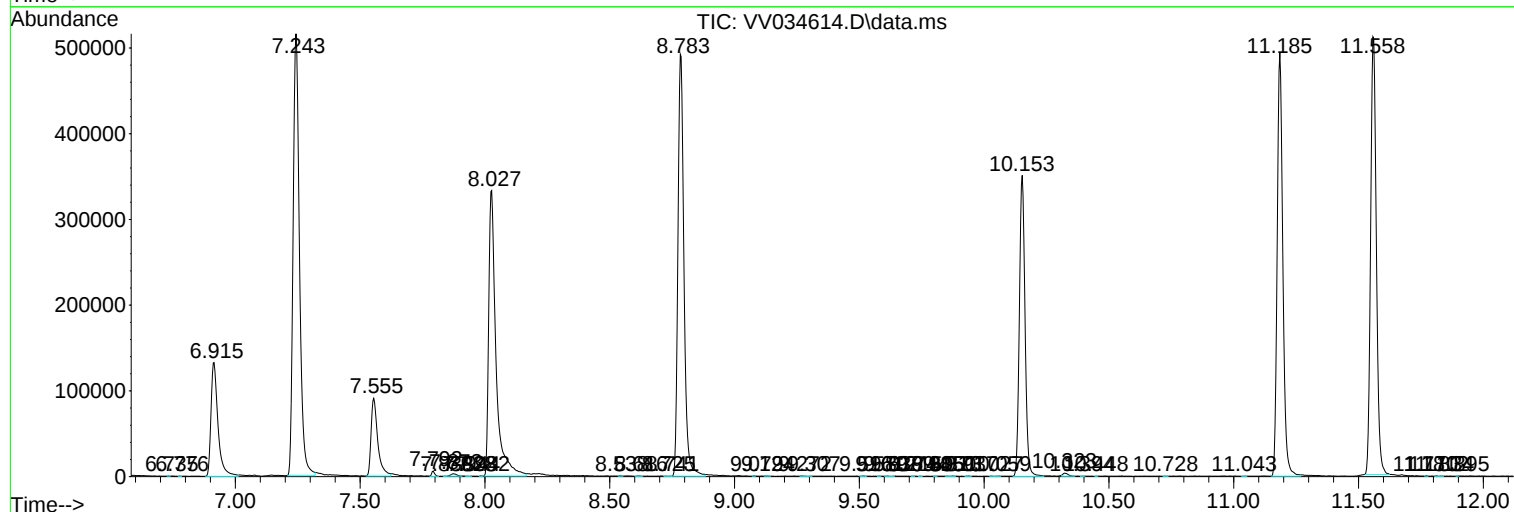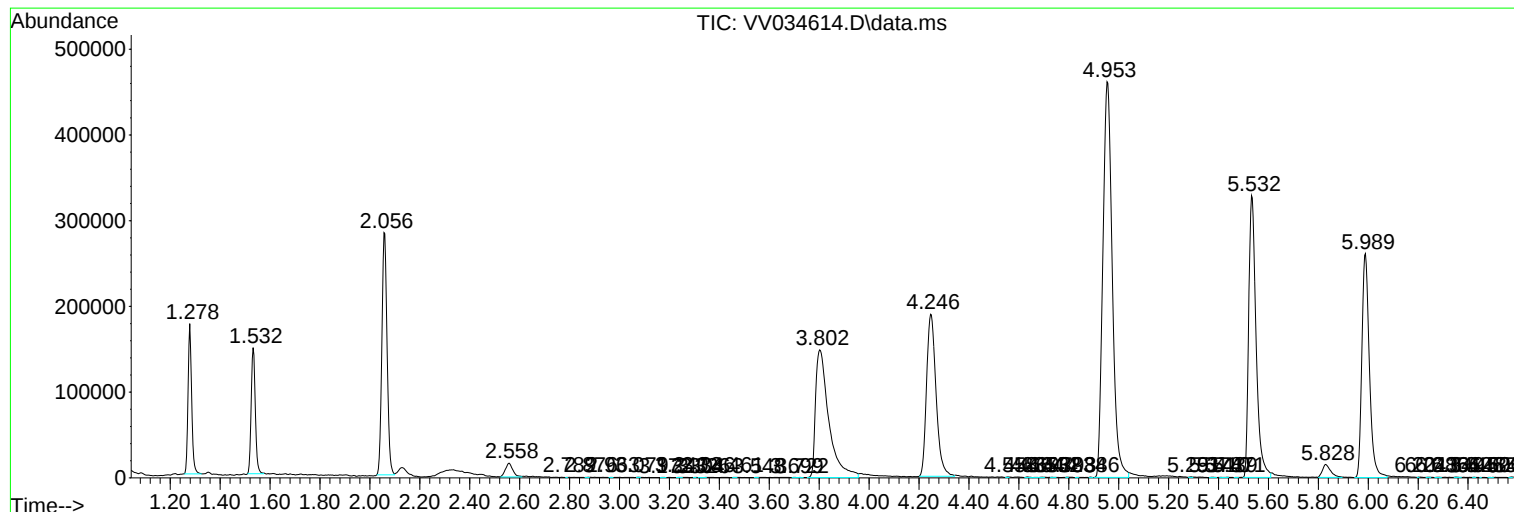

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034614.D
Acq On : 14 Mar 2024 19:26
Operator : SY/MD
Sample : P1751-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034614.D
Acq On : 14 Mar 2024 19:26
Operator : SY/MD
Sample : P1751-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------