

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034617.D
 Acq On : 14 Mar 2024 21:02
 Operator : SY/MD
 Sample : P1751-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M

Title : VOC Analysis

Signal : TIC: VV034617.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.192	43	47	58	rBV	13576	12122	0.92%	0.119%
2	1.278	68	74	88	rVB	178307	187528	14.30%	1.835%
3	1.532	146	153	171	rVB	156848	181613	13.85%	1.777%
4	2.063	307	318	329	rBV3	493681	839011	63.99%	8.208%
5	2.127	330	338	366	rVB	181190	417297	31.83%	4.083%
6	2.954	589	595	597	rBV2	450	408	0.03%	0.004%
7	2.970	597	600	603	rVB	257	184	0.01%	0.002%
8	3.034	619	620	622	rBV	225	92	0.01%	0.001%
9	3.118	632	646	668	rVB2	13519	29821	2.27%	0.292%
10	3.346	715	717	719	rBV	121	72	0.01%	0.001%
11	3.391	729	731	736	rBV2	178	127	0.01%	0.001%
12	3.446	744	748	751	rBV2	188	123	0.01%	0.001%
13	3.529	771	774	777	rBV2	231	168	0.01%	0.002%
14	3.577	785	789	793	rVB	206	165	0.01%	0.002%
15	3.597	793	795	797	rBV	146	71	0.01%	0.001%
16	3.664	813	816	820	rVB2	116	104	0.01%	0.001%
17	3.690	820	824	828	rBV	138	152	0.01%	0.001%
18	3.738	835	839	844	rBV3	257	279	0.02%	0.003%
19	3.802	848	859	897	rBV2	118219	408670	31.17%	3.998%
20	4.249	982	998	1027	rBV2	210456	553031	42.18%	5.411%
21	4.741	1146	1151	1153	rBV3	403	366	0.03%	0.004%
22	4.773	1160	1161	1164	rBV	157	60	0.00%	0.001%
23	4.790	1164	1166	1169	rVV2	223	105	0.01%	0.001%
24	4.902	1195	1201	1202	rBV4	380	412	0.03%	0.004%
25	4.954	1202	1217	1264	rVV2	493080	1311071	100.00%	12.827%
26	5.327	1331	1333	1335	rVB2	314	105	0.01%	0.001%
27	5.436	1364	1367	1371	rVB	412	249	0.02%	0.002%
28	5.458	1371	1374	1376	rBV3	231	143	0.01%	0.001%
29	5.471	1376	1378	1382	rVV	158	107	0.01%	0.001%
30	5.535	1387	1398	1431	rBV	261516	546104	41.65%	5.343%
31	5.838	1479	1492	1514	rBV3	102683	222070	16.94%	2.173%
32	5.989	1526	1539	1566	rBV	271849	572876	43.70%	5.605%
33	6.285	1629	1631	1635	rVB	408	201	0.02%	0.002%
34	6.314	1636	1640	1643	rBV2	173	126	0.01%	0.001%
35	6.378	1658	1660	1662	rBV	264	113	0.01%	0.001%
36	6.510	1692	1701	1718	rVB5	4229	9066	0.69%	0.089%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034617.D
 Acq On : 14 Mar 2024 21:02
 Operator : SY/MD
 Sample : P1751-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.577	1718	1722	1724	rBV3	993	902	0.07%	0.009%
38	6.757	1776	1778	1780	rBV2	219	119	0.01%	0.001%
39	6.793	1785	1789	1792	rVB3	342	241	0.02%	0.002%
40	6.812	1792	1795	1796	rBV	181	99	0.01%	0.001%
41	6.828	1798	1800	1802	rBV2	171	64	0.00%	0.001%
42	6.915	1815	1827	1860	rBV	137363	269974	20.59%	2.641%
43	7.198	1912	1915	1917	rBV2	441	256	0.02%	0.003%
44	7.243	1917	1929	1954	rBV	561389	980375	74.78%	9.591%
45	7.555	2013	2026	2054	rBV	96090	178349	13.60%	1.745%
46	7.767	2090	2092	2095	rVB3	327	122	0.01%	0.001%
47	7.783	2095	2097	2100	rBV2	314	129	0.01%	0.001%
48	7.841	2112	2115	2117	rVB2	194	106	0.01%	0.001%
49	7.876	2117	2126	2137	rVB3	2706	4729	0.36%	0.046%
50	7.931	2140	2143	2146	rBV2	271	209	0.02%	0.002%
51	7.986	2156	2160	2162	rVB2	317	218	0.02%	0.002%
52	8.024	2162	2172	2218	rBV	364359	720854	54.98%	7.052%
53	8.442	2299	2302	2304	rBV	460	245	0.02%	0.002%
54	8.542	2331	2333	2342	rBV3	381	485	0.04%	0.005%
55	8.622	2355	2358	2360	rBV	201	115	0.01%	0.001%
56	8.641	2360	2364	2367	rVV2	313	288	0.02%	0.003%
57	8.696	2377	2381	2383	rBV2	203	162	0.01%	0.002%
58	8.783	2398	2408	2442	rBV	394591	663762	50.63%	6.494%
59	8.995	2472	2474	2476	rBV2	500	291	0.02%	0.003%
60	9.085	2500	2502	2503	rBV2	216	112	0.01%	0.001%
61	9.124	2512	2514	2517	rVB2	223	138	0.01%	0.001%
62	9.169	2527	2528	2531	rVB2	180	67	0.01%	0.001%
63	9.249	2551	2553	2559	rBV2	168	113	0.01%	0.001%
64	9.317	2570	2574	2577	rVB2	363	270	0.02%	0.003%
65	9.333	2577	2579	2583	rVB2	124	75	0.01%	0.001%
66	9.362	2583	2588	2589	rBV2	143	125	0.01%	0.001%
67	9.391	2594	2597	2599	rBV	162	98	0.01%	0.001%
68	9.410	2599	2603	2607	rBV	247	237	0.02%	0.002%
69	9.490	2622	2628	2632	rBV2	493	484	0.04%	0.005%
70	9.567	2649	2652	2653	rBV2	225	118	0.01%	0.001%
71	9.596	2660	2661	2665	rVB2	167	61	0.00%	0.001%
72	9.629	2668	2671	2675	rVV	274	221	0.02%	0.002%
73	9.670	2680	2684	2685	rBV	185	124	0.01%	0.001%
74	9.693	2689	2691	2693	rVB	168	63	0.00%	0.001%
75	9.744	2704	2707	2711	rBV	185	136	0.01%	0.001%
76	9.764	2711	2713	2715	rBV2	205	121	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034617.D
 Acq On : 14 Mar 2024 21:02
 Operator : SY/MD
 Sample : P1751-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	9.905	2755	2757	2758	rBV2	271	108	0.01%	0.001%
78	9.960	2767	2774	2778	rBV4	964	1343	0.10%	0.013%
79	10.056	2803	2804	2807	rBV2	191	109	0.01%	0.001%
80	10.076	2807	2810	2814	rVV2	200	195	0.01%	0.002%
81	10.153	2822	2834	2861	rBV	377680	604694	46.12%	5.916%
82	10.477	2932	2935	2939	rBV2	359	343	0.03%	0.003%
83	10.561	2958	2961	2965	rBV2	185	162	0.01%	0.002%
84	10.706	3002	3006	3008	rVV2	221	127	0.01%	0.001%
85	10.764	3022	3024	3028	rBV2	251	205	0.02%	0.002%
86	10.866	3048	3056	3057	rBV2	443	474	0.04%	0.005%
87	11.111	3130	3132	3135	rBV2	168	101	0.01%	0.001%
88	11.130	3135	3138	3139	rBV2	353	260	0.02%	0.003%
89	11.185	3144	3155	3181	rBV	391000	612926	46.75%	5.997%
90	11.561	3259	3272	3294	rBV	549711	874930	66.73%	8.560%
91	11.921	3379	3384	3387	rBV	230	222	0.02%	0.002%
92	11.982	3401	3403	3406	rBV2	164	92	0.01%	0.001%
93	12.294	3498	3500	3503	rBV2	463	332	0.03%	0.003%
94	12.452	3546	3549	3550	rBV	474	247	0.02%	0.002%
95	12.484	3556	3559	3561	rBV	255	179	0.01%	0.002%
96	12.574	3584	3587	3589	rBV	303	165	0.01%	0.002%
97	12.590	3589	3592	3599	rVB3	382	476	0.04%	0.005%
98	13.098	3745	3750	3754	rBV2	376	385	0.03%	0.004%
99	13.458	3855	3862	3871	rBV3	2707	3964	0.30%	0.039%
100	13.677	3927	3930	3931	rBV	606	389	0.03%	0.004%




Sum of corrected areas: 10221297

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034617.D
Acq On : 14 Mar 2024 21:02
Operator : SY/MD
Sample : P1751-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

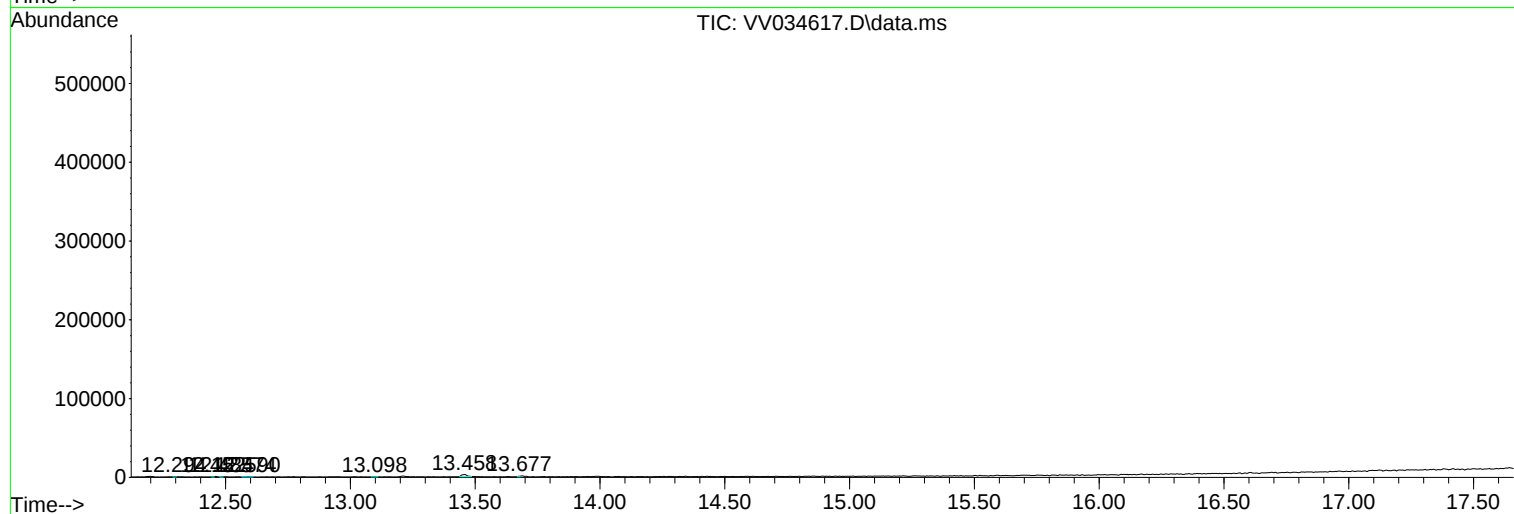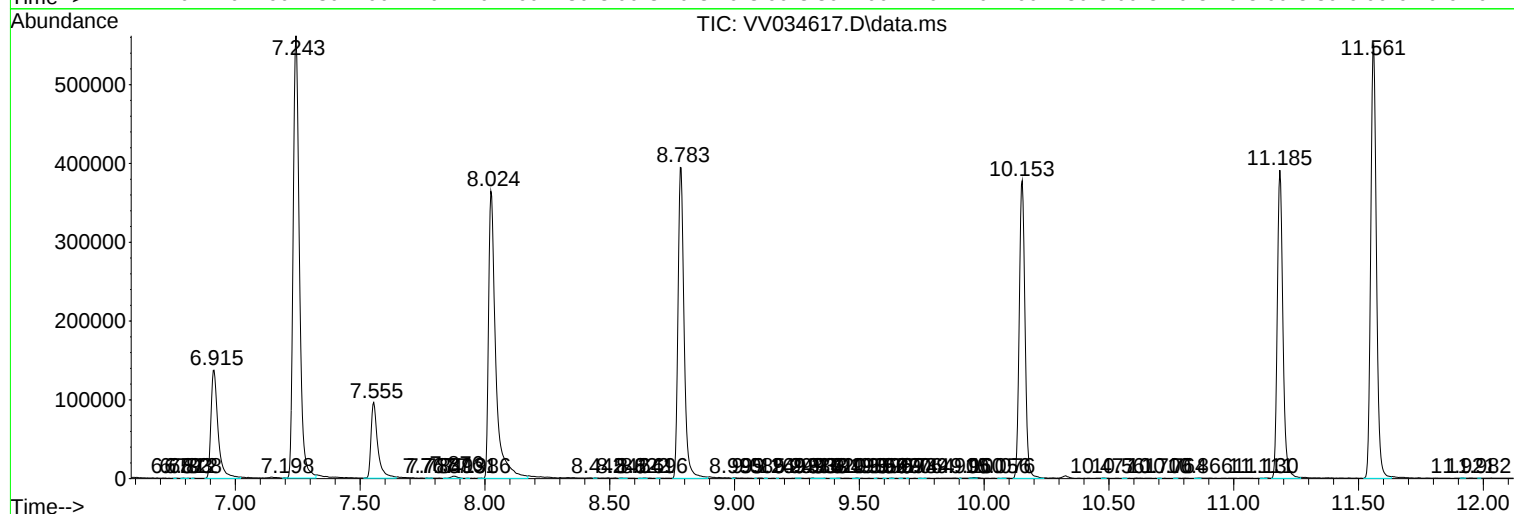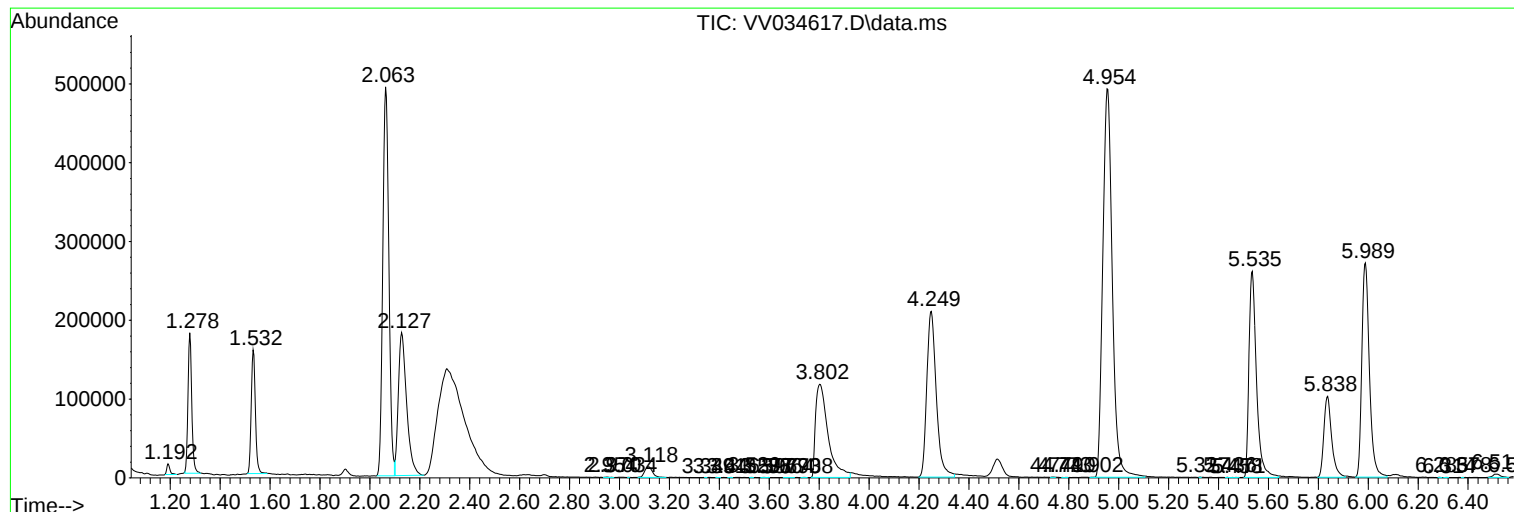

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034617.D
Acq On : 14 Mar 2024 21:02
Operator : SY/MD
Sample : P1751-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034617.D
Acq On : 14 Mar 2024 21:02
Operator : SY/MD
Sample : P1751-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc