

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034618.D
 Acq On : 14 Mar 2024 21:26
 Operator : SY/MD
 Sample : P1751-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	43	47	60	rBV	13005	14141	1.11%	0.139%
2	1.278	67	74	89	rVB	190326	213605	16.76%	2.099%
3	1.532	146	153	169	rVB	161867	184214	14.45%	1.810%
4	2.063	307	318	329	rBV3	471928	792035	62.14%	7.784%
5	2.127	330	338	366	rVB	229352	507876	39.84%	4.991%
6	2.963	595	598	600	rBV3	438	302	0.02%	0.003%
7	3.114	630	645	663	rBV	14722	31347	2.46%	0.308%
8	3.227	679	680	683	rVB2	360	158	0.01%	0.002%
9	3.265	689	692	693	rBV2	111	55	0.00%	0.001%
10	3.301	701	703	705	rBV	92	53	0.00%	0.001%
11	3.317	705	708	712	rVV3	488	261	0.02%	0.003%
12	3.333	712	713	714	rVB3	89	19	0.00%	0.000%
13	3.487	756	761	766	rBV	166	204	0.02%	0.002%
14	3.577	787	789	792	rVB	153	71	0.01%	0.001%
15	3.616	799	801	806	rVB2	294	135	0.01%	0.001%
16	3.699	824	827	829	rBV2	236	161	0.01%	0.002%
17	3.712	829	831	834	rVV2	231	129	0.01%	0.001%
18	3.802	848	859	906	rBV2	115967	415274	32.58%	4.081%
19	4.249	982	998	1032	rBV	205302	537699	42.18%	5.285%
20	4.767	1154	1159	1162	rBV2	488	507	0.04%	0.005%
21	4.863	1187	1189	1190	rBV	254	128	0.01%	0.001%
22	4.956	1202	1218	1250	rBV2	478737	1274673	100.00%	12.528%
23	5.339	1333	1337	1340	rBV2	525	363	0.03%	0.004%
24	5.391	1351	1353	1355	rBV	229	77	0.01%	0.001%
25	5.535	1386	1398	1425	rBV	276078	575234	45.13%	5.653%
26	5.837	1479	1492	1510	rBV5	64955	144470	11.33%	1.420%
27	5.989	1526	1539	1565	rBV	275343	575251	45.13%	5.654%
28	6.236	1613	1616	1617	rBV	209	85	0.01%	0.001%
29	6.246	1617	1619	1624	rVV2	303	249	0.02%	0.002%
30	6.265	1624	1625	1628	rVV	272	130	0.01%	0.001%
31	6.278	1628	1629	1635	rVB	361	207	0.02%	0.002%
32	6.378	1658	1660	1663	rVB2	441	187	0.01%	0.002%
33	6.400	1663	1667	1668	rBV	102	71	0.01%	0.001%
34	6.410	1668	1670	1673	rVV2	158	68	0.01%	0.001%
35	6.516	1693	1703	1706	rBV3	963	1666	0.13%	0.016%
36	6.561	1715	1717	1719	rBV	314	164	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034618.D
 Acq On : 14 Mar 2024 21:26
 Operator : SY/MD
 Sample : P1751-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.583	1719	1724	1725	rBV2	764	511	0.04%	0.005%
38	6.731	1769	1770	1777	rBV3	386	405	0.03%	0.004%
39	6.828	1797	1800	1804	rBV2	274	233	0.02%	0.002%
40	6.915	1816	1827	1848	rBV	137716	261718	20.53%	2.572%
41	7.140	1891	1897	1903	rBV5	1174	1954	0.15%	0.019%
42	7.243	1918	1929	1953	rBV	548782	964631	75.68%	9.480%
43	7.554	2014	2026	2056	rBV	93741	178605	14.01%	1.755%
44	7.725	2078	2079	2081	rVB	300	114	0.01%	0.001%
45	7.741	2081	2084	2088	rBV2	466	368	0.03%	0.004%
46	7.850	2115	2118	2119	rBV2	350	185	0.01%	0.002%
47	7.879	2120	2127	2135	rVB3	2686	4420	0.35%	0.043%
48	8.024	2163	2172	2212	rBV	361312	710681	55.75%	6.985%
49	8.538	2330	2332	2337	rVB2	250	208	0.02%	0.002%
50	8.561	2337	2339	2340	rBV	272	116	0.01%	0.001%
51	8.596	2348	2350	2351	rBV2	285	91	0.01%	0.001%
52	8.699	2379	2382	2387	rBV2	281	294	0.02%	0.003%
53	8.738	2391	2394	2396	rBV	196	113	0.01%	0.001%
54	8.786	2397	2409	2435	rBV	416559	695661	54.58%	6.837%
55	9.075	2498	2499	2501	rBV	393	124	0.01%	0.001%
56	9.091	2501	2504	2508	rVV2	354	298	0.02%	0.003%
57	9.181	2529	2532	2537	rBV2	201	188	0.01%	0.002%
58	9.204	2537	2539	2542	rVB	289	178	0.01%	0.002%
59	9.329	2577	2578	2581	rBV	117	41	0.00%	0.000%
60	9.361	2586	2588	2591	rBV2	133	98	0.01%	0.001%
61	9.378	2591	2593	2595	rVB2	168	70	0.01%	0.001%
62	9.435	2609	2611	2614	rVB	326	143	0.01%	0.001%
63	9.490	2626	2628	2632	rBV	216	95	0.01%	0.001%
64	9.522	2636	2638	2640	rBV	290	122	0.01%	0.001%
65	9.619	2667	2668	2669	rBV	143	41	0.00%	0.000%
66	9.770	2714	2715	2717	rBV2	79	28	0.00%	0.000%
67	9.834	2732	2735	2737	rBV2	178	118	0.01%	0.001%
68	9.869	2744	2746	2749	rVB2	296	165	0.01%	0.002%
69	10.021	2790	2793	2797	rBV2	199	128	0.01%	0.001%
70	10.040	2797	2799	2802	rBV2	293	158	0.01%	0.002%
71	10.152	2821	2834	2854	rBV	380293	599802	47.06%	5.895%
72	10.281	2869	2874	2878	rVB3	468	446	0.03%	0.004%
73	10.326	2878	2888	2896	rBV4	3963	6385	0.50%	0.063%
74	10.381	2900	2905	2908	rBV	218	244	0.02%	0.002%
75	10.480	2933	2936	2938	rBV	426	299	0.02%	0.003%
76	10.603	2973	2974	2975	rVB	202	39	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
 Data File : VV034618.D
 Acq On : 14 Mar 2024 21:26
 Operator : SY/MD
 Sample : P1751-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.641	2982	2986	2989	rBV	378	263	0.02%	0.003%
78	10.673	2993	2996	3000	rBV2	183	170	0.01%	0.002%
79	11.111	3129	3132	3134	rBV	251	140	0.01%	0.001%
80	11.185	3145	3155	3178	rBV	377678	595195	46.69%	5.850%
81	11.561	3260	3272	3296	rBV	545193	872982	68.49%	8.580%
82	11.860	3363	3365	3369	rBV	235	191	0.01%	0.002%
83	12.040	3420	3421	3422	rBV	258	60	0.00%	0.001%
84	12.104	3438	3441	3442	rBV	252	145	0.01%	0.001%
85	12.175	3460	3463	3464	rBV	495	258	0.02%	0.003%
86	12.377	3524	3526	3530	rBV	242	163	0.01%	0.002%
87	12.590	3590	3592	3597	rBV2	308	196	0.02%	0.002%
88	12.805	3655	3659	3664	rBV3	452	408	0.03%	0.004%
89	12.998	3716	3719	3727	rVB2	304	241	0.02%	0.002%
90	13.242	3793	3795	3797	rBV	292	109	0.01%	0.001%
91	13.455	3854	3861	3866	rBV3	1404	1846	0.14%	0.018%
92	13.548	3887	3890	3895	rBV3	444	398	0.03%	0.004%
93	13.619	3908	3912	3914	rBV	382	336	0.03%	0.003%
94	13.667	3925	3927	3929	rBV2	293	110	0.01%	0.001%
95	13.985	4020	4026	4027	rBV2	1096	992	0.08%	0.010%




Sum of corrected areas: 10174990

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034618.D
Acq On : 14 Mar 2024 21:26
Operator : SY/MD
Sample : P1751-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

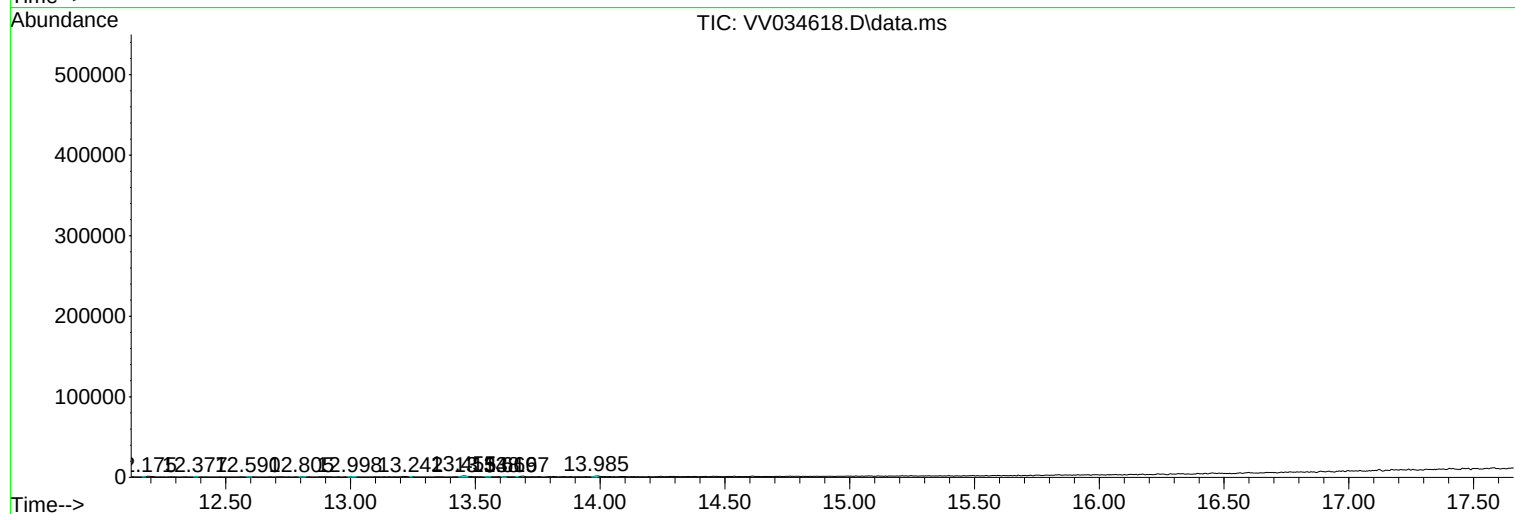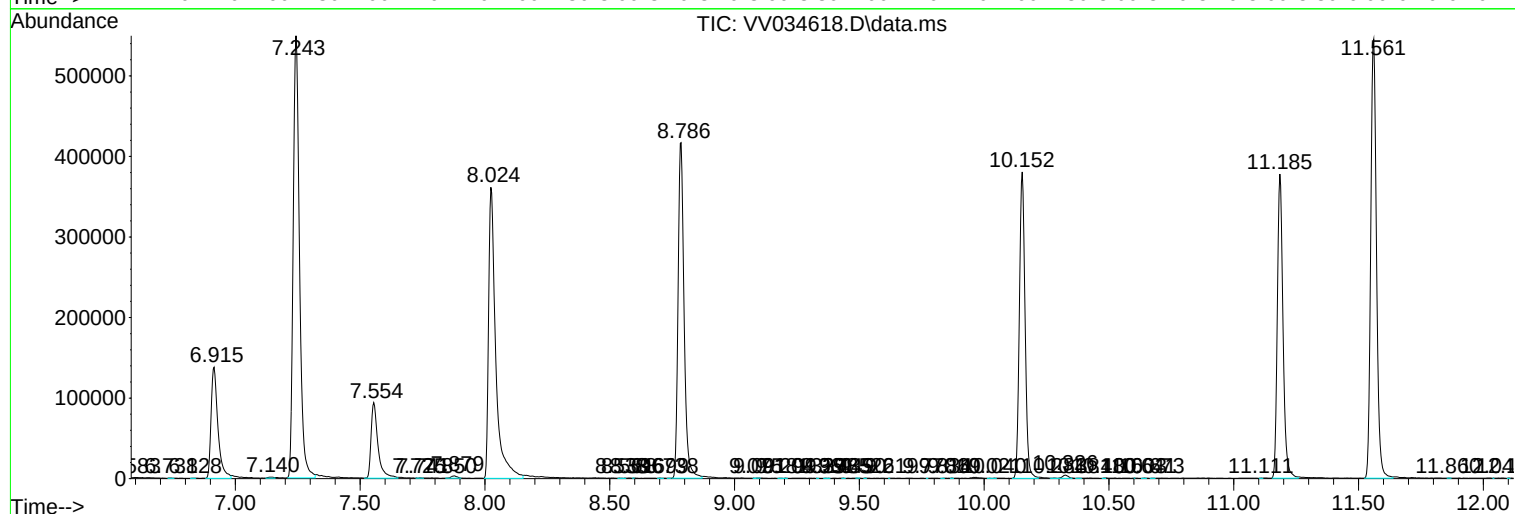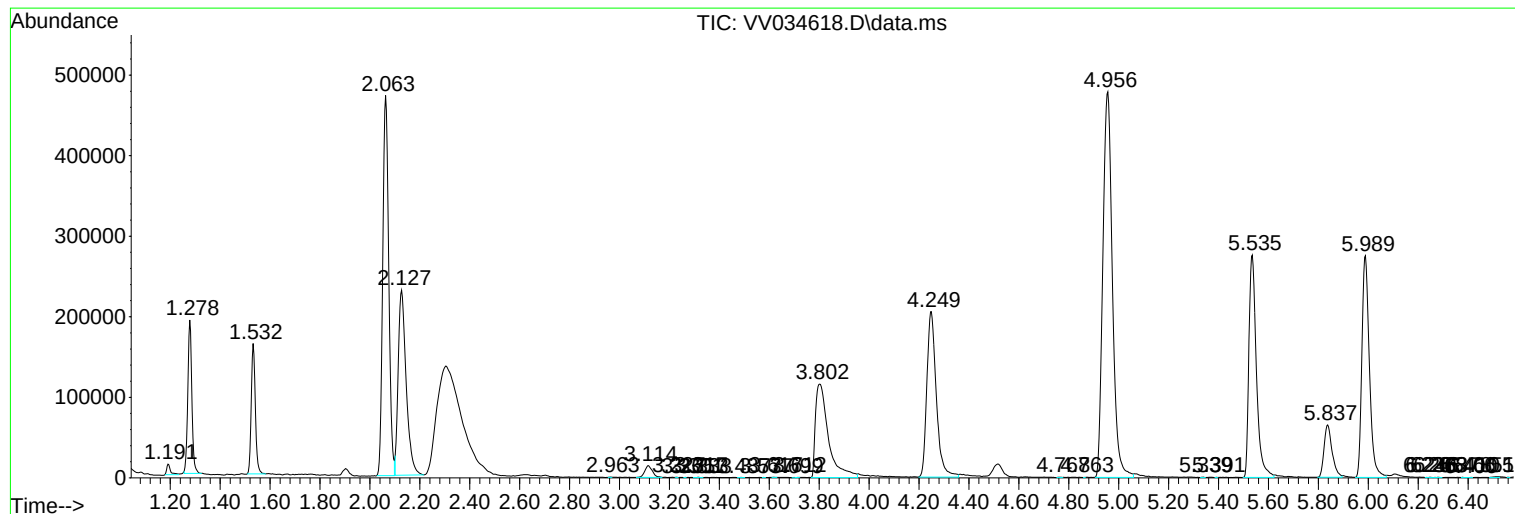

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034618.D
Acq On : 14 Mar 2024 21:26
Operator : SY/MD
Sample : P1751-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034618.D
Acq On : 14 Mar 2024 21:26
Operator : SY/MD
Sample : P1751-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------