


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031424\
Data File : VV034588.D
Acq On : 14 Mar 2024 08:39
Operator : SY/MD
Sample : BFB268
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB268

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Title : VOC Analysis
Last Update : Fri Mar 15 06:40:01 2024

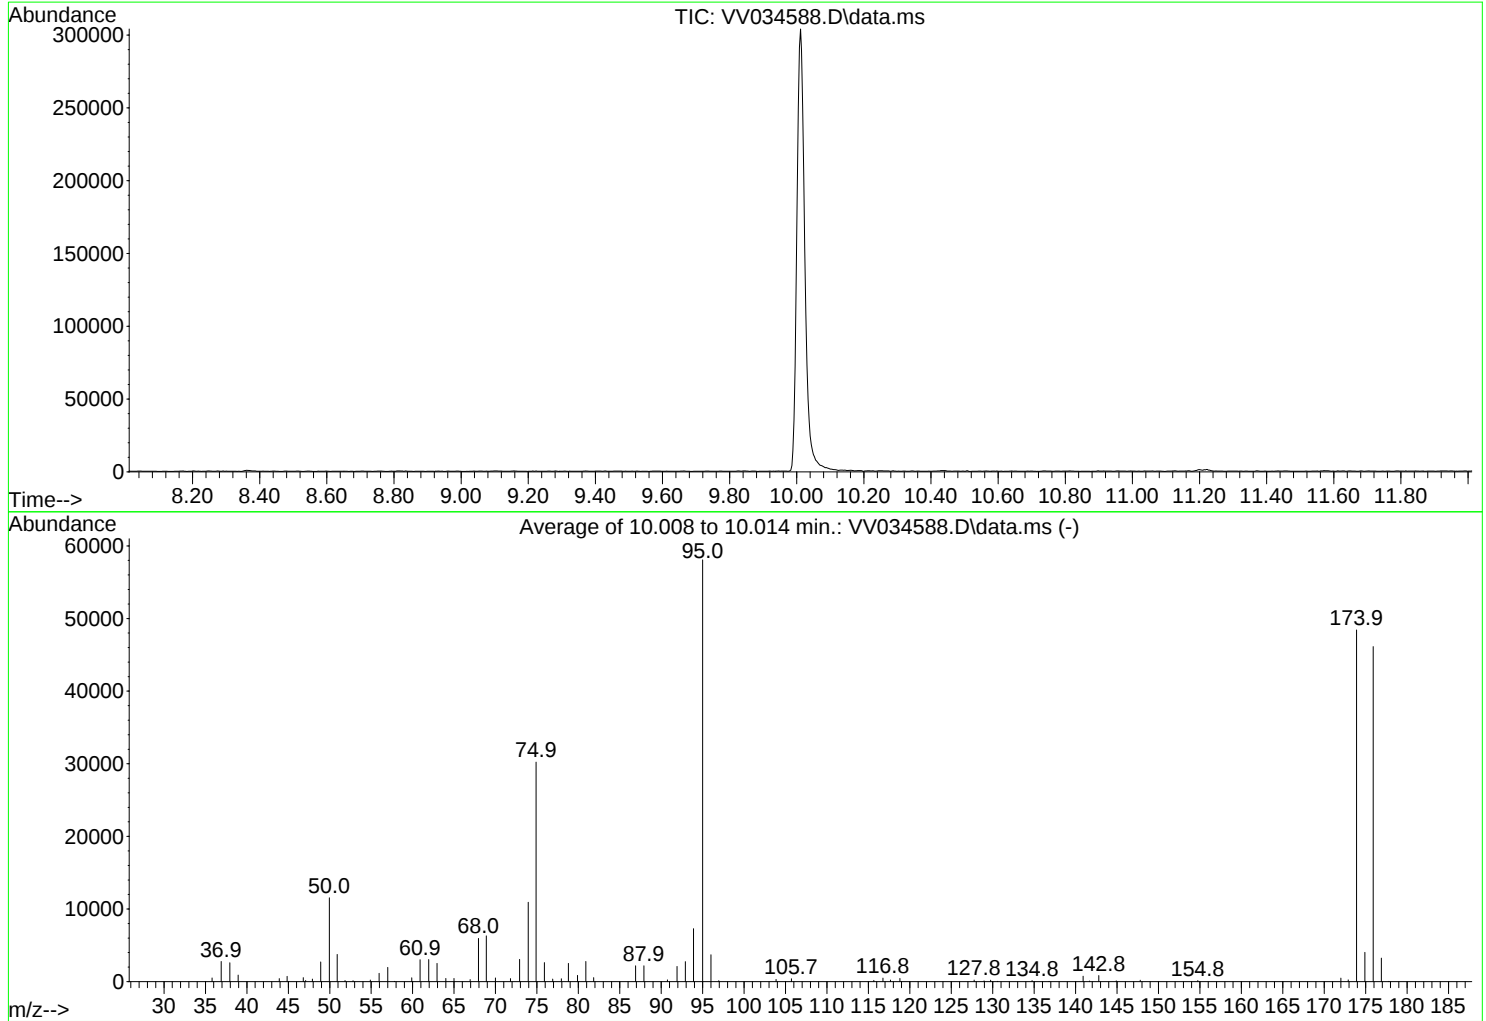

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	11543	PASS
75	95	30	80	52.1	30232	PASS
95	95	100	100	100.0	58080	PASS
96	95	5	9	6.4	3698	PASS
173	174	0.00	2	0.5	239	PASS
174	95	50	120	83.4	48437	PASS
175	174	5	9	8.3	4023	PASS
176	174	95	105	95.3	46147	PASS
177	176	5	10	7.0	3246	PASS

m/z	Abundance
39.90	238.0
43.90	252.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

m/z	Abundance
35.80	502.0
36.90	2886.0
37.90	2608.0
38.90	895.0
39.80	168.0
43.90	728.0
44.90	658.0
46.80	614.0
47.90	342.0
48.90	2741.0
50.00	11618.0
50.90	3685.0
51.80	190.0
52.80	148.0
54.90	165.0
55.90	1182.0
57.00	1899.0
59.90	486.0
60.90	3117.0
61.90	3051.0
62.90	2546.0
64.00	498.0
65.00	417.0
67.00	214.0
67.90	5967.0
68.90	6410.0
70.00	458.0
71.80	379.0
72.90	2997.0
74.00	11035.0
74.90	30608.0
75.90	2624.0
76.90	328.0
78.00	370.0
78.80	2517.0
79.90	870.0
80.90	2715.0
81.90	513.0
86.90	2168.0
87.90	2196.0
90.80	281.0
91.90	2013.0
92.90	2598.0
93.90	7284.0
95.00	57832.0
96.00	3517.0
96.90	110.0
103.90	249.0
105.70	405.0
115.70	162.0
116.70	456.0
117.60	174.0
118.80	415.0
127.80	195.0
129.00	106.0
129.80	214.0
130.60	117.0
134.70	149.0
140.90	683.0
142.80	780.0
147.80	174.0
154.80	149.0
172.00	495.0
173.90	47136.0
174.90	4006.0
175.90	45112.0
176.90	3084.0
177.80	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

m/z	Abundance
35.80	539.0
36.90	2850.0
38.00	2703.0
39.00	909.0
39.80	181.0
43.90	688.0
44.90	777.0
46.80	579.0
47.90	371.0
48.90	2811.0
49.90	11916.0
50.90	3865.0
51.90	167.0
52.80	143.0
54.90	214.0
55.90	1235.0
57.00	2055.0
59.90	530.0
60.90	3162.0
62.00	3174.0
62.90	2569.0
64.00	462.0
65.00	448.0
66.90	310.0
67.90	6157.0
68.90	6509.0
70.00	543.0
71.80	441.0
72.90	3231.0
74.00	11234.0
74.90	30976.0
75.90	2674.0
76.90	362.0
78.00	455.0
78.80	2542.0
79.90	887.0
80.90	2910.0
81.80	558.0
86.90	2235.0
87.90	2218.0
90.80	261.0
91.90	2127.0
92.90	2852.0
93.90	7598.0
95.00	59808.0
96.00	3858.0
96.90	141.0
103.80	323.0
105.70	422.0
115.60	200.0
116.80	502.0
117.70	222.0
118.80	452.0
127.70	220.0
129.00	126.0
129.70	193.0
134.70	147.0
140.90	765.0
141.70	119.0
142.80	892.0
144.90	134.0
147.80	214.0
154.70	165.0
172.00	507.0
173.90	50336.0
174.90	4216.0
175.90	47448.0
176.90	3364.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

m/z	Abundance
35.80	515.0
36.90	2584.0
38.00	2518.0
39.00	941.0
39.90	201.0
43.90	590.0
44.80	767.0
46.80	434.0
47.10	480.0
47.90	353.0
48.90	2561.0
49.90	11095.0
50.90	3660.0
51.90	130.0
52.80	103.0
54.90	256.0
56.00	1018.0
57.00	1929.0
57.80	105.0
59.90	551.0
60.90	2802.0
62.00	2911.0
63.00	2432.0
64.00	353.0
65.00	467.0
66.90	357.0
68.00	5737.0
68.90	5999.0
70.00	511.0
71.80	447.0
72.90	2941.0
73.90	10497.0
74.90	29112.0
75.90	2586.0
76.90	402.0
77.90	353.0
78.80	2447.0
79.90	804.0
80.90	2674.0
81.80	592.0
86.90	2145.0
87.90	2149.0
90.70	221.0
91.90	2130.0
92.90	2832.0
93.90	6979.0
95.00	56600.0
96.00	3718.0
97.00	134.0
103.80	330.0
105.70	352.0
115.60	195.0
116.80	470.0
117.70	248.0
118.80	446.0
127.70	214.0
128.90	126.0
129.70	200.0
134.80	146.0
136.80	113.0
140.90	783.0
141.70	134.0
142.80	841.0
144.90	205.0
147.80	191.0
154.70	152.0
172.00	488.0
172.90	717.0
173.90	47840.0
174.90	3846.0
175.90	45880.0
176.90	3290.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268