
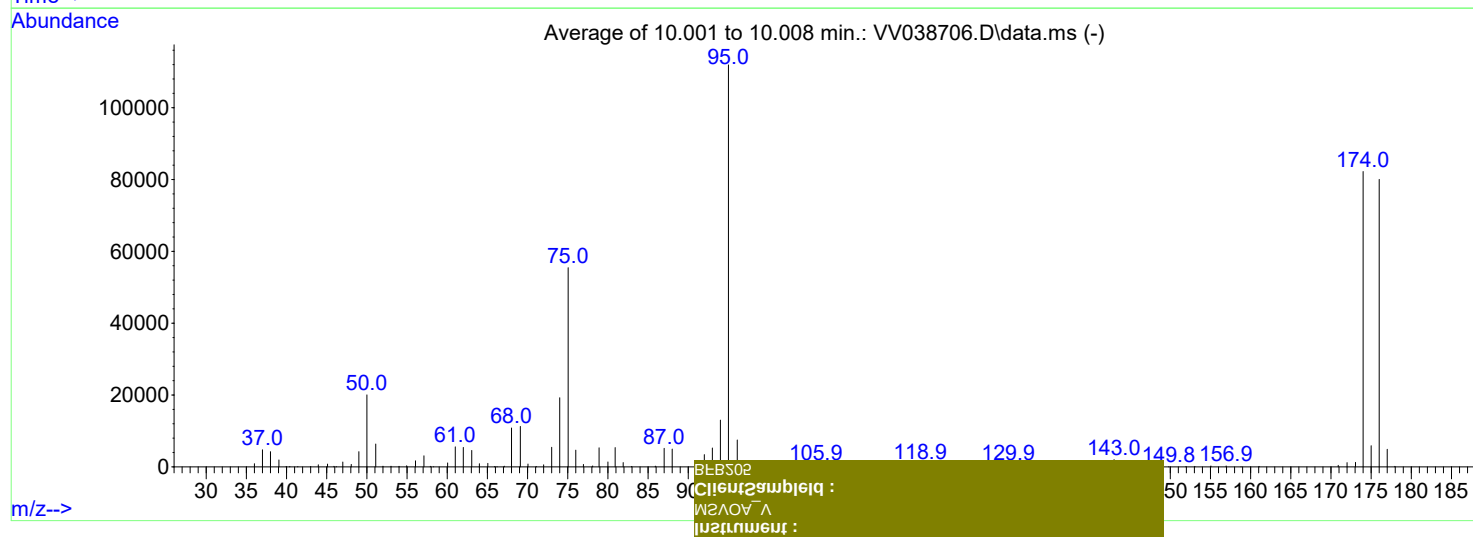


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031425\
Data File : VV038706.D
Acq On : 14 Mar 2025 08:54
Operator : SY/MD
Sample : BFB207
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031325WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Mar 13 13:15:04 2025

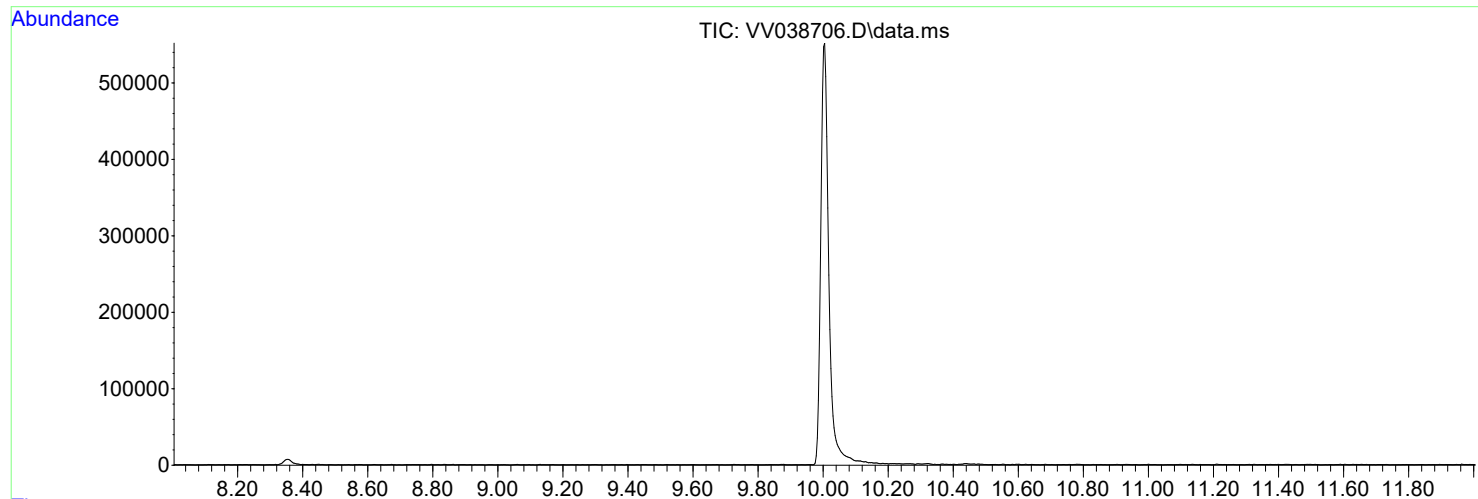

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	20048	PASS
75	95	30	80	49.5	55456	PASS
95	95	100	100	100.0	111920	PASS
96	95	5	9	6.7	7492	PASS
173	174	0.00	2	1.5	1252	PASS
174	95	50	120	73.5	82232	PASS
175	174	5	9	7.2	5893	PASS
176	174	95	105	97.3	80043	PASS
177	176	5	10	6.1	4896	PASS

m/z	Abundance
39.90	291.0
44.00	528.0

BFB207
Client Sample :
MS/MS
Instrument :

m/z	Abundance
36.00	895.0
37.00	5054.0
38.00	4617.0
39.00	1974.0
40.00	342.0
40.40	315.0
41.40	128.0
43.00	172.0
44.00	1090.0
45.10	815.0
45.90	270.0
47.00	1418.0
48.10	707.0
49.00	4240.0
50.00	20704.0
51.10	6566.0
52.00	202.0
53.00	209.0
54.10	198.0
54.90	289.0
56.00	1790.0
57.10	3188.0
57.90	193.0
60.00	1088.0
61.00	5516.0
62.00	5537.0
63.10	4753.0
64.00	841.0
65.00	1028.0
65.90	156.0
67.10	122.0
68.00	11246.0
69.10	11577.0
70.10	814.0
71.10	127.0
72.00	568.0
73.00	5569.0
74.00	20160.0
75.00	57640.0
76.00	4965.0
76.90	664.0
78.10	426.0
78.90	5451.0
80.00	1414.0
80.90	5502.0
81.90	1250.0
82.90	103.0
85.90	266.0
87.00	5388.0
88.00	5296.0
90.90	472.0
92.00	3487.0
93.00	5101.0
94.00	13317.0
95.00	113216.0
96.10	7484.0
97.00	350.0
103.90	438.0
104.90	160.0
105.90	576.0
106.90	148.0
111.00	205.0
111.80	120.0
112.80	111.0
114.90	161.0
115.90	642.0
117.00	859.0
118.00	439.0
118.90	875.0
127.90	470.0
129.00	185.0
129.90	517.0
130.90	325.0
134.90	260.0
136.90	216.0
140.90	1282.0
141.90	274.0
143.00	1941.0
143.90	151.0
144.90	1044.0
145.90	248.0
146.90	107.0
147.90	285.0
148.90	127.0
152.00	111.0
153.10	115.0
155.00	271.0
157.00	271.0
161.00	101.0
170.90	470.0
171.90	1159.0
173.10	1467.0

BEBS02
ClientSampleId :
MS2A047A
Instrument :

174.00	82424.0
175.00	6275.0
176.00	80776.0
177.00	5140.0
177.90	160.0

BEB502
Client :
MSAOA
Instrument :

m/z	Abundance
36.00	926.0
37.00	4900.0
38.00	4276.0
39.00	1953.0
40.00	384.0
41.40	106.0
43.00	136.0
44.00	1152.0
45.10	796.0
45.90	227.0
47.00	1422.0
48.00	734.0
49.00	4426.0
50.00	20704.0
51.10	6703.0
52.00	192.0
53.00	204.0
54.00	163.0
55.00	327.0
56.10	1741.0
57.10	3223.0
57.90	172.0
60.00	1157.0
61.00	5698.0
62.00	5481.0
63.10	4745.0
64.00	889.0
65.10	1029.0
65.90	141.0
67.10	194.0
68.00	11185.0
69.10	11515.0
70.00	797.0
71.10	125.0
72.00	611.0
73.00	5691.0
74.00	19832.0
75.10	57088.0
76.00	4775.0
77.00	686.0
78.90	5452.0
80.00	1423.0
80.90	5462.0
81.90	1192.0
83.00	127.0
85.90	204.0
87.00	5368.0
88.00	5169.0
90.90	483.0
92.00	3547.0
93.00	5431.0
94.00	13332.0
95.00	115712.0
96.10	7841.0
97.00	343.0
104.00	476.0
104.90	189.0
105.90	528.0
106.90	148.0
108.10	142.0
110.90	226.0
111.80	132.0
115.00	169.0
115.90	662.0
117.00	774.0
118.00	473.0
118.90	907.0
127.80	446.0
129.00	225.0
129.90	512.0
130.90	282.0
134.90	308.0
137.00	192.0
140.90	1281.0
141.90	245.0
143.00	2107.0
143.90	170.0
144.80	1024.0
145.90	202.0
147.90	269.0
149.00	104.0
151.90	112.0
153.00	146.0
155.00	257.0
157.00	287.0
161.10	136.0
170.90	460.0
172.00	1166.0
173.00	1275.0
174.00	84824.0
175.00	6047.0
176.00	82408.0

BFB207
Client Sample :
MS2007-1
Instrument :

177.00

178.00

4999.0

158.0

BEB502

Client :
MSAOA
Instrument :

m/z	Abundance
36.00	846.0
37.00	4330.0
38.00	3820.0
39.10	1868.0
40.10	400.0
43.90	1099.0
45.10	733.0
46.20	214.0
47.00	1226.0
48.00	641.0
49.00	4059.0
50.00	18736.0
51.10	5824.0
52.00	187.0
53.00	163.0
53.90	134.0
55.00	345.0
56.00	1550.0
57.10	2847.0
57.90	124.0
58.30	113.0
60.10	1070.0
61.00	5510.0
62.00	5225.0
63.00	4236.0
64.00	913.0
65.10	885.0
66.20	125.0
67.10	274.0
68.00	10065.0
69.10	10697.0
70.00	784.0
72.00	565.0
73.00	5113.0
74.00	17752.0
75.10	51640.0
76.00	4244.0
77.00	700.0
78.10	381.0
78.90	5040.0
80.00	1270.0
80.90	5161.0
81.90	1164.0
83.00	161.0
85.90	168.0
87.00	4734.0
88.00	4410.0
90.90	479.0
92.00	3216.0
93.00	5237.0
94.00	12411.0
95.00	106832.0
96.10	7151.0
97.10	261.0
104.00	496.0
104.90	186.0
105.90	462.0
106.90	141.0
108.10	173.0
110.90	178.0
115.00	144.0
115.90	554.0
117.10	721.0
117.90	507.0
118.90	860.0
127.90	360.0
129.00	229.0
129.90	421.0
131.00	236.0
134.90	285.0
137.00	154.0
140.90	1103.0
141.90	186.0
143.00	2023.0
143.90	164.0
144.80	893.0
145.90	147.0
147.90	242.0
149.80	113.0
151.90	102.0
153.00	158.0
155.10	242.0
156.90	234.0
158.80	117.0
161.10	165.0
170.90	385.0
172.10	1246.0
173.00	1013.0
174.00	79448.0
175.00	5358.0
176.00	76944.0
177.00	4549.0

BEBS02
ClientSampleId :
MS2A047A
Instrument :

178.00

147.0

BEBS02
Client :
Sample :
MS/MS
Instrument :