




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025014.D
 Acq On : 15 Mar 2022 22:03
 Operator : SY/MD
 Sample : N1933-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDC1

Manual IntegrationsAPPROVED

Quant Time: Mar 16 03:42:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 16 03:30:21 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

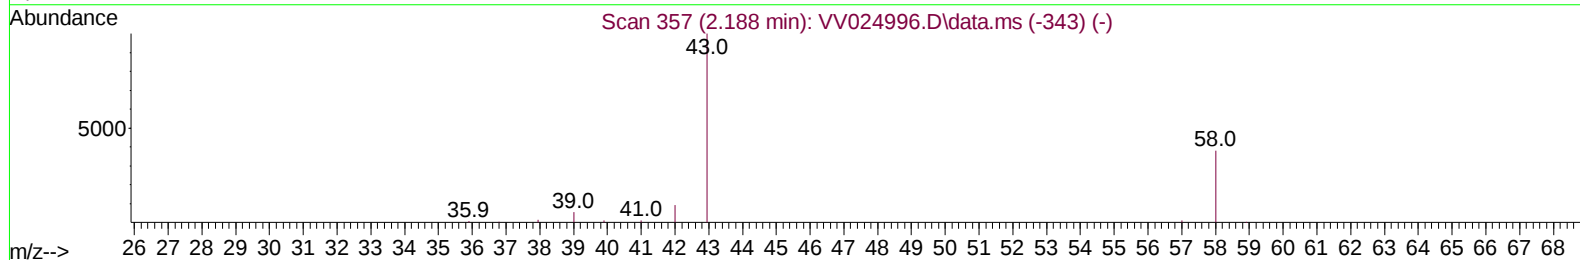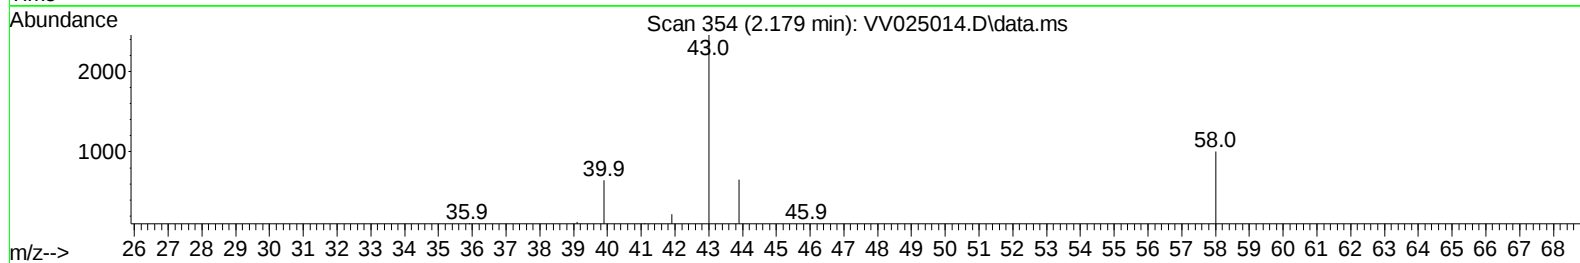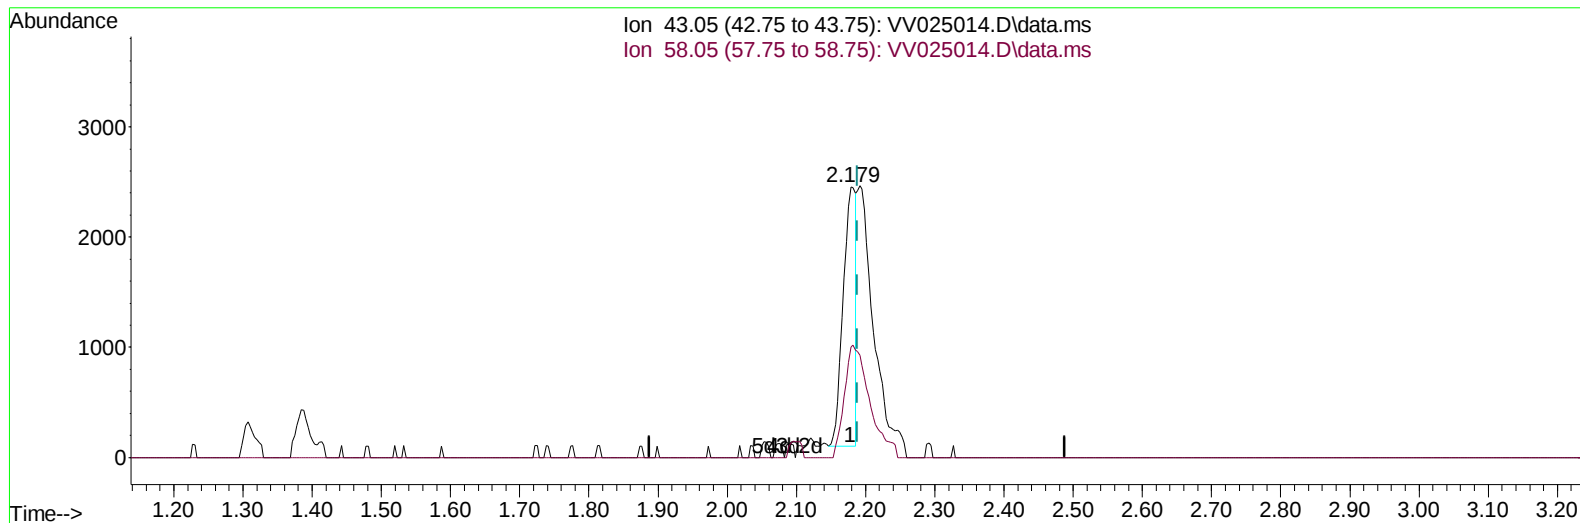

TIC: VV025014.D\data.ms

(13) Acetone (T)

2.179min (-0.009) 2.84 ug/L

response 2936

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.10	87.84#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025014.D
 Acq On : 15 Mar 2022 22:03
 Operator : SY/MD
 Sample : N1933-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDC1

Manual IntegrationsAPPROVED

Quant Time: Mar 16 03:42:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 16 03:30:21 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

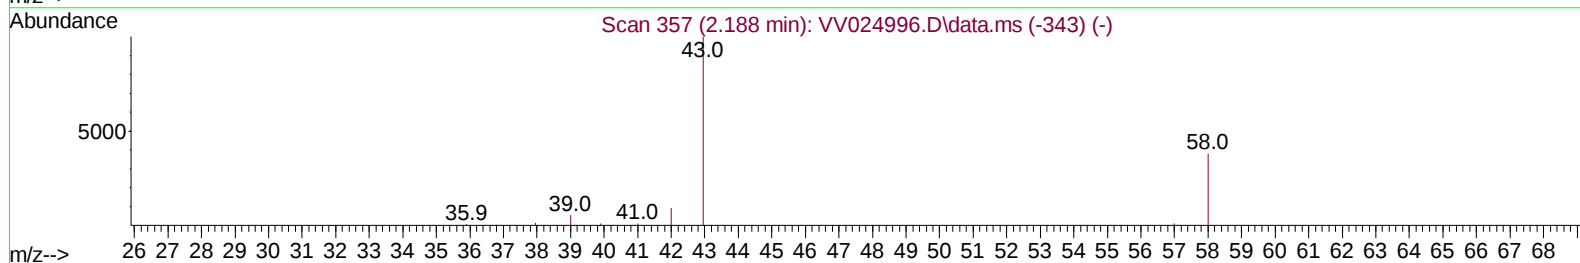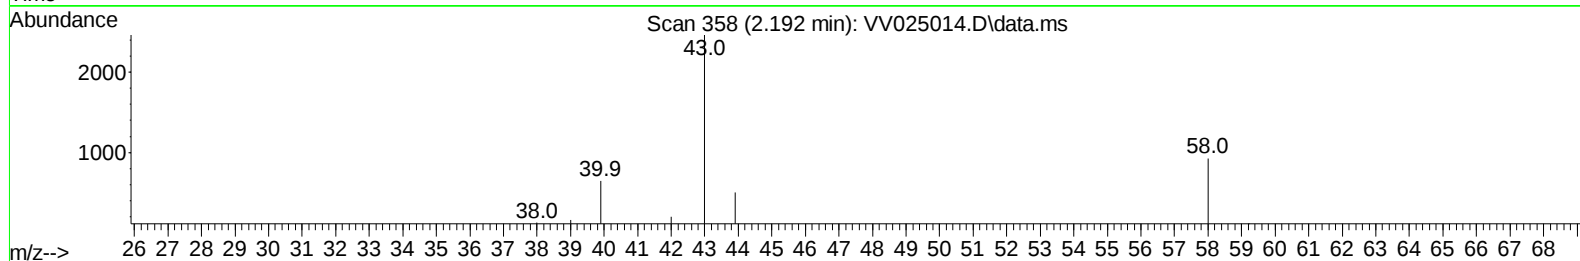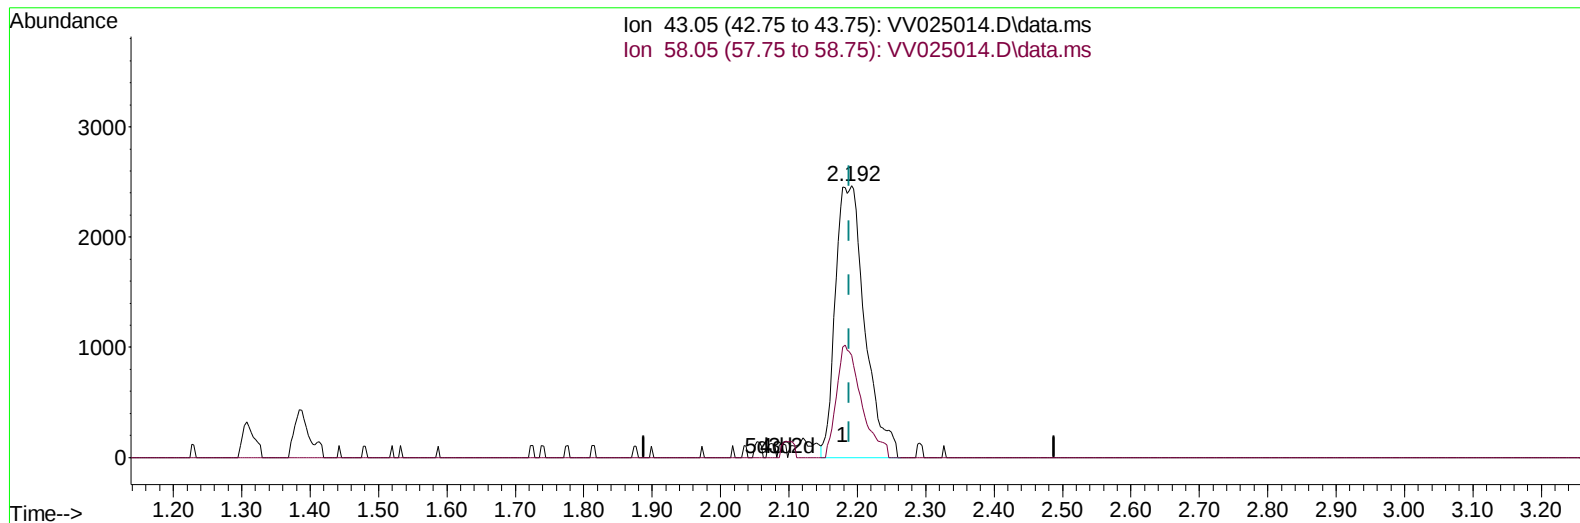

TIC: VV025014.D\data.ms

(13) Acetone (T)

2.192min (+ 0.003) 7.11 ug/L m

response 7354

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.10	35.07
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025014.D
 Acq On : 15 Mar 2022 22:03
 Operator : SY/MD
 Sample : N1933-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDC1

Manual IntegrationsAPPROVED

Quant Time: Mar 16 03:42:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 16 03:30:21 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/16/2022
 Supervised By :Mahesh Dadoda 03/16/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	162200	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	151804	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	66076	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	58882	4.598	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	92.000%		
7) Chloroethane-d5	1.568	69	45198	4.820	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	96.400%		
11) 1,1-Dichloroethene-d2	2.111	63	74294	3.590	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	71.800%		
20) 2-Butanone-d5	3.892	46	87439	56.500	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	113.000%		
24) Chloroform-d	4.349	84	99218	4.672	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	93.400%		
26) 1,2-Dichloroethane-d4	5.034	65	44521	5.014	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	100.200%		
32) Benzene-d6	5.050	84	209419	4.756	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	95.200%		
36) 1,2-Dichloropropane-d6	6.069	67	61951	4.892	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	97.800%		
41) Toluene-d8	7.317	98	180790	4.505	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	90.000%		
43) trans-1,3-Dichloroprop...	7.625	79	20140	4.562	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	91.200%		
46) 2-Hexanone-d5	8.088	63	70228	46.640	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	93.280%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	36414	4.888	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	97.800%		
66) 1,2-Dichlorobenzene-d4	11.622	152	57456	5.136	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	102.800%		
Target Compounds						
						Qvalue
13) Acetone	2.192	43	7354m	7.105	ug/L	
25) Chloroform	4.384	83	2746	0.125	ug/L	90
31) Carbon tetrachloride	4.831	117	175676	10.577	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025014.D
Acq On : 15 Mar 2022 22:03
Operator : SY/MD
Sample : N1933-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC1

Manual IntegrationsAPPROVED

Quant Time: Mar 16 03:42:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 16 03:30:21 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/16/2022
Supervised By :Mahesh Dadoda 03/16/2022

