

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031522\
 Data File : VW025003.D
 Acq On : 15 Mar 2022 17:46
 Operator : SY/MD
 Sample : N1934-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDD5

Quant Time: Mar 16 03:39:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 16 03:30:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	174437	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	166167	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	77493	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	58780	4.268	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.400%
7) Chloroethane-d5	1.568	69	45901	4.552	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.000%
11) 1,1-Dichloroethene-d2	2.108	63	74220	3.335	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.600%
20) 2-Butanone-d5	3.921	46	84249	50.620	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.240%
24) Chloroform-d	4.352	84	104509	4.576	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
26) 1,2-Dichloroethane-d4	5.037	65	44103	4.618	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.400%
32) Benzene-d6	5.050	84	217966	4.522	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%
36) 1,2-Dichloropropane-d6	6.069	67	65209	4.704	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.000%
41) Toluene-d8	7.317	98	192868	4.390	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.800%
43) trans-1,3-Dichloroprop...	7.625	79	21538	4.457	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.200%
46) 2-Hexanone-d5	8.092	63	81225	49.281	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.560%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	39576	4.853	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	61572	4.693	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.800%
Target Compounds						Qvalue
14) Carbon disulfide	2.294	76	7467	0.188	ug/L	100
15) Methyl Acetate	2.449	43	20966	6.875	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025003.D
Acq On : 15 Mar 2022 17:46
Operator : SY/MD
Sample : N1934-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD5

Quant Time: Mar 16 03:39:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 16 03:30:21 2022
Response via : Initial Calibration




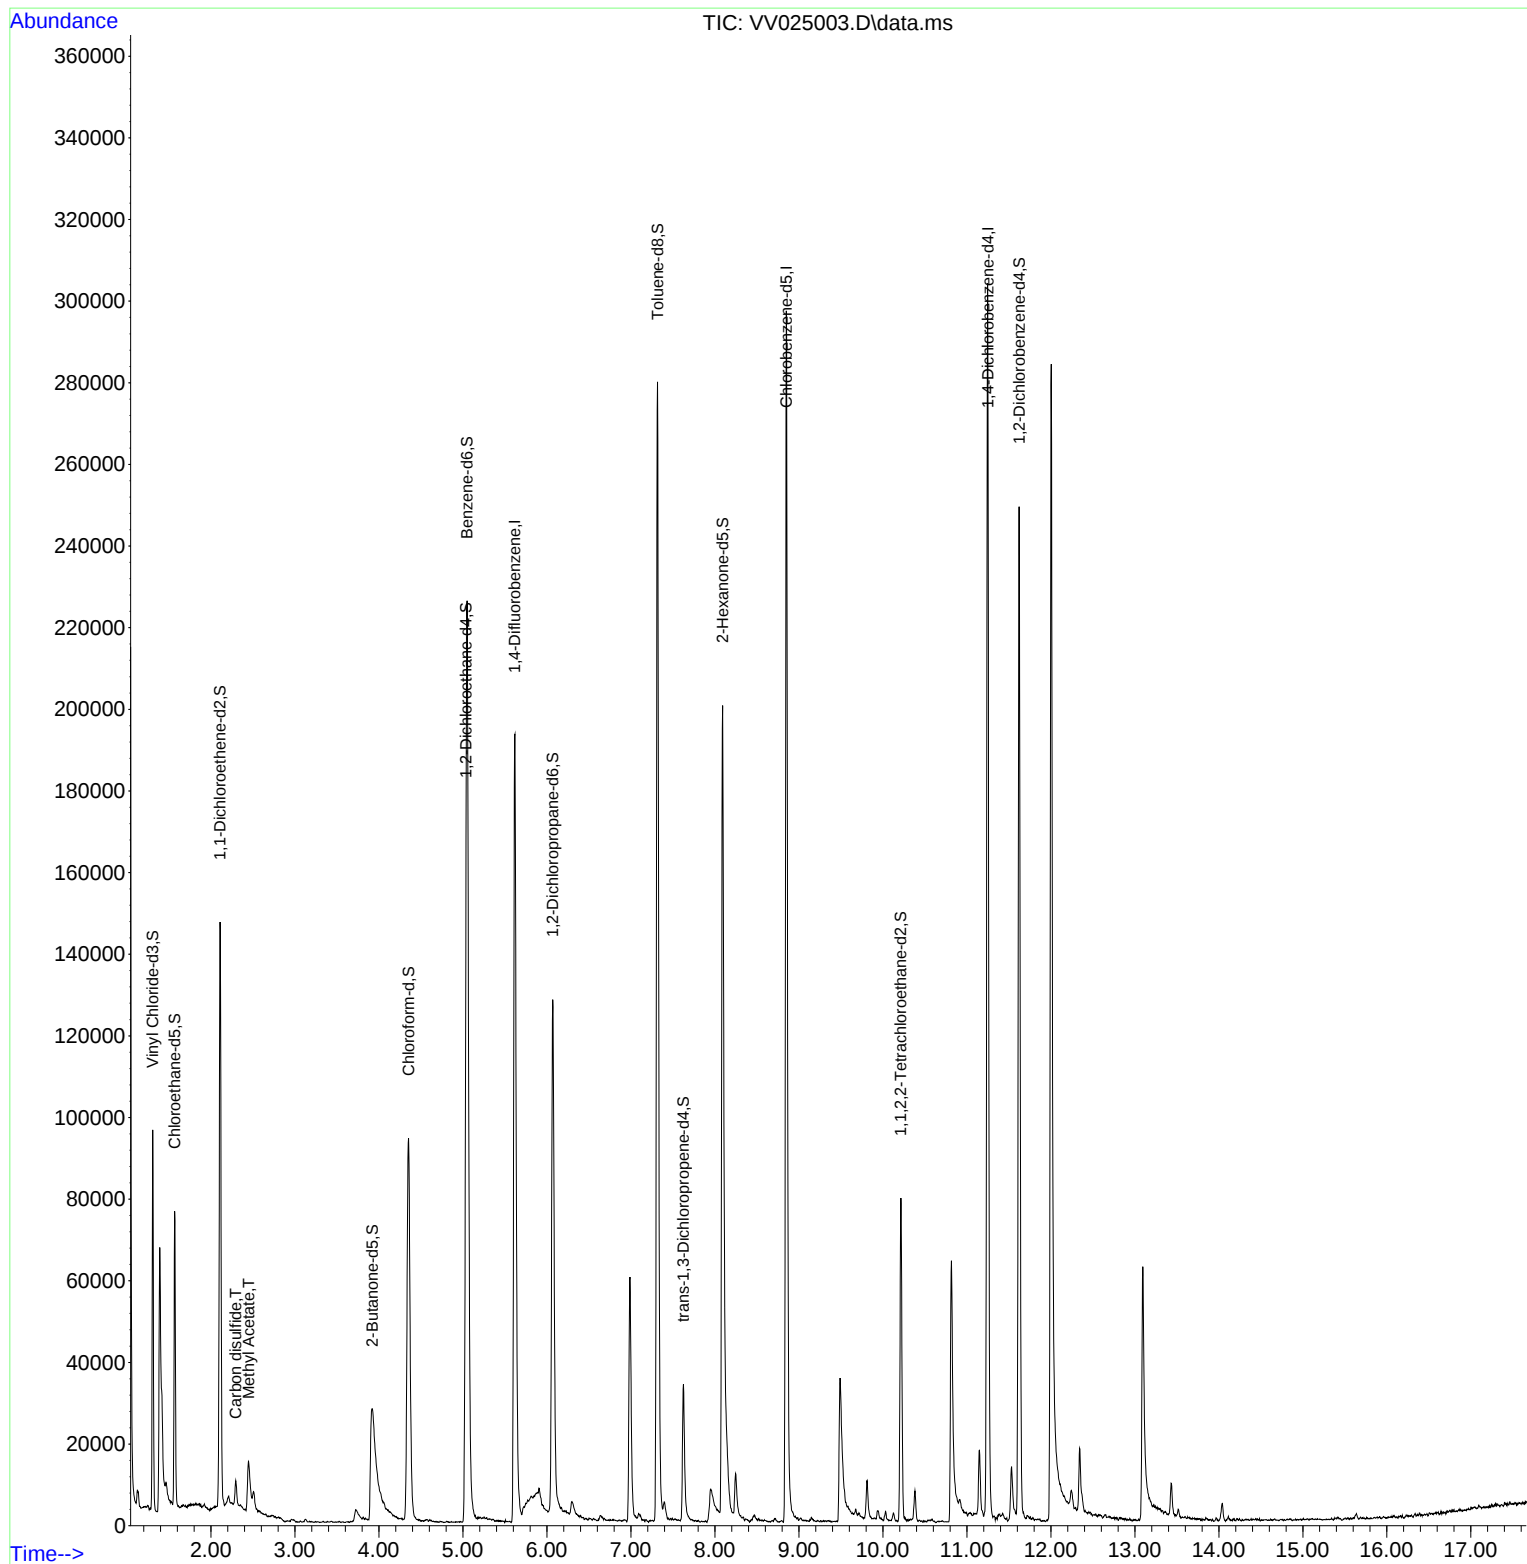


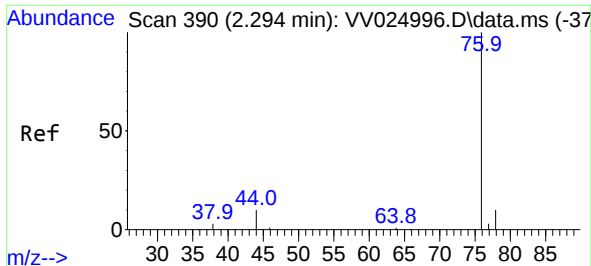

#14
Carbon disulfide
Concen: 0.188 ug/L
RT: 2.294 min Scan# 390
Delta R.T. 0.000 min
Lab File: VV025003.D
Acq: 15 Mar 2022 17:46

Instrument :
MSVOA_V
ClientSampleId :
GBDD5

Tgt Ion: 76 Resp: 7467
Ion Ratio Lower Upper
76 100
78 9.2 7.4 11.0

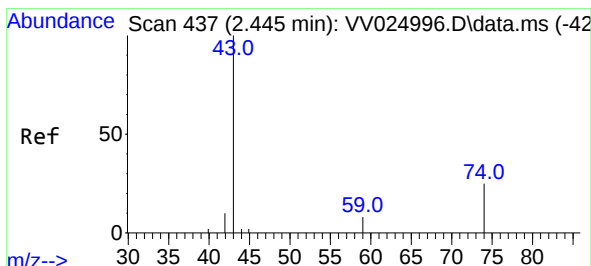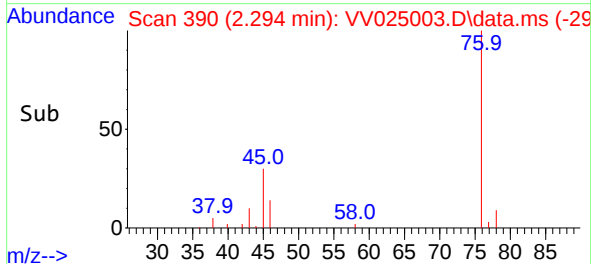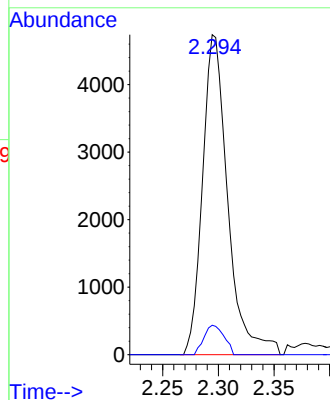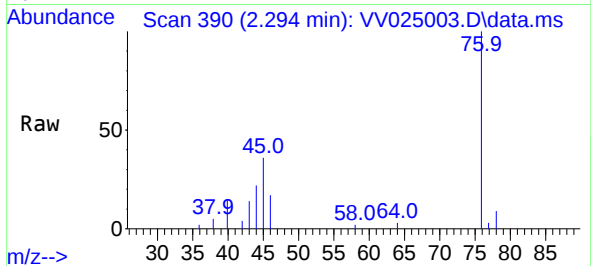

#15
Methyl Acetate
Concen: 6.875 ug/L
RT: 2.449 min Scan# 438
Delta R.T. 0.003 min
Lab File: VV025003.D
Acq: 15 Mar 2022 17:46

Tgt Ion: 43 Resp: 20966
Ion Ratio Lower Upper
43 100
74 26.1 24.2 36.4

