

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031522\
 Data File : VW025008.D
 Acq On : 15 Mar 2022 19:43
 Operator : SY/MD
 Sample : N1934-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDE0

Quant Time: Mar 16 03:41:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 16 03:30:21 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	159582	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	150740	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	65944	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	56121	4.454	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	89.000%	
7) Chloroethane-d5	1.571	69	44249	4.796	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.000%	
11) 1,1-Dichloroethene-d2	2.111	63	69525	3.414	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.200%	
20) 2-Butanone-d5	3.899	46	81927	53.807	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	107.620%	
24) Chloroform-d	4.352	84	99986	4.785	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.800%	
26) 1,2-Dichloroethane-d4	5.034	65	43089	4.932	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.600%	
32) Benzene-d6	5.050	84	201635	4.611	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.200%	
36) 1,2-Dichloropropane-d6	6.072	67	60609	4.820	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.400%	
41) Toluene-d8	7.317	98	173066	4.343	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.800%	
43) trans-1,3-Dichloroprop...	7.625	79	19569	4.464	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.200%	
46) 2-Hexanone-d5	8.088	63	67462	45.119	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.240%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34794	4.704	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	56068	5.022	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.400%	
Target Compounds						
25) Chloroform	4.378	83	35538	1.639	ug/L	93
38) Bromodichloromethane	6.516	83	1974	0.139	ug/L #	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025008.D
Acq On : 15 Mar 2022 19:43
Operator : SY/MD
Sample : N1934-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDE0

Quant Time: Mar 16 03:41:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 16 03:30:21 2022
Response via : Initial Calibration

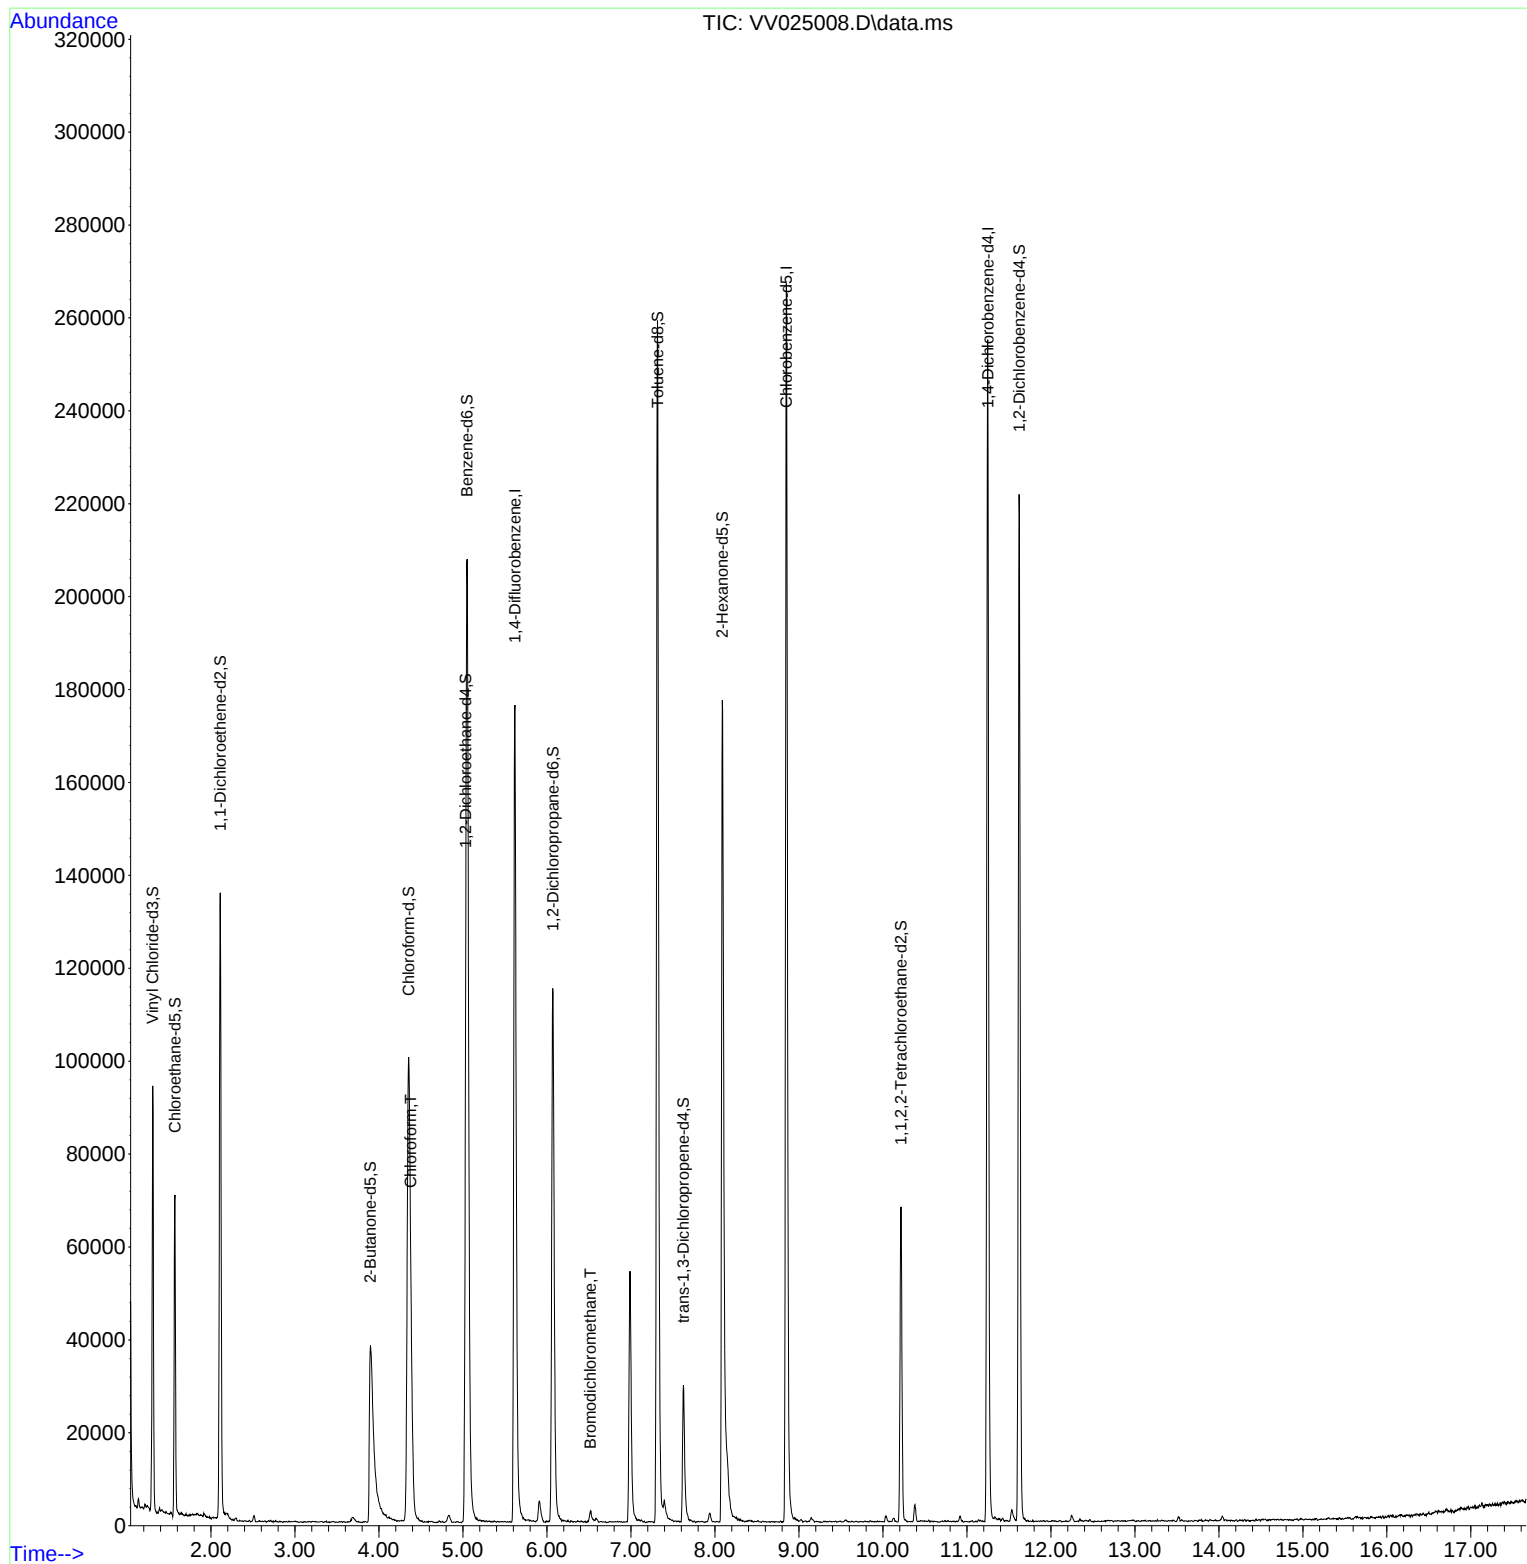

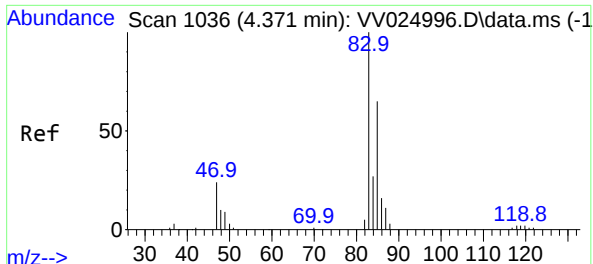

#25

Chloroform

Concen: 1.639 ug/L

RT: 4.378 min Scan# 1036

Delta R.T. 0.007 min

Lab File: VV025008.D

Acq: 15 Mar 2022 19:43

Instrument :

MSVOA_V

ClientSampleId :





GBDE0

Tgt Ion: 83 Resp: 35538

Ion Ratio Lower Upper

83 100

85 69.0 44.5 82.7

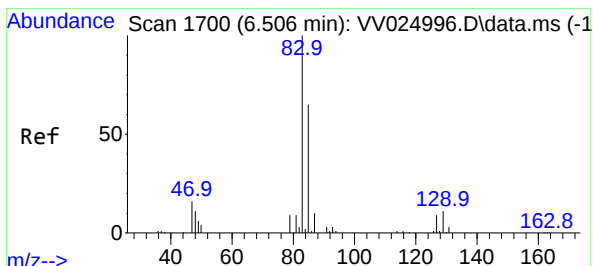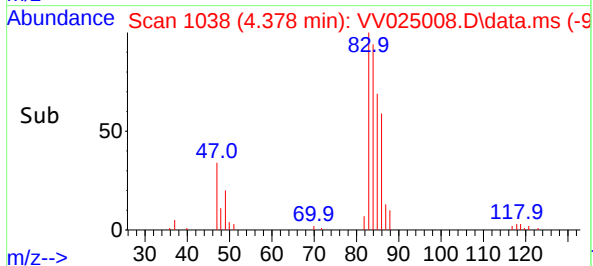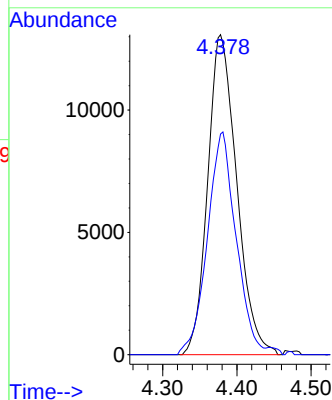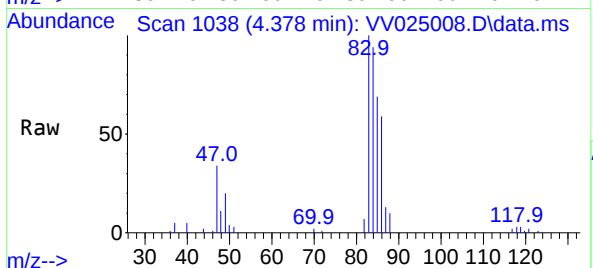

#38

Bromodichloromethane

Concen: 0.139 ug/L

RT: 6.516 min Scan# 1703

Delta R.T. 0.010 min

Lab File: VV025008.D

Acq: 15 Mar 2022 19:43

Tgt Ion: 83 Resp: 1974

Ion Ratio Lower Upper

83 100

85 67.9 44.8 83.2

127 0.0 6.3 9.5

