

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025021.D
 Acq On : 16 Mar 2022 01:11
 Operator : SY/MD
 Sample : N1933-13
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDC4

Quant Time: Mar 16 06:48:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 16 05:10:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	156814	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	149777	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	66272	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	57642	4.656	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.200%
7) Chloroethane-d5	1.568	69	44930	4.956	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.200%
11) 1,1-Dichloroethene-d2	2.108	63	72971	3.647	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.000%
20) 2-Butanone-d5	3.902	46	101278	67.690	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	135.380%#
24) Chloroform-d	4.352	84	100762	4.907	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	5.034	65	45334	5.281	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.600%
32) Benzene-d6	5.053	84	209609	4.824	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%
36) 1,2-Dichloropropane-d6	6.072	67	63440	5.078	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.600%
41) Toluene-d8	7.317	98	181265	4.578	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.600%
43) trans-1,3-Dichloroprop...	7.625	79	21510	4.939	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.800%
46) 2-Hexanone-d5	8.088	63	82591	55.593	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.180%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40376	5.493	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	59167	5.274	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.400%
Target Compounds						Qvalue
13) Acetone	2.191	43	8330	8.325	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025021.D
Acq On : 16 Mar 2022 01:11
Operator : SY/MD
Sample : N1933-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC4

Quant Time: Mar 16 06:48:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 16 05:10:39 2022
Response via : Initial Calibration

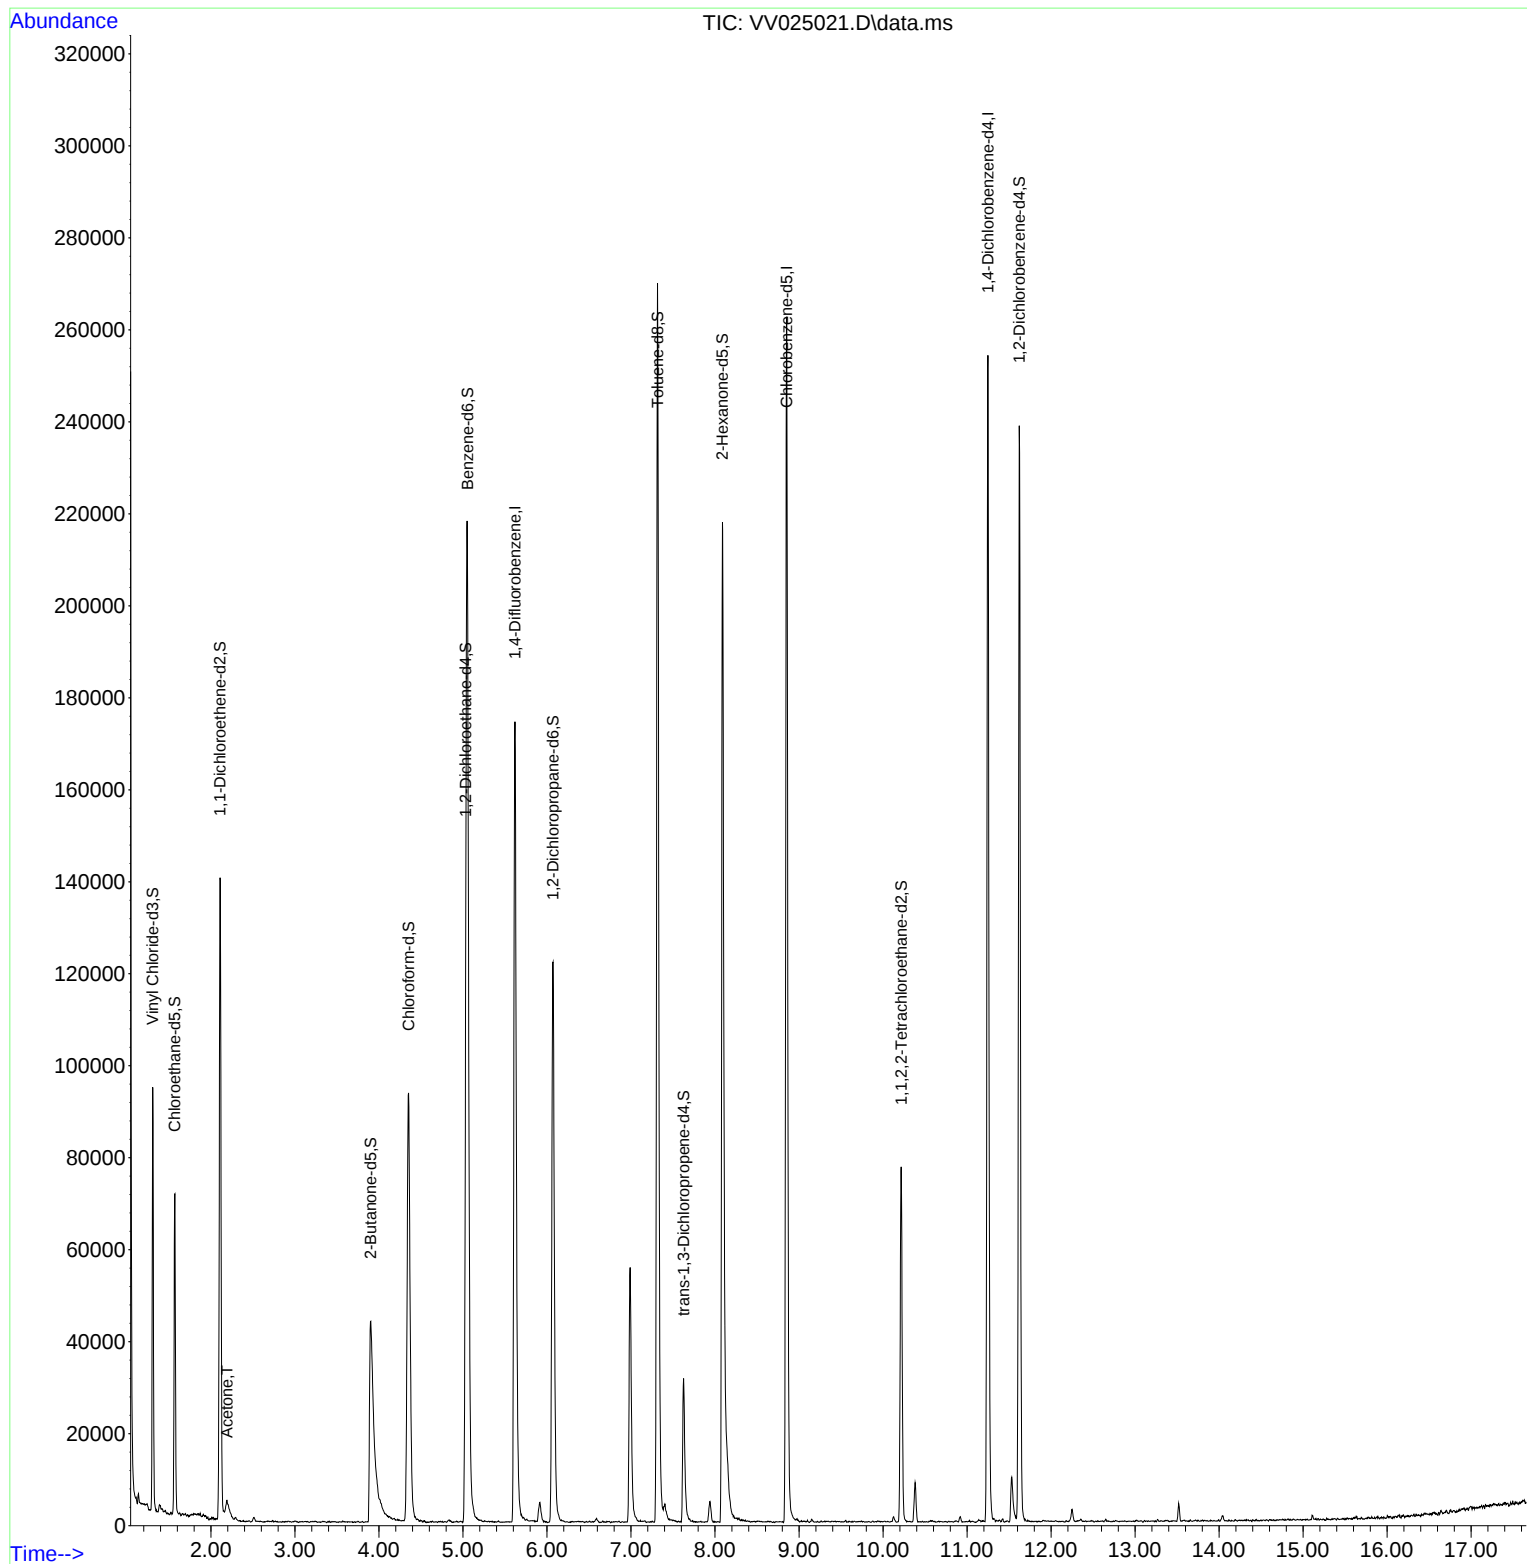

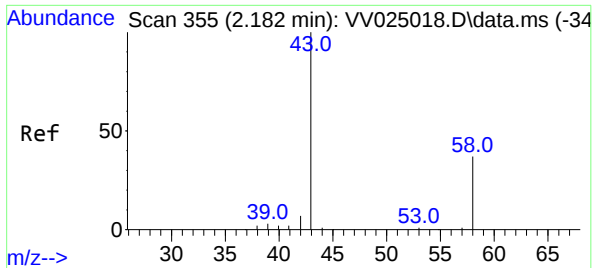

#13
Acetone
Concen: 8.325 ug/L
RT: 2.191 min Scan# 31
Delta R.T. 0.010 min
Lab File: VV025021.D
Acq: 16 Mar 2022 01:11

Instrument :
MSVOA_V
ClientSampleId :
GBDC4

Tgt Ion: 43 Resp: 8330
Ion Ratio Lower Upper
43 100
58 35.7 0.0 54.2

