

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV024997.D
 Acq On : 15 Mar 2022 14:54
 Operator : SY/MD
 Sample : VV0315WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK314

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	109592	108853	18.56%	2.415%
2	1.568	157	164	176	rVB	78986	87543	14.93%	1.942%
3	2.108	321	332	345	rBV	159331	227826	38.85%	5.054%
4	2.507	444	456	471	rVB2	9554	15882	2.71%	0.352%
5	3.899	880	889	924	rBV	27085	97041	16.55%	2.153%
6	4.346	1012	1028	1056	rVB	97289	244829	41.75%	5.431%
7	5.043	1229	1245	1276	rBV2	236127	586477	100.00%	13.011%
8	5.613	1410	1422	1446	rBV	192034	391949	66.83%	8.695%
9	5.905	1504	1513	1525	rBV5	4194	8792	1.50%	0.195%
10	6.066	1549	1563	1592	rBV	128318	264722	45.14%	5.873%
11	6.985	1839	1849	1867	rBV	60949	112890	19.25%	2.504%
12	7.313	1939	1951	1971	rBV	300837	522032	89.01%	11.581%
13	7.391	1971	1975	1993	rVB4	4923	9963	1.70%	0.221%
14	7.622	2037	2047	2069	rBV	33300	60661	10.34%	1.346%
15	8.088	2182	2192	2235	rBV	166433	393166	67.04%	8.722%
16	8.850	2418	2429	2460	rBV	276958	461902	78.76%	10.247%
17	10.214	2842	2853	2874	rBV	73647	118075	20.13%	2.619%
18	11.246	3163	3174	3194	rBV	261862	410093	69.92%	9.098%
19	11.622	3280	3291	3310	rBV	236318	376529	64.20%	8.353%
20	13.506	3865	3877	3891	rBV2	4818	8393	1.43%	0.186%




Sum of corrected areas: 4507618

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV024997.D
Acq On : 15 Mar 2022 14:54
Operator : SY/MD
Sample : VV0315WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK314

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

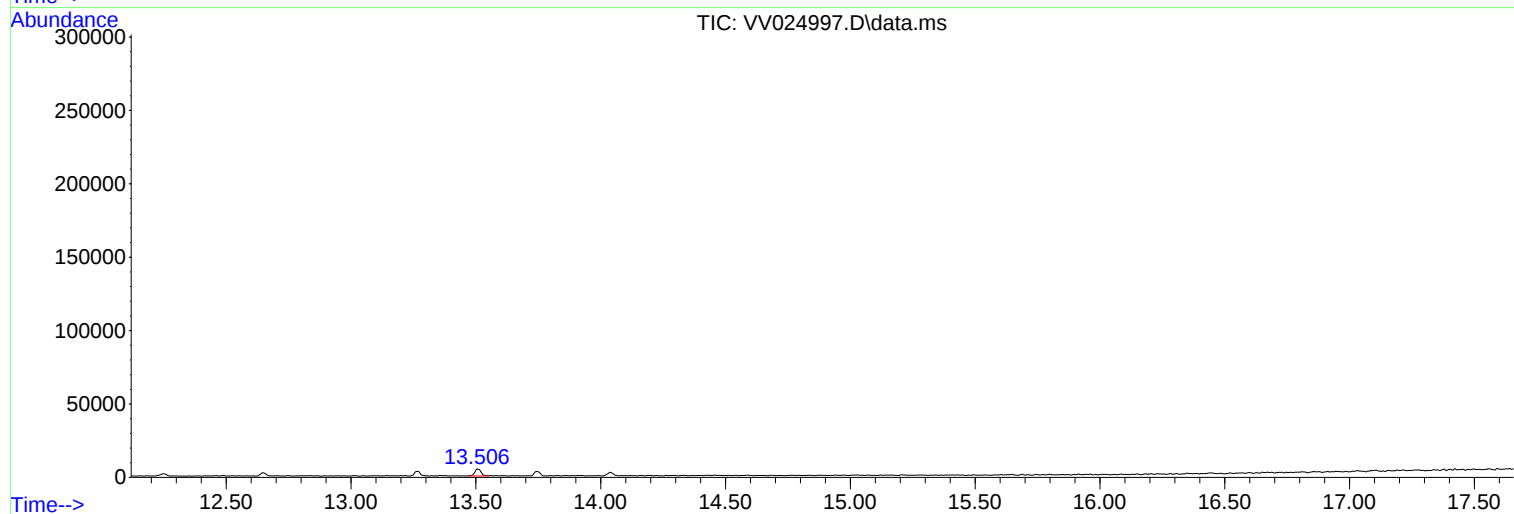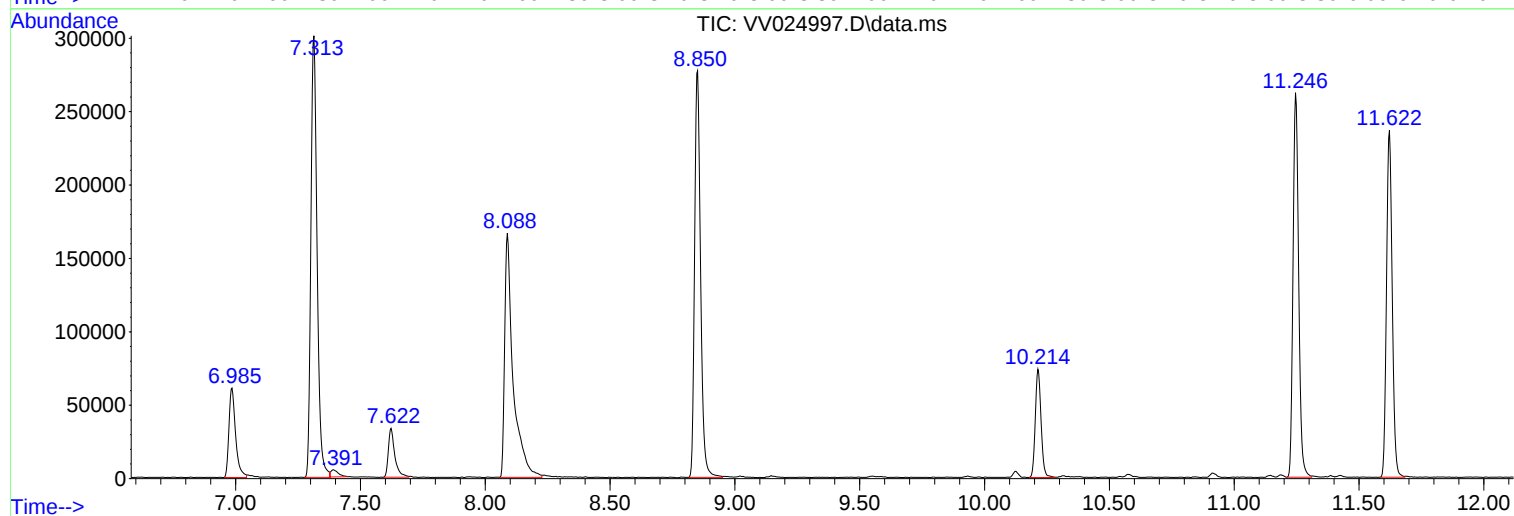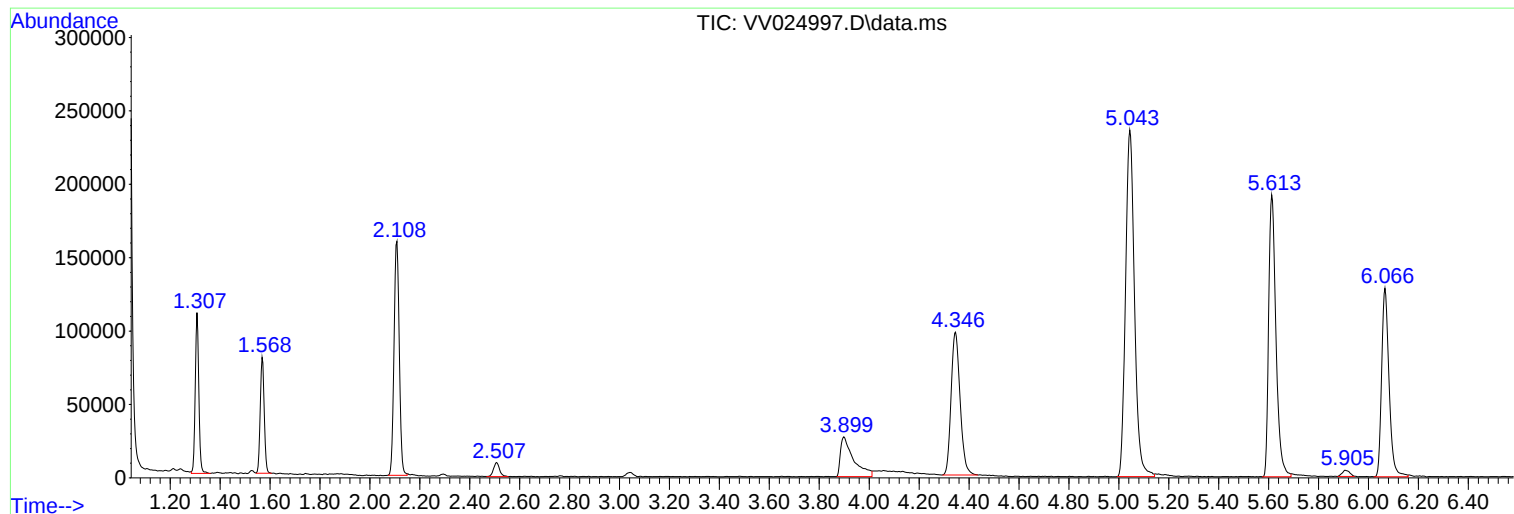

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV024997.D
Acq On : 15 Mar 2022 14:54
Operator : SY/MD
Sample : VV0315WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK314

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV024997.D
Acq On : 15 Mar 2022 14:54
Operator : SY/MD
Sample : VV0315WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK314

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc