

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV024998.D
 Acq On : 15 Mar 2022 15:49
 Operator : SY/MD
 Sample : N1933-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDB5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	99	rVB	96081	98122	17.82%	1.910%
2	1.571	157	165	175	rBV	74247	83847	15.23%	1.633%
3	2.111	322	333	348	rBV	148321	212754	38.64%	4.142%
4	2.510	447	457	475	rBV	20866	35275	6.41%	0.687%
5	3.905	878	891	930	rBV	36749	145634	26.45%	2.836%
6	4.352	1013	1030	1063	rBV	96597	265691	48.25%	5.173%
7	4.828	1161	1178	1202	rBV	181625	435763	79.14%	8.485%
8	5.050	1229	1247	1278	rBV2	221875	550650	100.00%	10.721%
9	5.619	1411	1424	1452	rBV	225753	464503	84.36%	9.044%
10	5.915	1506	1516	1534	rVB7	5378	12468	2.26%	0.243%
11	6.069	1550	1564	1598	rBV	121457	251285	45.63%	4.893%
12	6.989	1836	1850	1877	rBV	57145	109383	19.86%	2.130%
13	7.316	1941	1952	1973	rBV	276447	484138	87.92%	9.426%
14	7.625	2038	2048	2072	rBV	31325	57335	10.41%	1.116%
15	8.091	2183	2193	2236	rBV	186821	389513	70.74%	7.584%
16	8.850	2418	2429	2459	rBV	335014	549260	99.75%	10.694%
17	10.217	2842	2854	2866	rBV	72924	113548	20.62%	2.211%
18	11.246	3163	3174	3198	rBV	320749	494545	89.81%	9.629%
19	11.532	3254	3263	3278	rBV2	7896	14494	2.63%	0.282%
20	11.622	3280	3291	3310	rVB	236845	367769	66.79%	7.161%




Sum of corrected areas: 5135977

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV024998.D
Acq On : 15 Mar 2022 15:49
Operator : SY/MD
Sample : N1933-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

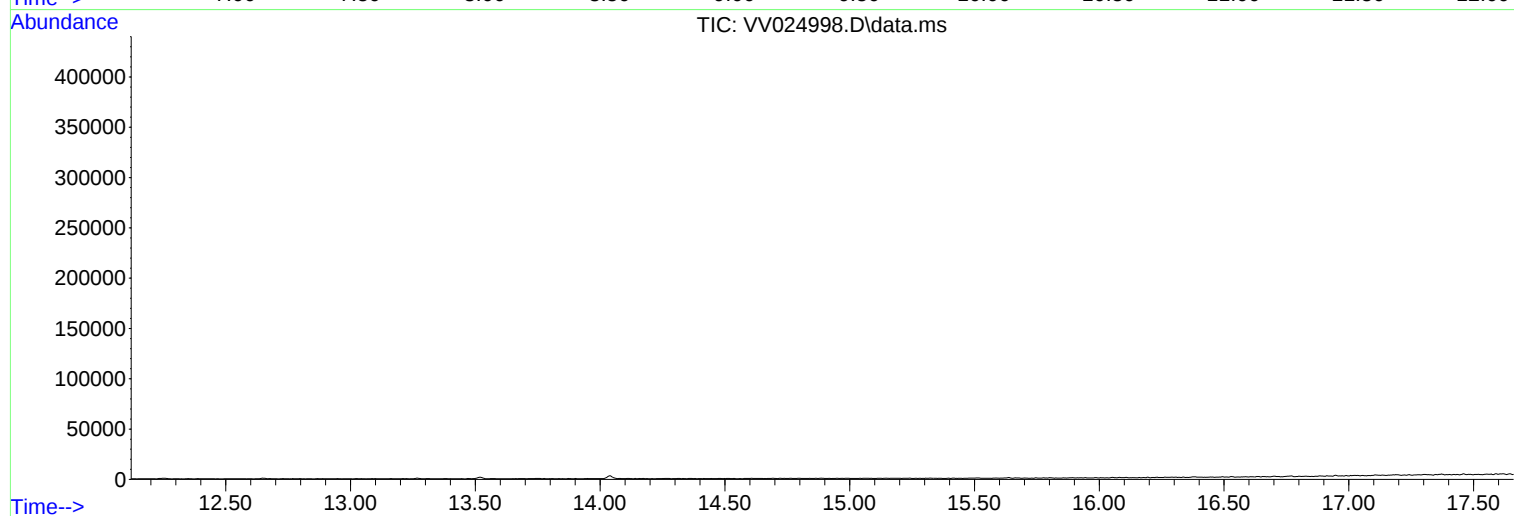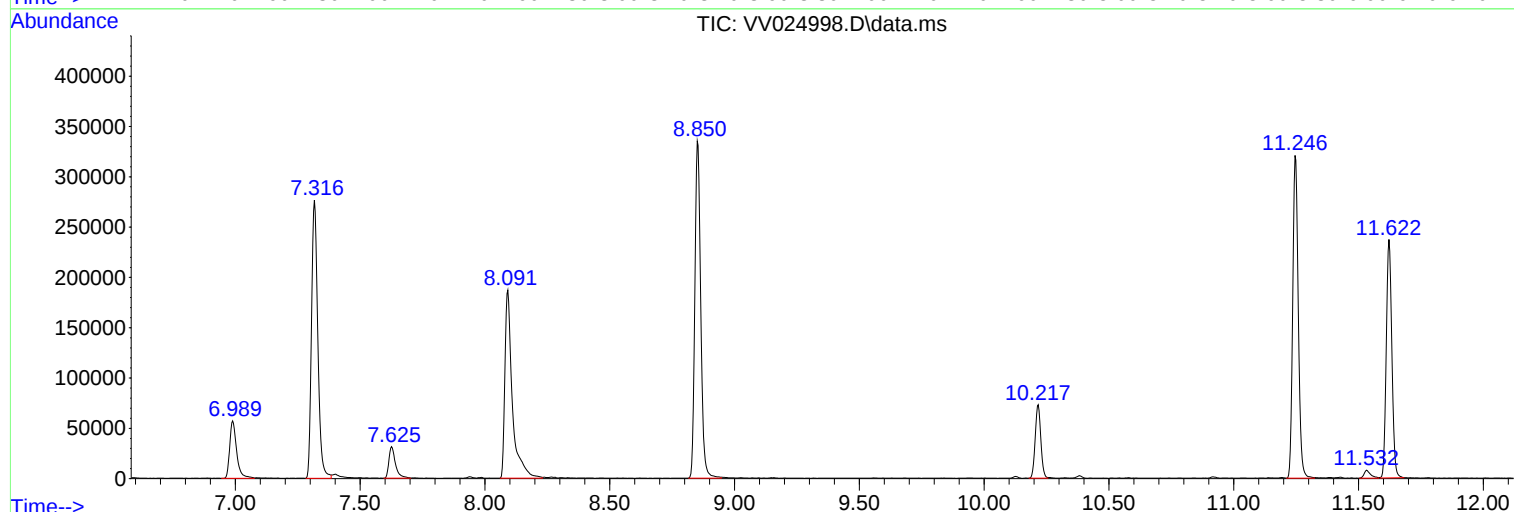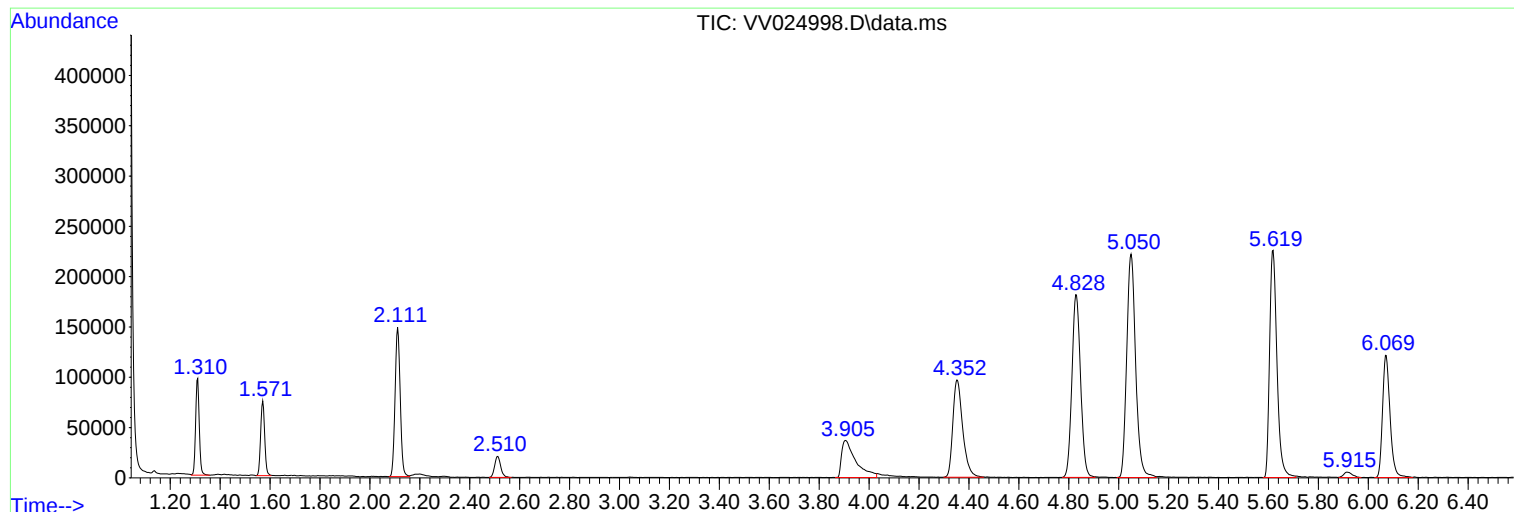

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV024998.D
Acq On : 15 Mar 2022 15:49
Operator : SY/MD
Sample : N1933-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV024998.D
Acq On : 15 Mar 2022 15:49
Operator : SY/MD
Sample : N1933-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc