

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025004.D
 Acq On : 15 Mar 2022 18:09
 Operator : SY/MD
 Sample : N1934-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDD6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025004.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	93860	94720	2.74%	1.150%
2	1.571	156	165	179	rBV	73744	83664	2.42%	1.016%
3	2.111	320	333	346	rBV	144734	210046	6.07%	2.551%
4	2.185	346	356	381	rVB	19348	49667	1.44%	0.603%
5	3.896	877	888	936	rBV2	47271	170858	4.94%	2.075%
6	4.349	1014	1029	1070	rBV2	125133	346274	10.01%	4.206%
7	4.828	1156	1178	1207	rBV	1466308	3458644	100.00%	42.009%
8	5.050	1230	1247	1278	rBV2	220830	545312	15.77%	6.623%
9	5.616	1412	1423	1450	rBV	214631	433954	12.55%	5.271%
10	6.069	1551	1564	1591	rVB	122364	251298	7.27%	3.052%
11	6.989	1838	1850	1867	rBV	59644	110176	3.19%	1.338%
12	7.317	1940	1952	1972	rBV	273568	473961	13.70%	5.757%
13	7.625	2036	2048	2066	rBV	33251	59413	1.72%	0.722%
14	8.088	2182	2192	2233	rBV	206529	396875	11.47%	4.820%
15	8.850	2418	2429	2453	rBV	314347	515572	14.91%	6.262%
16	10.214	2842	2853	2868	rBV	77166	121309	3.51%	1.473%
17	11.246	3163	3174	3194	rBV	300494	462836	13.38%	5.622%
18	11.529	3250	3262	3280	rBV2	18678	37704	1.09%	0.458%
19	11.622	3280	3291	3316	rVB	241250	372596	10.77%	4.526%
20	12.008	3400	3411	3429	rBV3	18955	38204	1.10%	0.464%




Sum of corrected areas: 8233083

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025004.D
Acq On : 15 Mar 2022 18:09
Operator : SY/MD
Sample : N1934-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

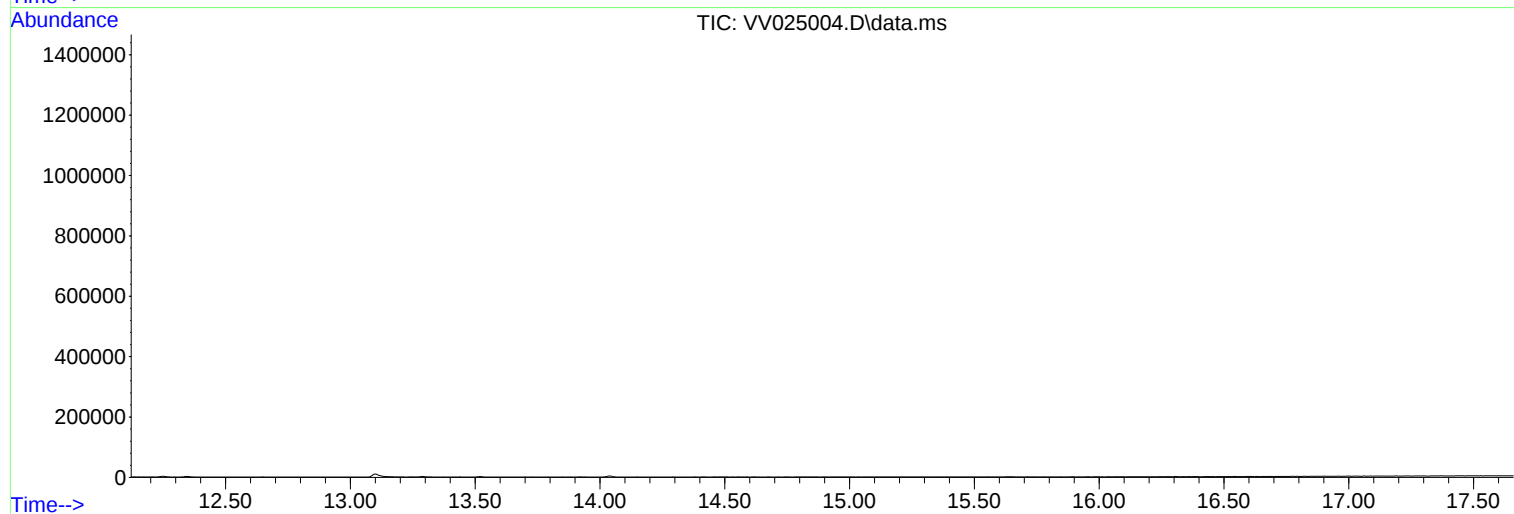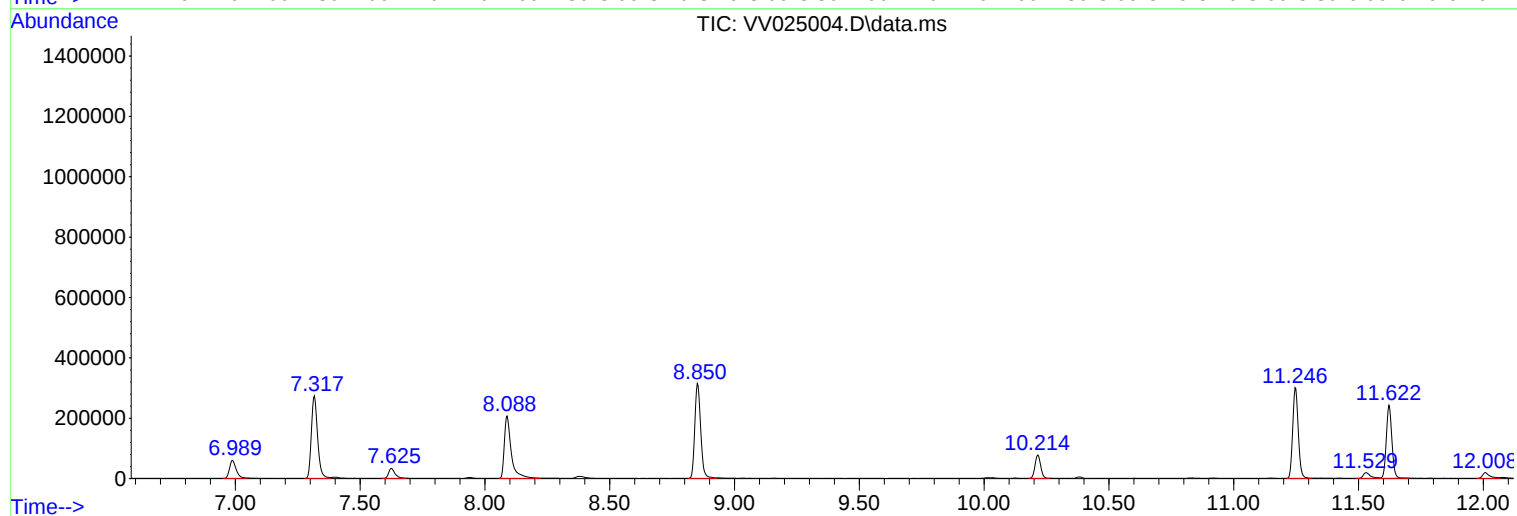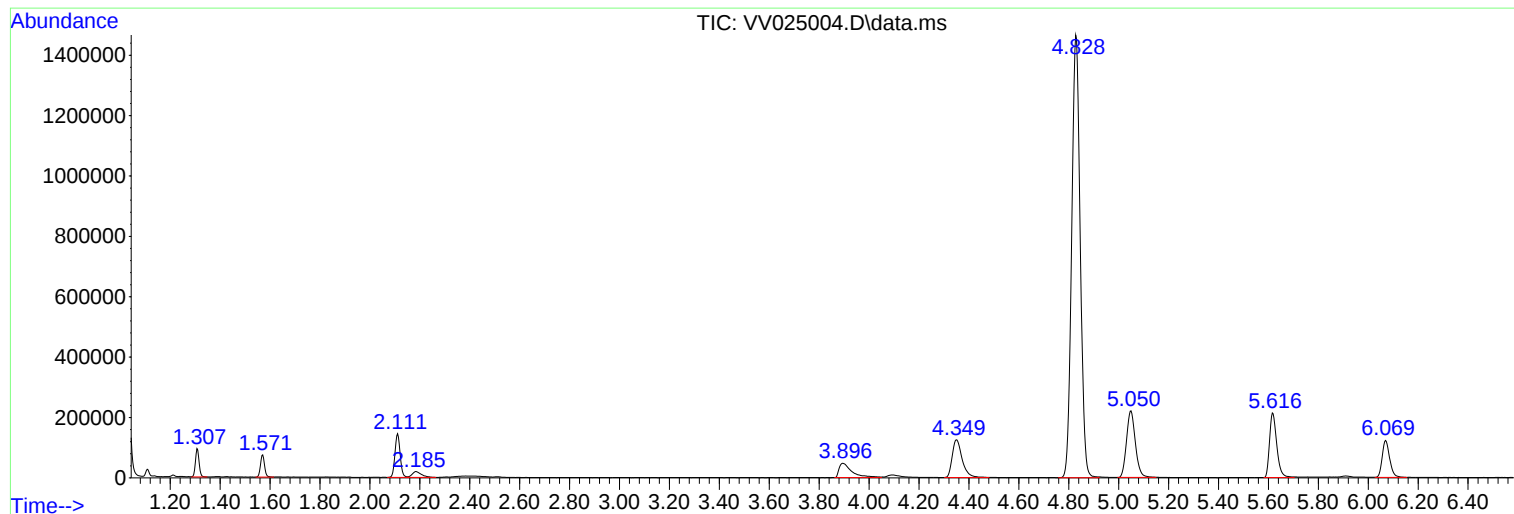

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025004.D
Acq On : 15 Mar 2022 18:09
Operator : SY/MD
Sample : N1934-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025004.D
Acq On : 15 Mar 2022 18:09
Operator : SY/MD
Sample : N1934-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc