

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025009.D
 Acq On : 15 Mar 2022 20:06
 Operator : SY/MD
 Sample : N1934-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDE1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	95	rVB	92049	89735	17.31%	2.155%
2	1.571	156	165	179	rBV	67139	77605	14.97%	1.864%
3	2.111	321	333	350	rBV	137375	197771	38.15%	4.749%
4	3.896	877	888	933	rBV2	46343	157361	30.35%	3.779%
5	4.352	1014	1030	1064	rBV2	90711	225716	43.54%	5.420%
6	5.050	1231	1247	1275	rBV2	210055	518447	100.00%	12.450%
7	5.619	1411	1424	1456	rBV	178239	363395	70.09%	8.726%
8	5.912	1505	1515	1531	rVB6	4986	11011	2.12%	0.264%
9	6.069	1551	1564	1593	rBV	117053	239494	46.19%	5.751%
10	6.989	1840	1850	1870	rBV	54311	100061	19.30%	2.403%
11	7.317	1938	1952	1970	rBV	255855	447955	86.40%	10.757%
12	7.625	2037	2048	2068	rBV	28983	52700	10.16%	1.266%
13	8.088	2183	2192	2227	rBV	185305	363632	70.14%	8.732%
14	8.850	2419	2429	2459	rBV	269603	444878	85.81%	10.683%
15	10.217	2842	2854	2870	rBV	68408	107309	20.70%	2.577%
16	10.381	2896	2905	2915	rVB3	4497	6708	1.29%	0.161%
17	11.249	3163	3175	3195	rBV	255808	396497	76.48%	9.521%
18	11.622	3278	3291	3314	rBV	220212	346966	66.92%	8.332%
19	12.345	3509	3516	3527	rVB4	6016	8174	1.58%	0.196%
20	13.435	3848	3855	3864	rBV4	6530	8914	1.72%	0.214%




Sum of corrected areas: 4164329

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025009.D
Acq On : 15 Mar 2022 20:06
Operator : SY/MD
Sample : N1934-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

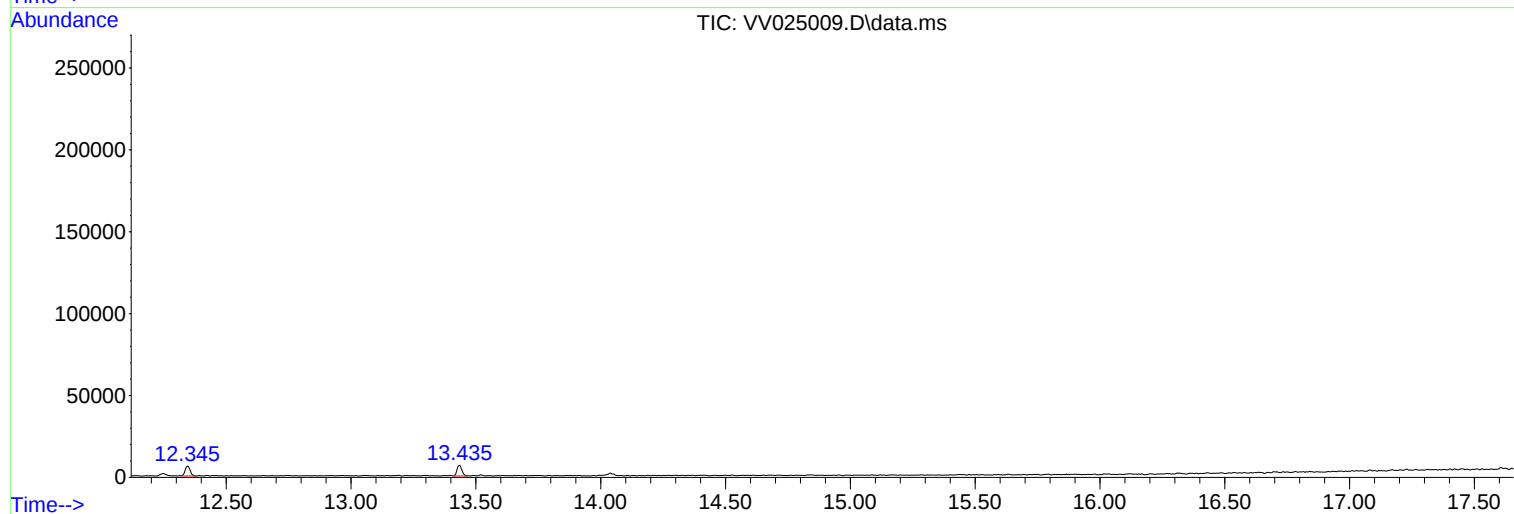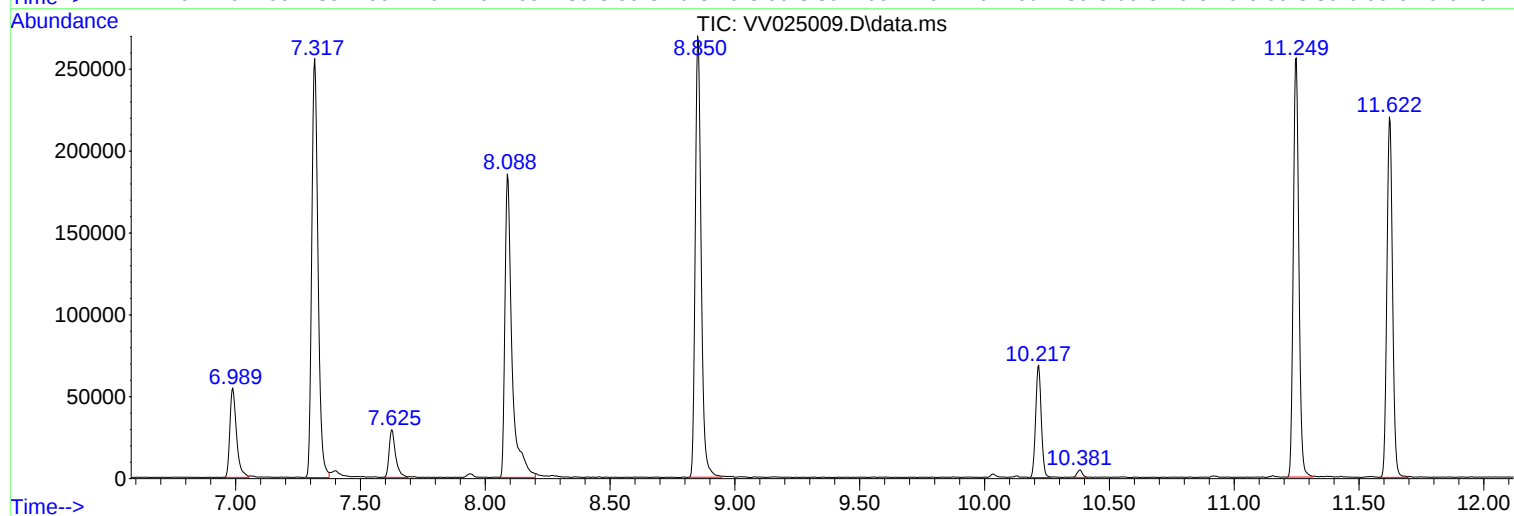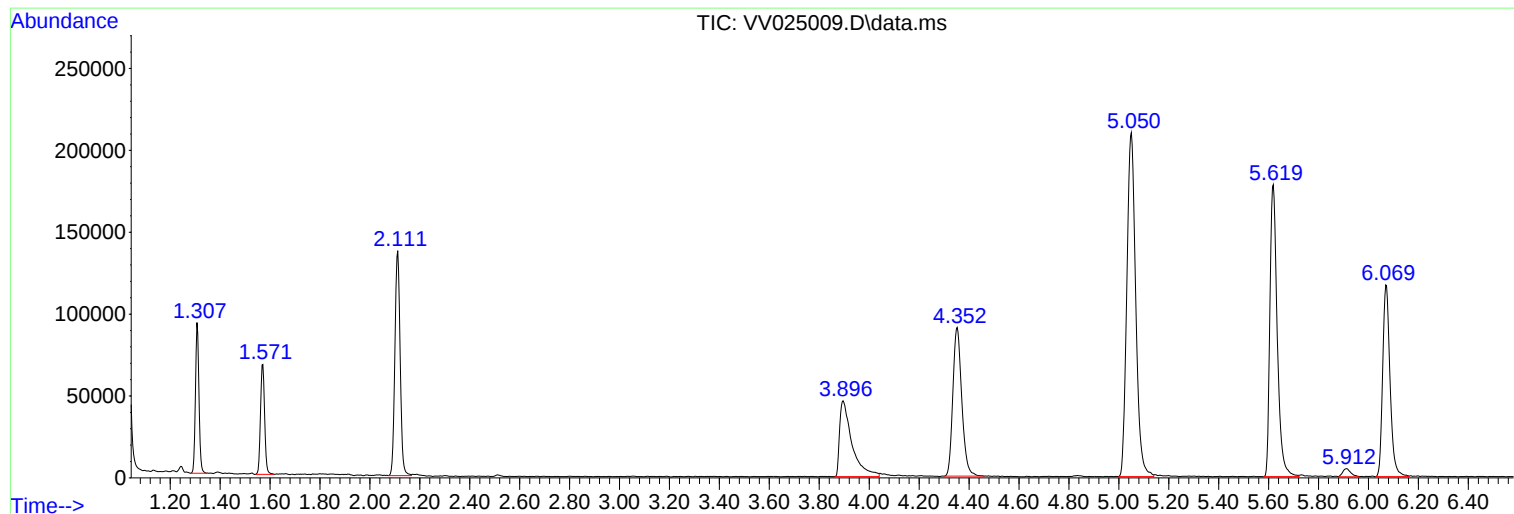

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025009.D
Acq On : 15 Mar 2022 20:06
Operator : SY/MD
Sample : N1934-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025009.D
Acq On : 15 Mar 2022 20:06
Operator : SY/MD
Sample : N1934-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
