

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025010.D
 Acq On : 15 Mar 2022 20:30
 Operator : SY/MD
 Sample : N1933-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDB7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025010.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	95	rVB	97345	99459	17.65%	2.061%
2	1.571	157	165	179	rBV	77678	85791	15.22%	1.778%
3	2.111	320	333	346	rBV	153167	219462	38.94%	4.547%
4	2.182	346	355	373	rVB2	4685	11345	2.01%	0.235%
5	3.892	878	887	927	rBV2	45996	150679	26.73%	3.122%
6	4.352	1014	1030	1059	rBV2	95478	242781	43.08%	5.030%
7	4.831	1157	1179	1208	rBV	179679	431228	76.51%	8.935%
8	5.050	1231	1247	1284	rBV2	228721	563604	100.00%	11.678%
9	5.619	1412	1424	1450	rBV	180147	362876	64.38%	7.519%
10	5.908	1505	1514	1529	rVB4	4110	8156	1.45%	0.169%
11	6.069	1550	1564	1592	rBV	125094	257267	45.65%	5.330%
12	6.989	1839	1850	1876	rBV	59099	108805	19.31%	2.254%
13	7.317	1938	1952	1971	rBV	283578	491793	87.26%	10.190%
14	7.625	2038	2048	2073	rBV	31768	57686	10.24%	1.195%
15	8.088	2182	2192	2236	rBV	194015	385390	68.38%	7.985%
16	8.850	2418	2429	2452	rBV	265651	437325	77.59%	9.061%
17	10.217	2842	2854	2866	rBV	73793	116669	20.70%	2.417%
18	10.381	2897	2905	2918	rVB3	4489	6973	1.24%	0.144%
19	11.246	3164	3174	3195	rBV	259722	401806	71.29%	8.325%
20	11.532	3254	3263	3272	rBV3	7006	12443	2.21%	0.258%
21	11.622	3280	3291	3310	rVB	241578	374804	66.50%	7.766%




Sum of corrected areas: 4826342

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025010.D
Acq On : 15 Mar 2022 20:30
Operator : SY/MD
Sample : N1933-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

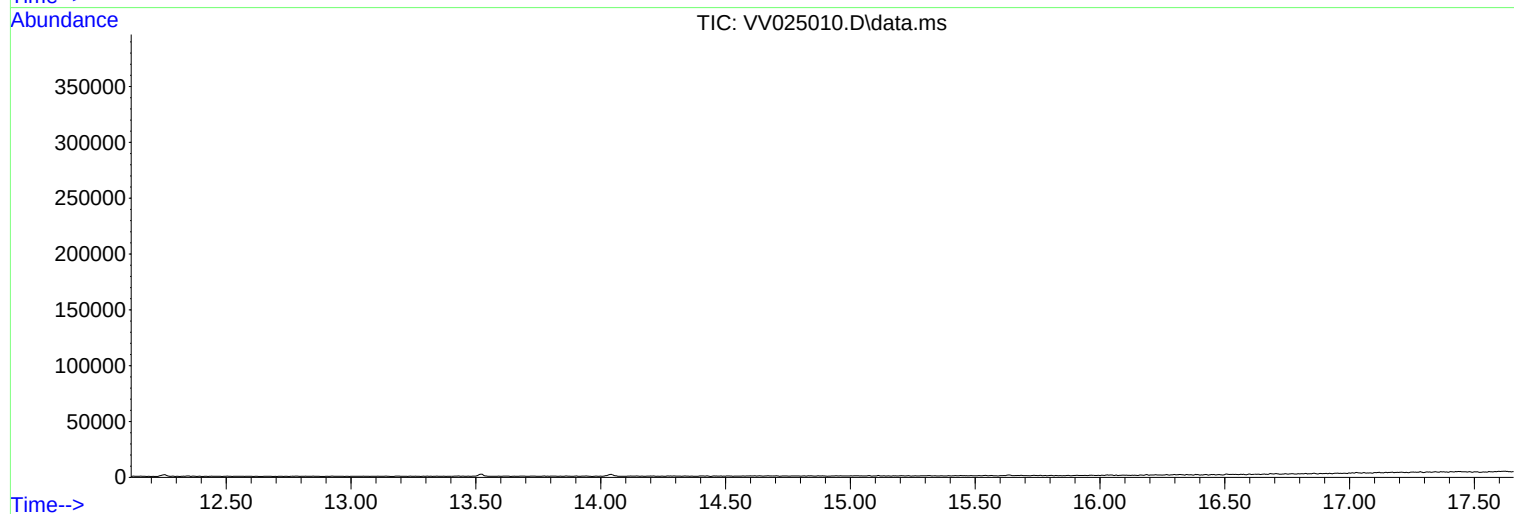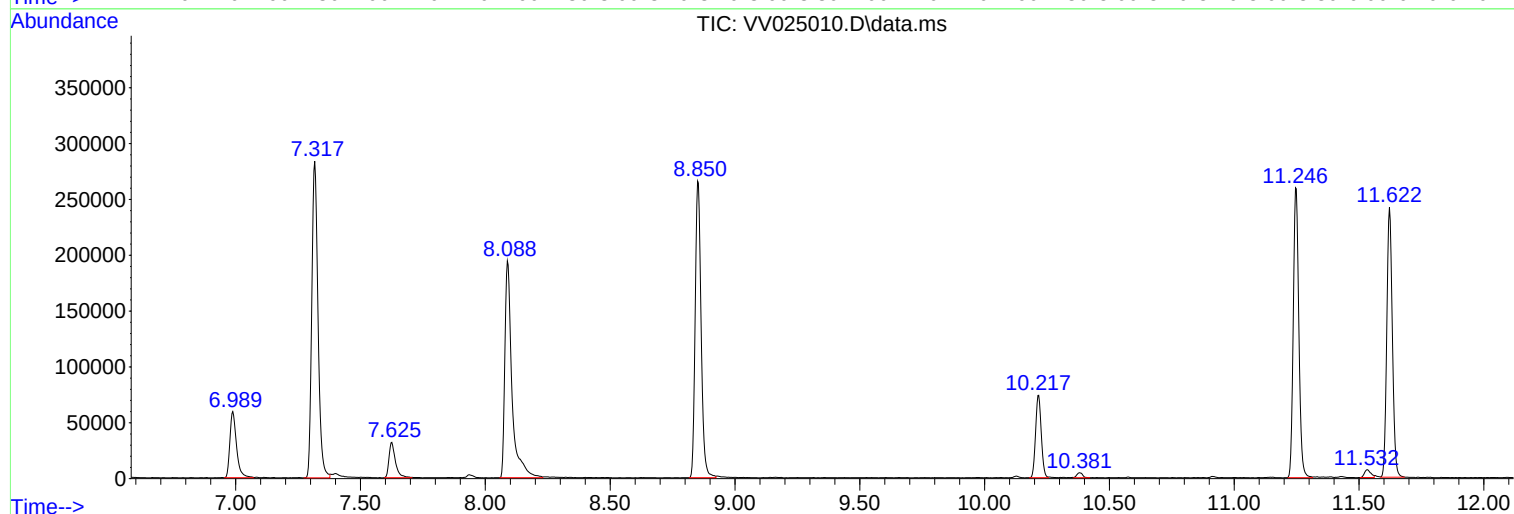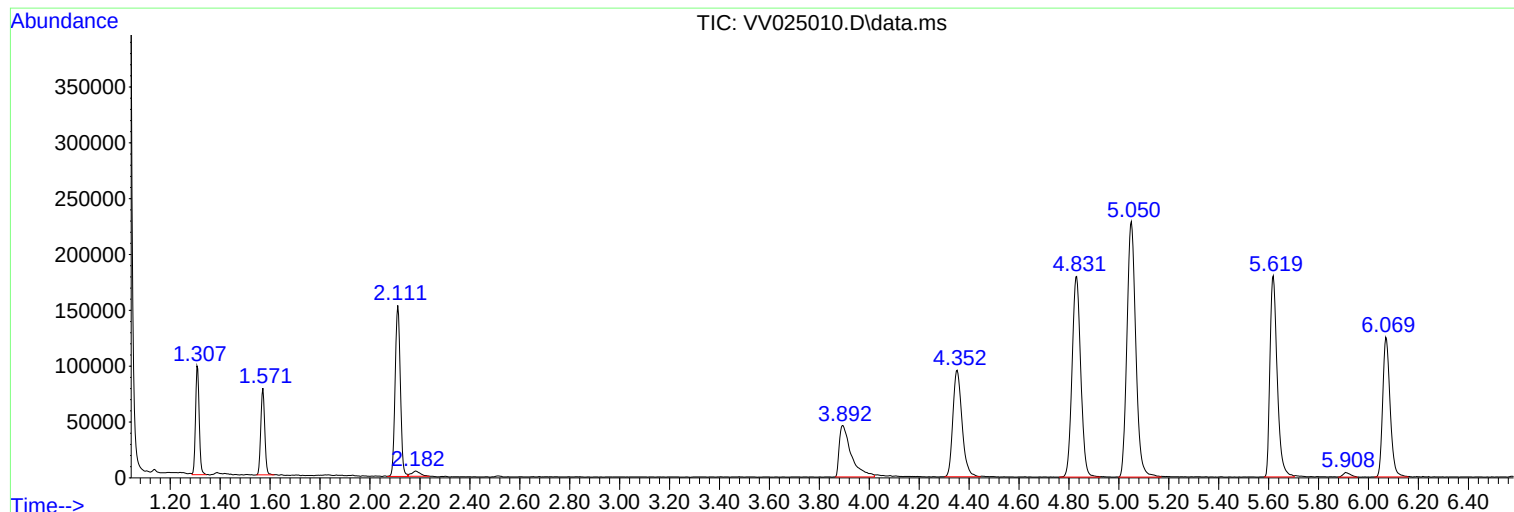

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025010.D
Acq On : 15 Mar 2022 20:30
Operator : SY/MD
Sample : N1933-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025010.D
Acq On : 15 Mar 2022 20:30
Operator : SY/MD
Sample : N1933-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
