

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025014.D
 Acq On : 15 Mar 2022 22:03
 Operator : SY/MD
 Sample : N1933-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDC1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	96570	93573	17.22%	1.967%
2	1.571	156	165	174	rBV	70201	78868	14.51%	1.658%
3	2.111	318	333	347	rBV	143891	206879	38.06%	4.348%
4	3.892	877	887	919	rBV	45921	142776	26.27%	3.001%
5	4.352	1013	1030	1055	rBV	91427	229537	42.23%	4.824%
6	4.828	1157	1178	1203	rBV	227697	543532	100.00%	11.423%
7	5.050	1227	1247	1279	rBV2	216552	531987	97.88%	11.180%
8	5.619	1410	1424	1446	rBV	177778	362659	66.72%	7.622%
9	5.908	1506	1514	1527	rVB4	3918	7692	1.42%	0.162%
10	6.069	1551	1564	1588	rBV	121089	244746	45.03%	5.144%
11	6.989	1839	1850	1869	rBV	53856	101683	18.71%	2.137%
12	7.317	1940	1952	1971	rBV	267255	462549	85.10%	9.721%
13	7.394	1974	1976	1995	rVB4	3603	7093	1.30%	0.149%
14	7.625	2039	2048	2072	rBV2	30539	55131	10.14%	1.159%
15	8.088	2182	2192	2230	rBV	188531	368117	67.73%	7.736%
16	8.850	2419	2429	2454	rBV	260925	433790	79.81%	9.117%
17	10.217	2841	2854	2866	rBV	71130	111477	20.51%	2.343%
18	10.381	2897	2905	2914	rVB3	5083	8052	1.48%	0.169%
19	11.246	3164	3174	3199	rBV	259598	398375	73.29%	8.372%
20	11.532	3255	3263	3279	rBV3	7568	14631	2.69%	0.307%
21	11.622	3279	3291	3313	rVB	228239	355052	65.32%	7.462%




Sum of corrected areas: 4758199

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025014.D
Acq On : 15 Mar 2022 22:03
Operator : SY/MD
Sample : N1933-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

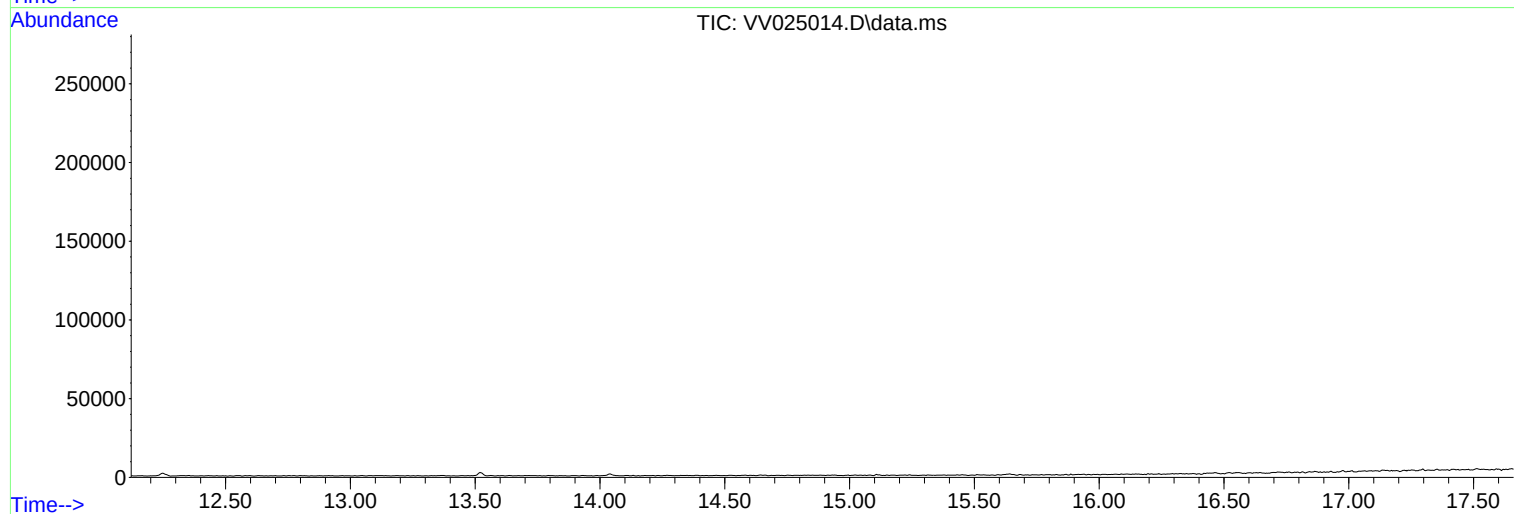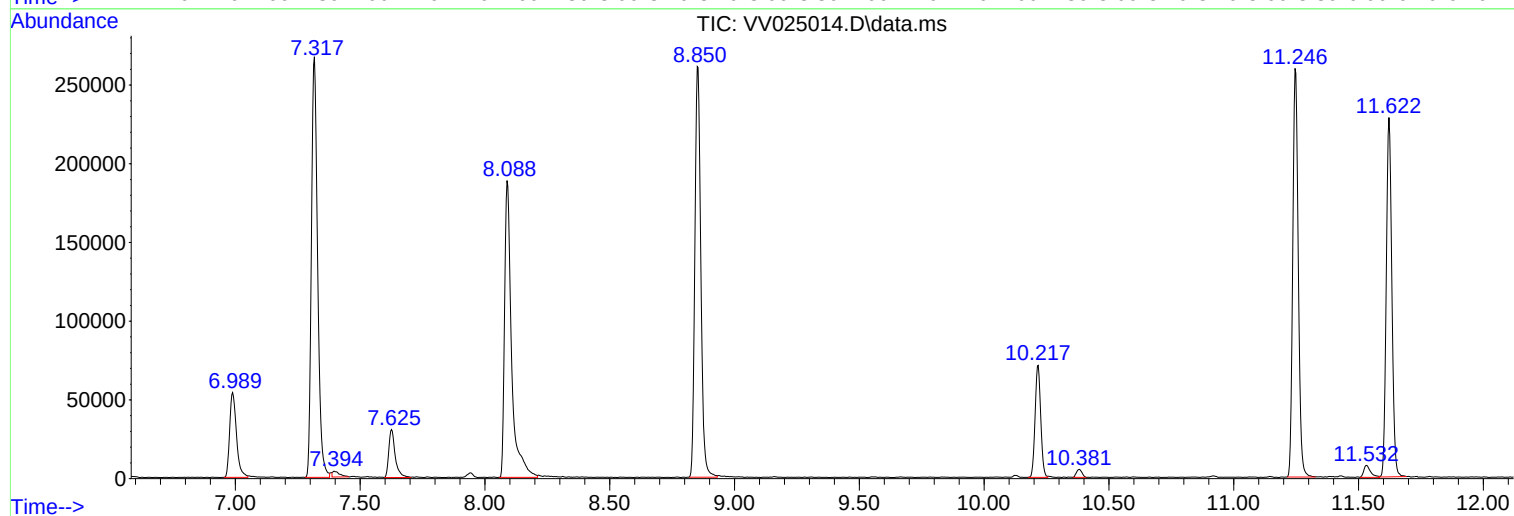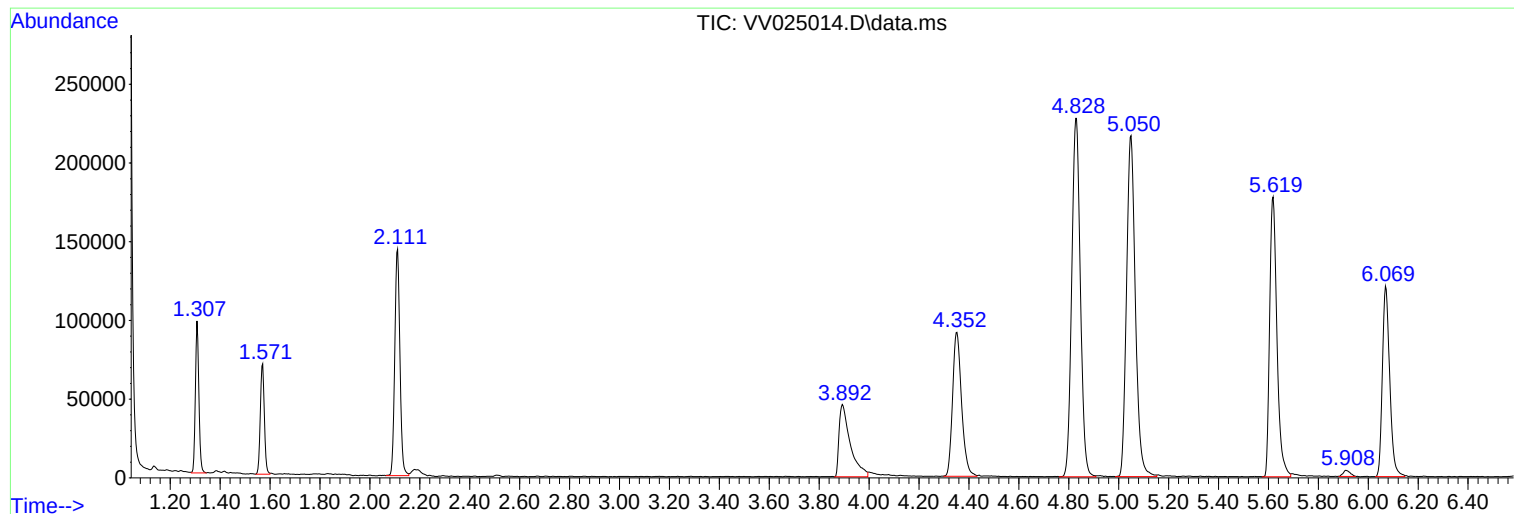

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025014.D
Acq On : 15 Mar 2022 22:03
Operator : SY/MD
Sample : N1933-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025014.D
Acq On : 15 Mar 2022 22:03
Operator : SY/MD
Sample : N1933-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------