

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025019.D
 Acq On : 16 Mar 2022 00:00
 Operator : SY/MD
 Sample : VV0315WBL02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK315

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	97613	96574	17.99%	2.308%
2	1.568	157	164	178	rVB	70134	78458	14.62%	1.875%
3	2.108	322	332	351	rBV	139694	204485	38.09%	4.887%
4	2.510	445	457	471	rVB3	6507	10670	1.99%	0.255%
5	3.895	878	888	929	rBV	45141	143332	26.70%	3.426%
6	4.349	1014	1029	1055	rBV	91004	231125	43.06%	5.524%
7	5.050	1231	1247	1277	rBV3	218742	536792	100.00%	12.829%
8	5.619	1412	1424	1456	rBV	167850	342028	63.72%	8.174%
9	5.911	1504	1515	1530	rBV7	4944	10114	1.88%	0.242%
10	6.069	1552	1564	1587	rBV	120532	245579	45.75%	5.869%
11	6.989	1840	1850	1873	rBV	54805	101589	18.93%	2.428%
12	7.316	1941	1952	1972	rBV	267935	470885	87.72%	11.254%
13	7.625	2039	2048	2074	rBV	30635	55519	10.34%	1.327%
14	8.088	2182	2192	2236	rBV	193771	373795	69.63%	8.933%
15	8.853	2417	2430	2461	rBV	251927	413086	76.95%	9.872%
16	10.217	2843	2854	2870	rBV2	70800	111779	20.82%	2.671%
17	11.249	3164	3175	3196	rBV	239204	372271	69.35%	8.897%
18	11.622	3280	3291	3319	rBV	228470	357573	66.61%	8.546%
19	12.647	3602	3610	3625	rVB4	3564	5439	1.01%	0.130%
20	13.265	3794	3802	3812	rBV3	4295	6410	1.19%	0.153%
21	13.509	3869	3878	3887	rBV2	5994	9489	1.77%	0.227%
22	13.744	3944	3951	3961	rBV5	4613	7231	1.35%	0.173%




Sum of corrected areas: 4184223

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025019.D
Acq On : 16 Mar 2022 00:00
Operator : SY/MD
Sample : VV0315WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

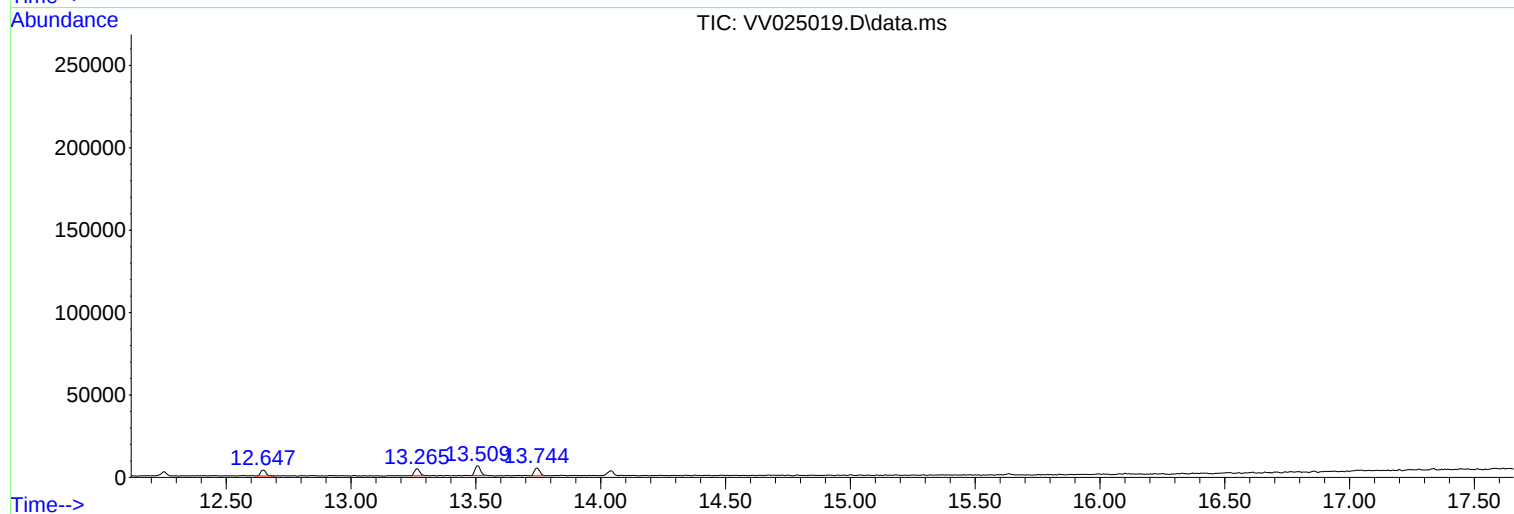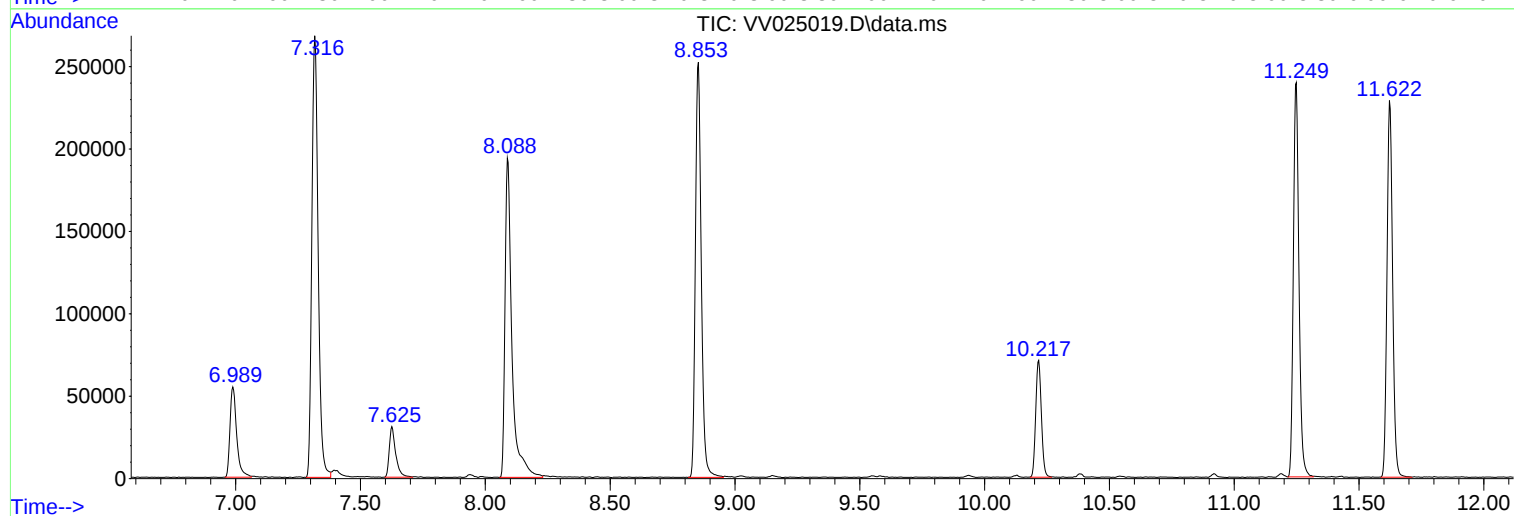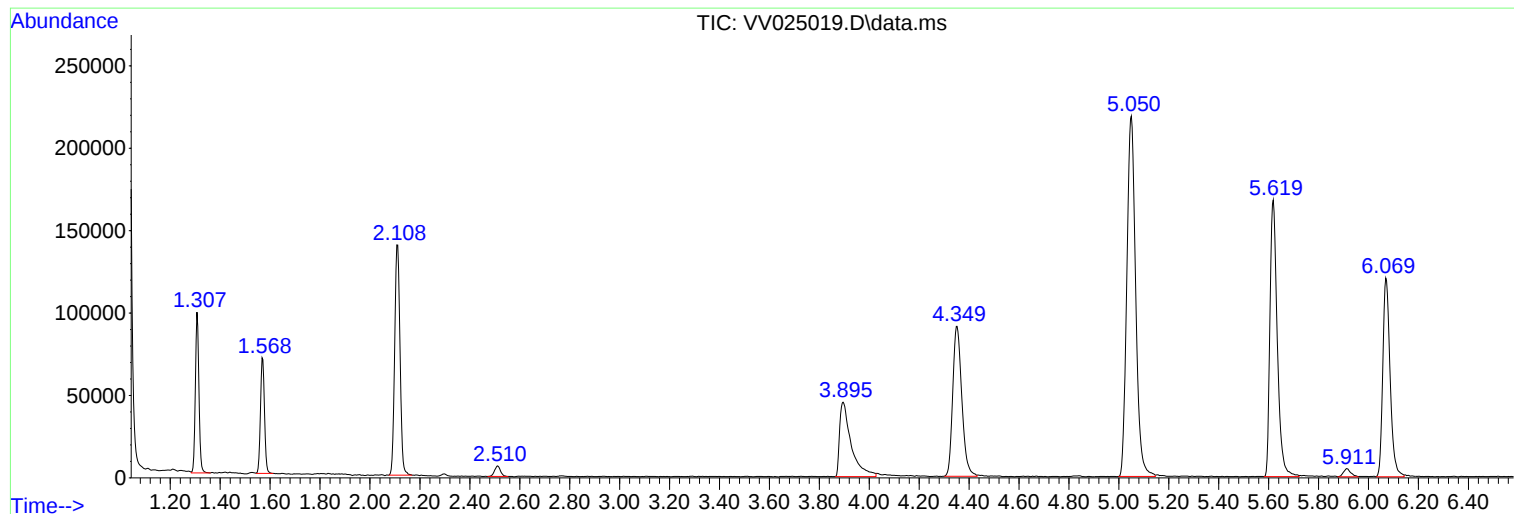

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025019.D
Acq On : 16 Mar 2022 00:00
Operator : SY/MD
Sample : VV0315WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025019.D
Acq On : 16 Mar 2022 00:00
Operator : SY/MD
Sample : VV0315WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
