

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025020.D
 Acq On : 16 Mar 2022 00:47
 Operator : SY/MD
 Sample : N1933-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDC3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025020.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	98376	96272	14.73%	1.879%
2	1.571	156	165	179	rBV	72948	83504	12.77%	1.629%
3	2.108	322	332	347	rBV	145579	212450	32.50%	4.146%
4	3.899	880	889	929	rBV2	44357	169488	25.93%	3.307%
5	4.352	1012	1030	1057	rBV2	96954	248401	38.00%	4.847%
6	4.828	1161	1178	1205	rBV	275838	653736	100.00%	12.757%
7	5.050	1230	1247	1274	rBV2	227066	559415	85.57%	10.916%
8	5.619	1411	1424	1453	rBV	178400	360781	55.19%	7.040%
9	5.918	1505	1517	1527	rBV8	4977	10777	1.65%	0.210%
10	6.069	1551	1564	1595	rBV	126775	260276	39.81%	5.079%
11	6.989	1834	1850	1872	rBV	58916	111002	16.98%	2.166%
12	7.317	1941	1952	1973	rBV	279452	484999	74.19%	9.464%
13	7.625	2039	2048	2062	rBV2	34314	58645	8.97%	1.144%
14	8.088	2183	2192	2228	rBV	224575	439601	67.24%	8.578%
15	8.854	2419	2430	2454	rBV	265726	436565	66.78%	8.519%
16	10.217	2840	2854	2875	rBV	80217	128903	19.72%	2.515%
17	10.384	2894	2906	2916	rBV3	4175	6745	1.03%	0.132%
18	11.249	3163	3175	3191	rBV	256786	399340	61.09%	7.793%
19	11.532	3254	3263	3279	rBV2	9535	18473	2.83%	0.360%
20	11.622	3279	3291	3318	rVB	247643	385245	58.93%	7.518%




Sum of corrected areas: 5124618

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025020.D
Acq On : 16 Mar 2022 00:47
Operator : SY/MD
Sample : N1933-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

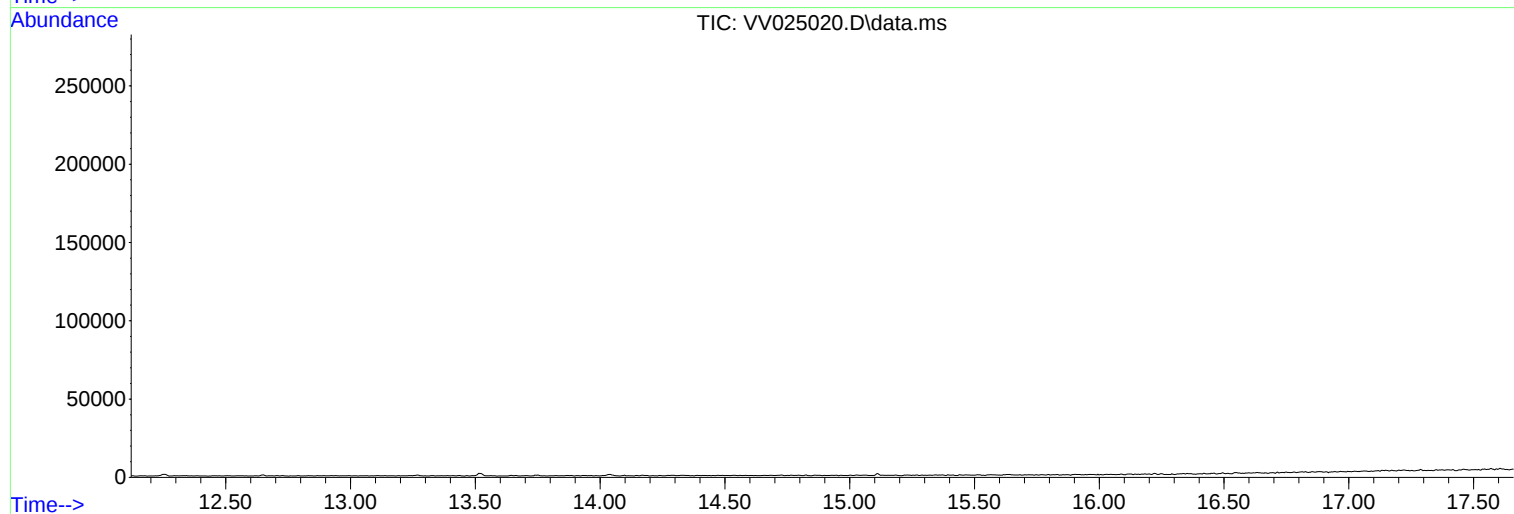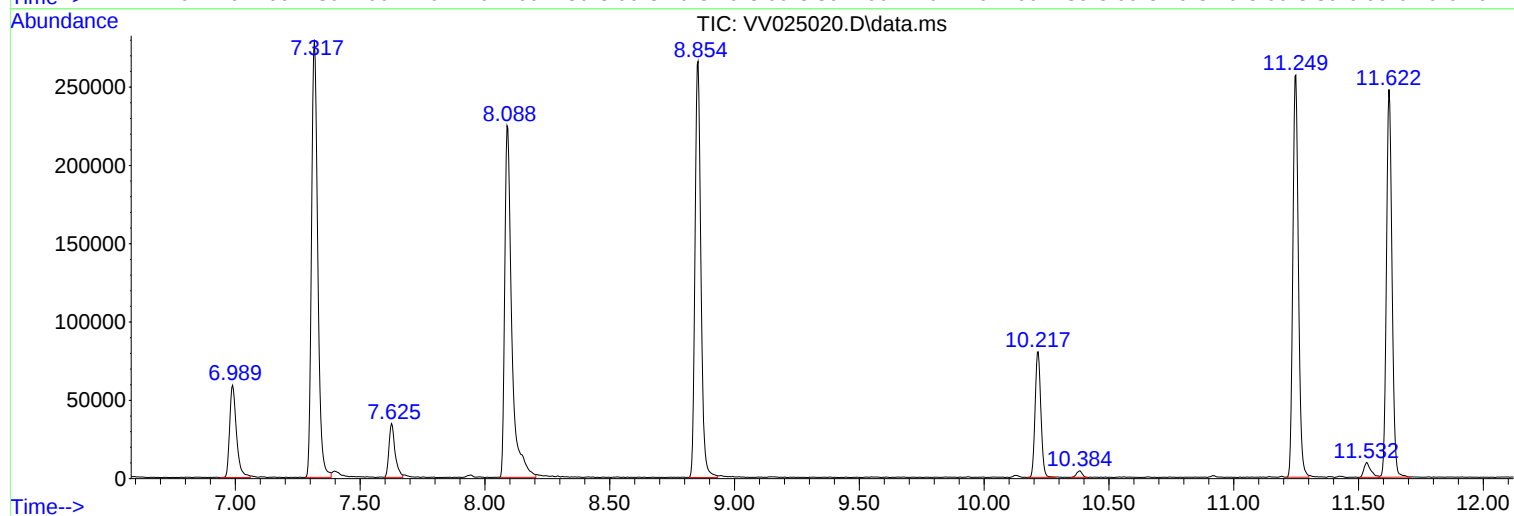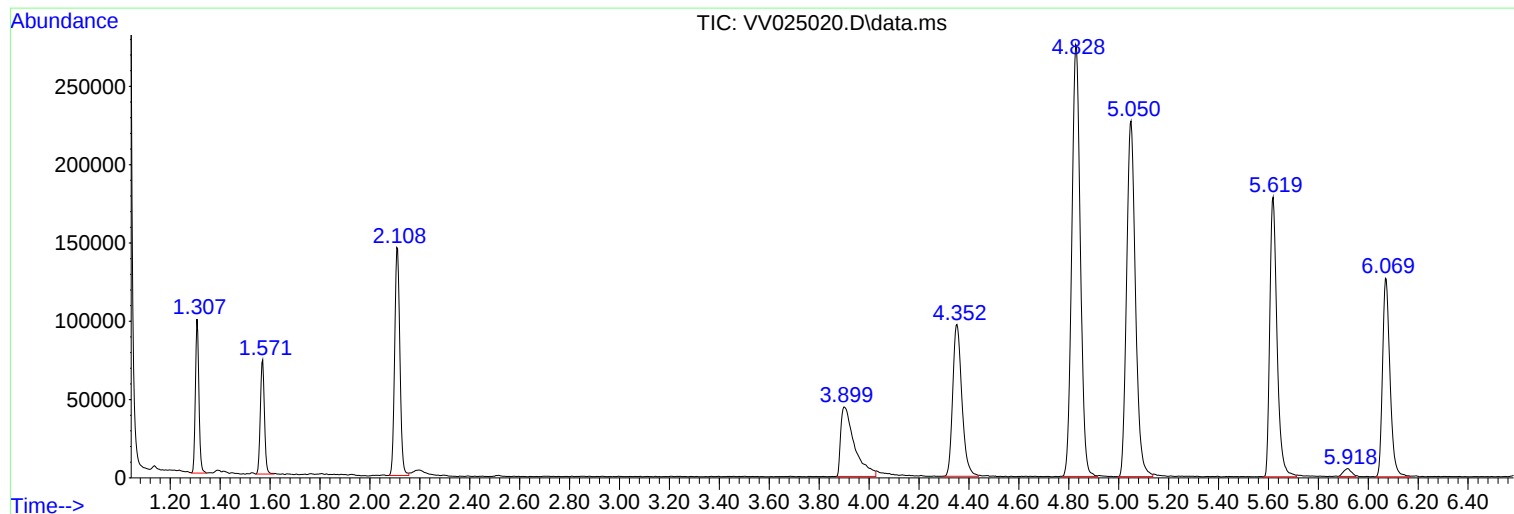

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025020.D
Acq On : 16 Mar 2022 00:47
Operator : SY/MD
Sample : N1933-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025020.D
Acq On : 16 Mar 2022 00:47
Operator : SY/MD
Sample : N1933-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc