

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025021.D
 Acq On : 16 Mar 2022 01:11
 Operator : SY/MD
 Sample : N1933-13
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDC4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025021.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	92216	92688	17.11%	2.130%
2	1.571	156	165	180	rVB	69647	79421	14.66%	1.825%
3	2.108	322	332	344	rBV	139443	201908	37.28%	4.641%
4	2.188	350	357	381	rVB2	4080	11947	2.21%	0.275%
5	3.902	880	890	945	rBV2	43627	170710	31.52%	3.924%
6	4.352	1013	1030	1053	rBV2	93024	229447	42.36%	5.273%
7	5.050	1231	1247	1282	rBV3	217738	541621	100.00%	12.448%
8	5.619	1411	1424	1447	rBV	173997	350355	64.69%	8.052%
9	5.915	1506	1516	1530	rVB6	4268	8889	1.64%	0.204%
10	6.072	1551	1565	1594	rBV	121742	248996	45.97%	5.723%
11	6.989	1840	1850	1880	rBV	55353	103595	19.13%	2.381%
12	7.317	1939	1952	1973	rBV	269359	468066	86.42%	10.758%
13	7.625	2039	2048	2068	rBV	31199	56488	10.43%	1.298%
14	7.940	2135	2146	2158	rVB3	4536	8245	1.52%	0.189%
15	8.088	2182	2192	2232	rBV	217431	430294	79.45%	9.890%
16	8.854	2418	2430	2462	rBV	262181	431350	79.64%	9.914%
17	10.217	2842	2854	2874	rVB	77243	123963	22.89%	2.849%
18	10.381	2895	2905	2916	rVB2	8622	13706	2.53%	0.315%
19	11.249	3164	3175	3193	rBV	253604	390484	72.10%	8.975%
20	11.532	3254	3263	3280	rBV2	9785	19894	3.67%	0.457%
21	11.622	3280	3291	3310	rVB	238003	368885	68.11%	8.478%




Sum of corrected areas: 4350952

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025021.D
Acq On : 16 Mar 2022 01:11
Operator : SY/MD
Sample : N1933-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

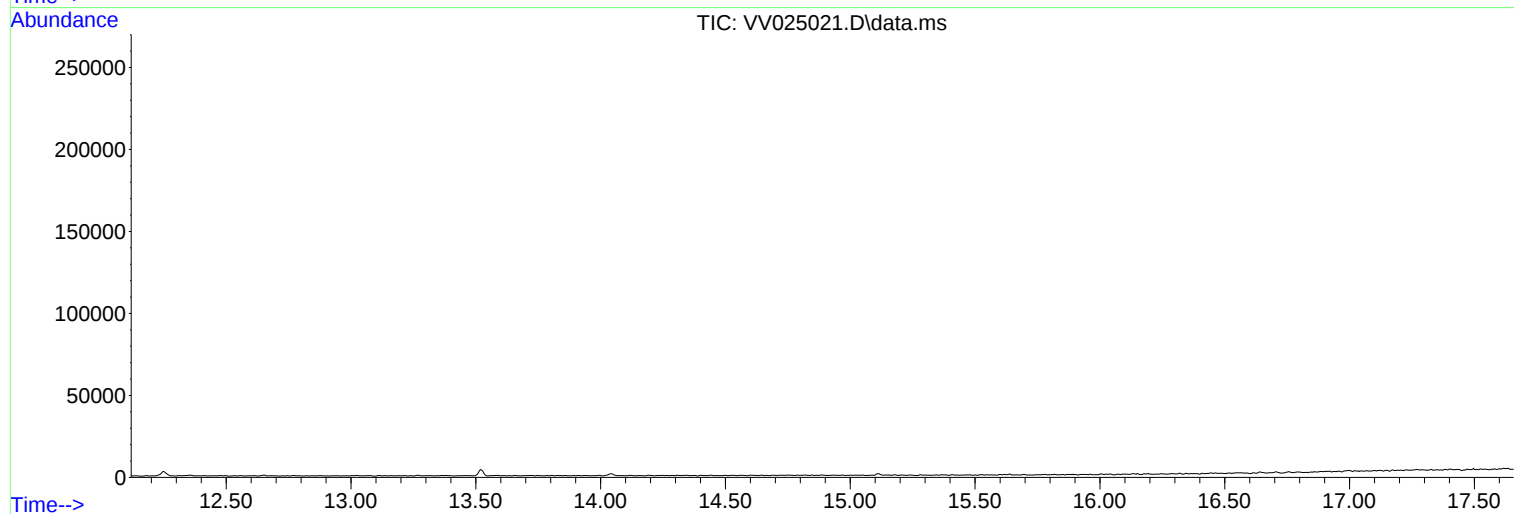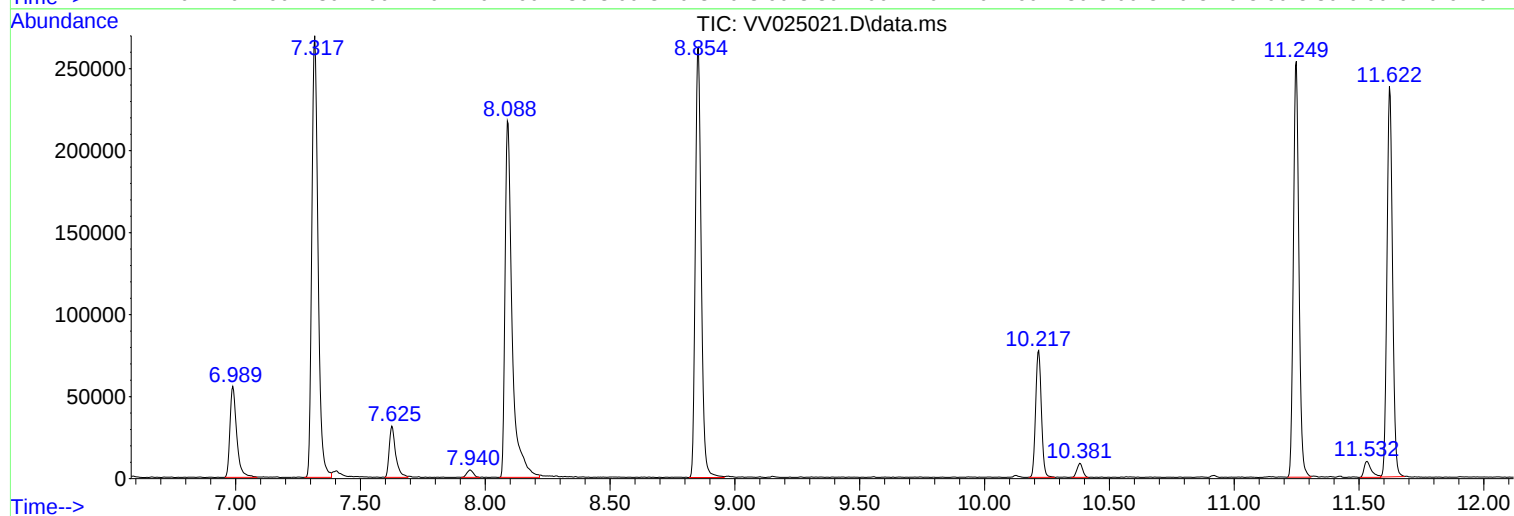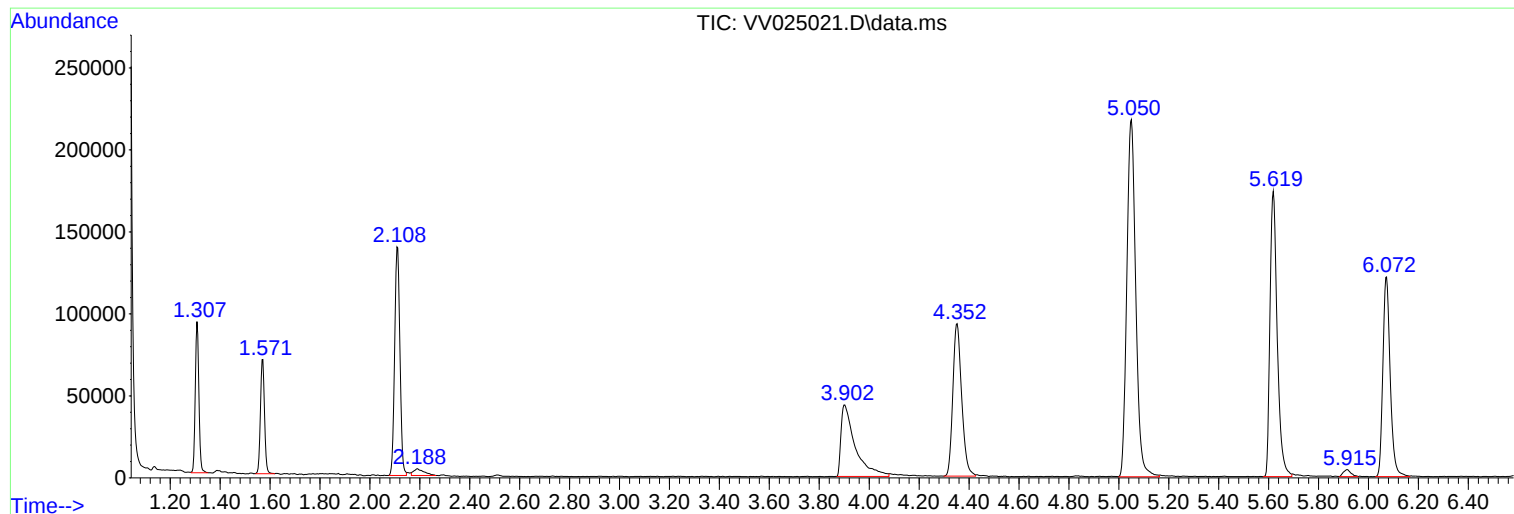

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025021.D
Acq On : 16 Mar 2022 01:11
Operator : SY/MD
Sample : N1933-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025021.D
Acq On : 16 Mar 2022 01:11
Operator : SY/MD
Sample : N1933-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc