

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
 Data File : VV025023.D
 Acq On : 16 Mar 2022 01:58
 Operator : SY/MD
 Sample : N1933-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDC6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.108	321	332	345	rBV	142071	205754	1.12%	0.884%
2	4.339	1008	1026	1072	rBV2	492892	1452997	7.91%	6.244%
3	4.831	1157	1179	1212	rBV	7741575	18368007	100.00%	78.929%
4	5.050	1230	1247	1276	rVB2	221269	541968	2.95%	2.329%
5	5.619	1413	1424	1456	rBV	174997	356775	1.94%	1.533%
6	6.069	1551	1564	1588	rBV2	121480	248508	1.35%	1.068%
7	7.317	1941	1952	1972	rBV	268519	463358	2.52%	1.991%
8	8.088	2182	2192	2234	rBV	226176	425043	2.31%	1.826%
9	8.850	2417	2429	2461	rBV	265371	436924	2.38%	1.877%
10	11.249	3164	3175	3198	rBV	259467	401689	2.19%	1.726%
11	11.622	3280	3291	3314	rVB	237728	370567	2.02%	1.592%




Sum of corrected areas: 23271590

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025023.D
Acq On : 16 Mar 2022 01:58
Operator : SY/MD
Sample : N1933-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

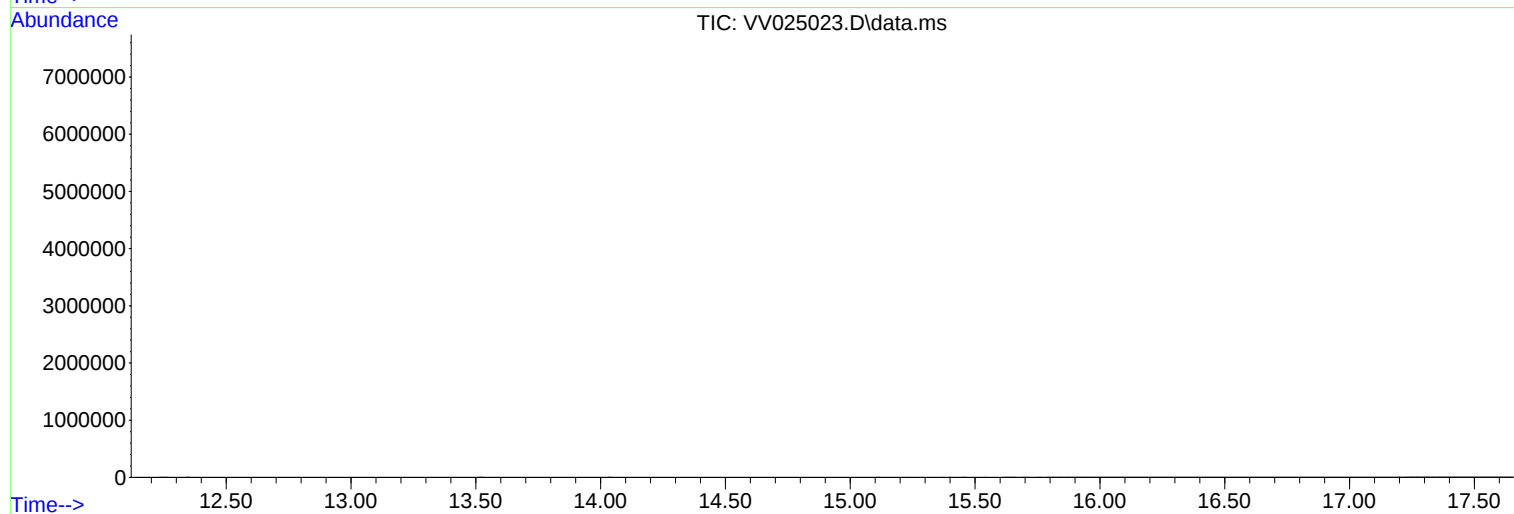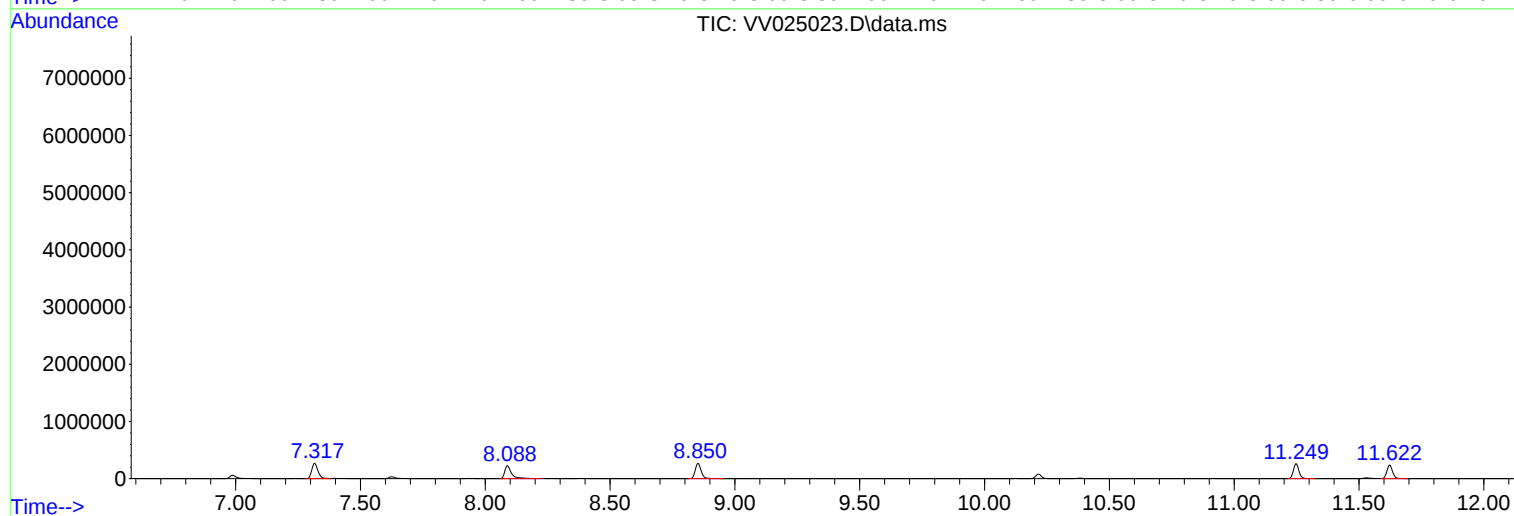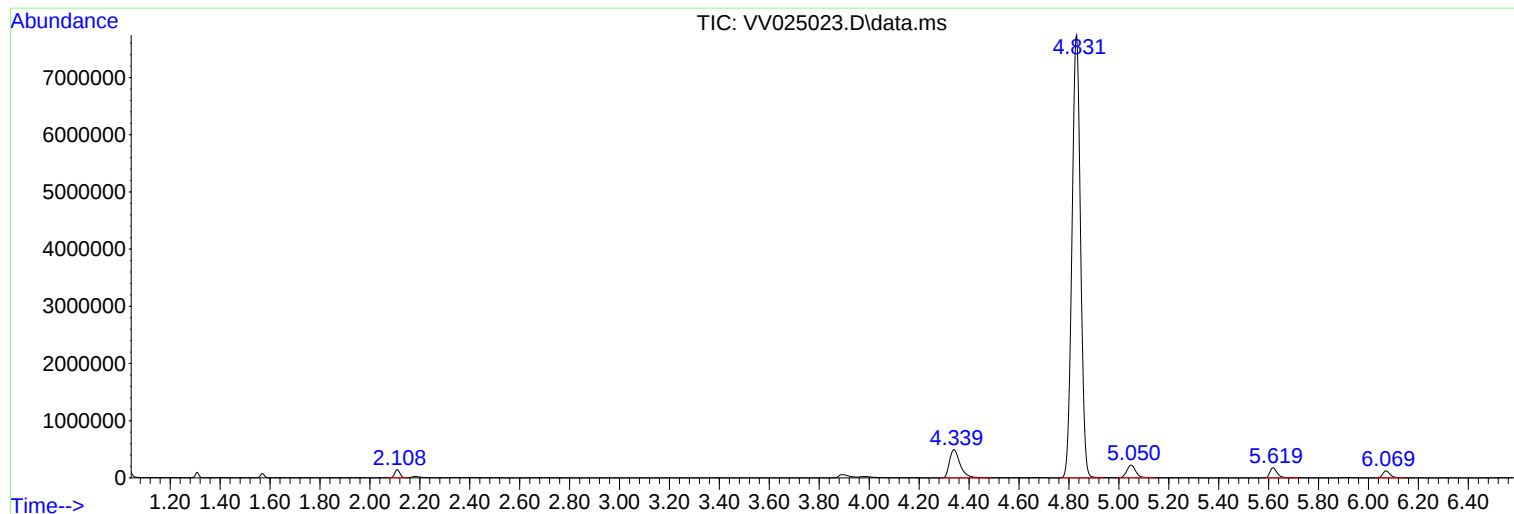

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025023.D
Acq On : 16 Mar 2022 01:58
Operator : SY/MD
Sample : N1933-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031522\
Data File : VV025023.D
Acq On : 16 Mar 2022 01:58
Operator : SY/MD
Sample : N1933-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR031522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc